

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032887.D
 Acq On : 10 Nov 2023 13:21
 Operator : SY/MD
 Sample : 05326-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.195	44	48	53	rBV2	6998	6285	0.41%	0.056%
2	1.281	69	75	88	rVB	217752	217448	14.14%	1.938%
3	1.532	147	153	166	rVB	182989	212770	13.83%	1.896%
4	2.063	309	318	330	rBV	354861	514454	33.45%	4.585%
5	2.426	429	431	433	rBV3	2003	1126	0.07%	0.010%
6	2.799	543	547	549	rBV4	1579	1072	0.07%	0.010%
7	2.973	596	601	607	rBV9	2378	2356	0.15%	0.021%
8	3.043	621	623	629	rVV6	1745	1366	0.09%	0.012%
9	3.088	635	637	640	rBV3	1236	666	0.04%	0.006%
10	3.108	640	643	646	rVB5	1072	648	0.04%	0.006%
11	3.233	676	682	683	rBV6	1348	1213	0.08%	0.011%
12	3.326	709	711	715	rVB4	1020	722	0.05%	0.006%
13	3.394	729	732	734	rVB4	1276	687	0.04%	0.006%
14	3.523	770	772	777	rVB6	1509	1183	0.08%	0.011%
15	3.548	777	780	787	rBV9	1767	1968	0.13%	0.018%
16	3.587	789	792	795	rBV5	1698	1132	0.07%	0.010%
17	3.622	799	803	805	rVV5	1478	1171	0.08%	0.010%
18	3.651	809	812	816	rBV5	1119	977	0.06%	0.009%
19	3.696	823	826	829	rBV5	1065	828	0.05%	0.007%
20	3.786	846	854	880	rBV	79384	214752	13.96%	1.914%
21	4.117	954	957	959	rBV4	2188	1597	0.10%	0.014%
22	4.159	968	970	973	rBV4	1227	712	0.05%	0.006%
23	4.252	980	999	1019	rBV	233931	615067	39.99%	5.481%
24	4.477	1066	1069	1075	rVB8	2018	1778	0.12%	0.016%
25	4.735	1146	1149	1152	rBV5	1353	1214	0.08%	0.011%
26	4.960	1202	1219	1264	rBV2	531686	1538074	100.00%	13.707%
27	5.339	1335	1337	1343	rBV7	1409	1606	0.10%	0.014%
28	5.535	1386	1398	1434	rBV	378754	857045	55.72%	7.638%
29	5.992	1528	1540	1574	rVB	306677	681780	44.33%	6.076%
30	6.551	1711	1714	1718	rBV6	1750	1229	0.08%	0.011%
31	6.825	1796	1799	1800	rBV3	1997	856	0.06%	0.008%
32	6.854	1804	1808	1810	rVB5	2186	1634	0.11%	0.015%
33	6.873	1810	1814	1815	rBV4	1398	1058	0.07%	0.009%
34	6.915	1817	1827	1852	rVV	154828	313536	20.38%	2.794%
35	7.246	1918	1930	1954	rBV	624914	1167898	75.93%	10.408%
36	7.555	2018	2026	2045	rBV2	117250	213773	13.90%	1.905%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111023\
 Data File : VW032887.D
 Acq On : 10 Nov 2023 13:21
 Operator : SY/MD
 Sample : 05326-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	7.911	2130	2137	2155	rVB3	20463	39325	2.56%	0.350%
38	8.027	2164	2173	2202	rBV	289022	601679	39.12%	5.362%
39	8.532	2328	2330	2333	rBV4	1244	803	0.05%	0.007%
40	8.606	2351	2353	2359	rVB6	1693	818	0.05%	0.007%
41	8.786	2397	2409	2431	rBV	656558	1107586	72.01%	9.870%
42	9.532	2638	2641	2643	rBV3	1775	775	0.05%	0.007%
43	9.545	2643	2645	2647	rBV2	1814	955	0.06%	0.009%
44	9.590	2656	2659	2660	rBV3	1436	745	0.05%	0.007%
45	9.657	2678	2680	2683	rVB4	1396	673	0.04%	0.006%
46	9.712	2693	2697	2700	rVB6	1484	1030	0.07%	0.009%
47	9.754	2705	2710	2711	rBV4	1759	1426	0.09%	0.013%
48	9.825	2730	2732	2736	rVB5	1727	1041	0.07%	0.009%
49	9.908	2755	2758	2764	rBV8	1855	2166	0.14%	0.019%
50	10.107	2818	2820	2822	rBV2	1264	651	0.04%	0.006%
51	10.156	2824	2835	2858	rVB	465441	737452	47.95%	6.572%
52	10.394	2902	2909	2910	rBV6	1284	1406	0.09%	0.013%
53	10.484	2932	2937	2939	rBV5	1886	1478	0.10%	0.013%
54	10.606	2973	2975	2976	rBV	1344	632	0.04%	0.006%
55	10.677	2995	2997	3000	rBV4	1425	822	0.05%	0.007%
56	10.715	3007	3009	3011	rBV3	1434	698	0.05%	0.006%
57	10.731	3012	3014	3019	rVV5	1666	1222	0.08%	0.011%
58	10.763	3022	3024	3027	rVB4	1513	672	0.04%	0.006%
59	10.821	3039	3042	3044	rBV3	1351	793	0.05%	0.007%
60	10.837	3044	3047	3049	rBV4	1358	813	0.05%	0.007%
61	10.924	3070	3074	3075	rBV4	1267	925	0.06%	0.008%
62	11.027	3102	3106	3109	rVB5	2207	1524	0.10%	0.014%
63	11.050	3109	3113	3117	rVB7	1177	1103	0.07%	0.010%
64	11.072	3117	3120	3123	rBV4	1892	1184	0.08%	0.011%
65	11.188	3145	3156	3177	rBV	639785	991993	64.50%	8.840%
66	11.355	3204	3208	3213	rBV8	1900	1665	0.11%	0.015%
67	11.509	3247	3256	3259	rVV8	5635	9129	0.59%	0.081%
68	11.561	3262	3272	3295	rVB	697850	1089472	70.83%	9.709%
69	11.783	3339	3341	3342	rBV2	2267	984	0.06%	0.009%
70	11.947	3387	3392	3396	rBV7	2111	2128	0.14%	0.019%
71	11.979	3396	3402	3404	rBV7	1933	1836	0.12%	0.016%
72	12.037	3417	3420	3427	rVB7	1708	1802	0.12%	0.016%
73	12.265	3489	3491	3494	rBV4	1228	1033	0.07%	0.009%
74	12.323	3507	3509	3513	rBV5	1859	1038	0.07%	0.009%
75	12.397	3528	3532	3533	rBV4	1742	954	0.06%	0.009%
76	12.535	3573	3575	3578	rVV3	1279	714	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032887.D
 Acq On : 10 Nov 2023 13:21
 Operator : SY/MD
 Sample : 05326-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.580	3586	3589	3590	rBV3	1494	1041	0.07%	0.009%
78	12.686	3620	3622	3625	rBV4	1333	744	0.05%	0.007%
79	12.705	3625	3628	3629	rBV3	1650	957	0.06%	0.009%
80	12.757	3641	3644	3645	rBV3	2261	1280	0.08%	0.011%
81	12.940	3697	3701	3702	rBV3	1448	747	0.05%	0.007%
82	13.046	3732	3734	3738	rBV5	1105	956	0.06%	0.009%
83	13.384	3836	3839	3842	rBV6	1121	653	0.04%	0.006%
84	13.426	3850	3852	3855	rBV4	2139	1121	0.07%	0.010%
85	13.448	3855	3859	3866	rVV10	2457	3330	0.22%	0.030%
86	13.554	3888	3892	3895	rBV4	1357	1128	0.07%	0.010%
87	13.593	3902	3904	3906	rBV3	1845	860	0.06%	0.008%
88	13.689	3930	3934	3938	rVB6	2009	1561	0.10%	0.014%
89	13.783	3961	3963	3966	rVB4	1738	974	0.06%	0.009%
90	13.808	3966	3971	3975	rBV8	2194	2085	0.14%	0.019%
91	13.995	4026	4029	4030	rBV3	1655	781	0.05%	0.007%
92	14.004	4030	4032	4037	rVB6	1201	882	0.06%	0.008%
93	14.056	4046	4048	4050	rBV3	1465	870	0.06%	0.008%
94	14.088	4056	4058	4062	rBV5	1601	1186	0.08%	0.011%
95	14.255	4107	4110	4112	rBV3	1204	742	0.05%	0.007%
96	14.638	4226	4229	4232	rBV5	1284	844	0.05%	0.008%
97	14.754	4263	4265	4267	rVV3	1943	832	0.05%	0.007%
98	14.792	4275	4277	4279	rBV3	1870	1138	0.07%	0.010%
99	14.863	4297	4299	4301	rBV3	1609	870	0.06%	0.008%
100	15.236	4413	4415	4418	rBV3	1600	929	0.06%	0.008%




Sum of corrected areas: 11221337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032887.D
Acq On : 10 Nov 2023 13:21
Operator : SY/MD
Sample : 05326-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

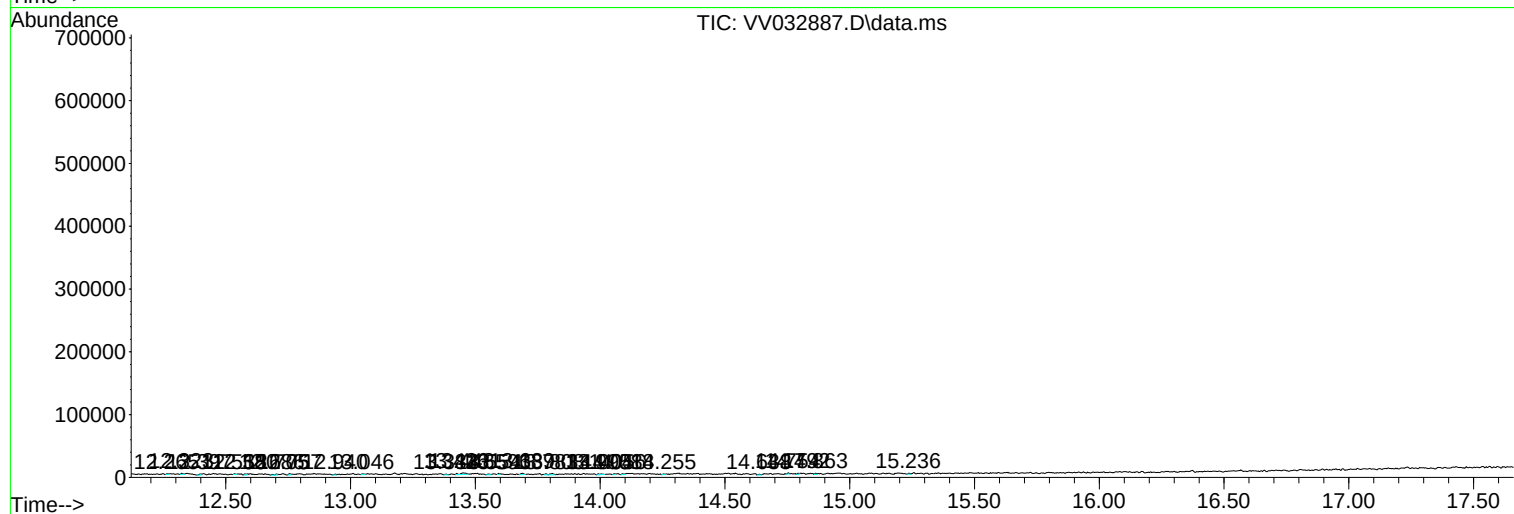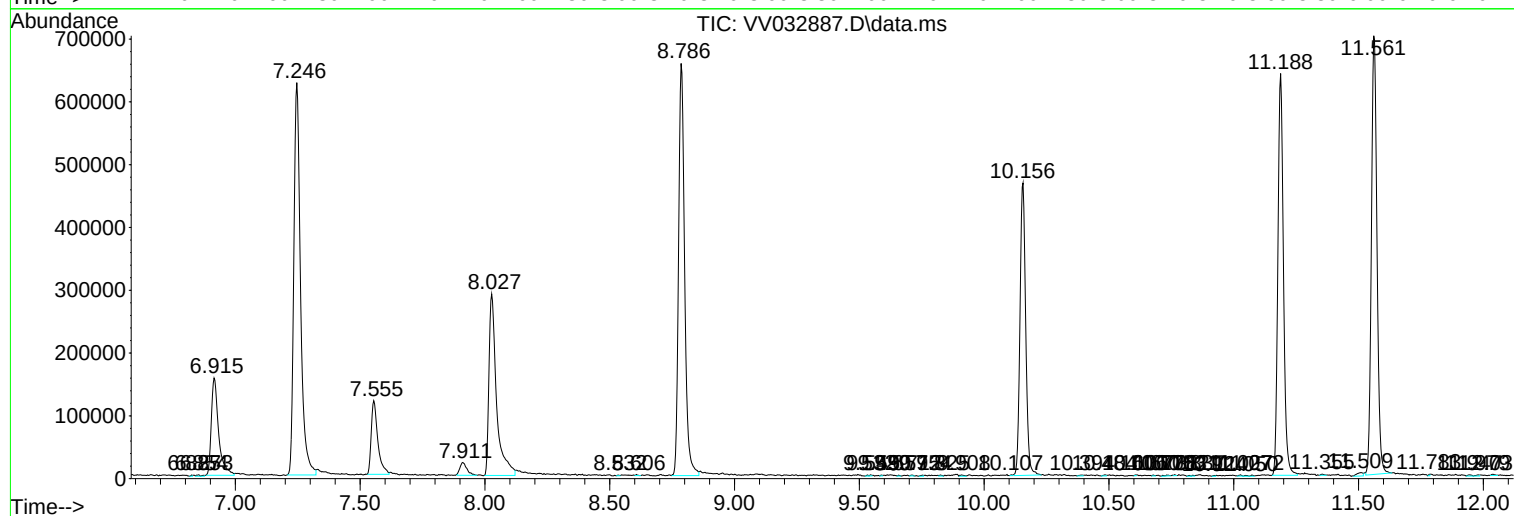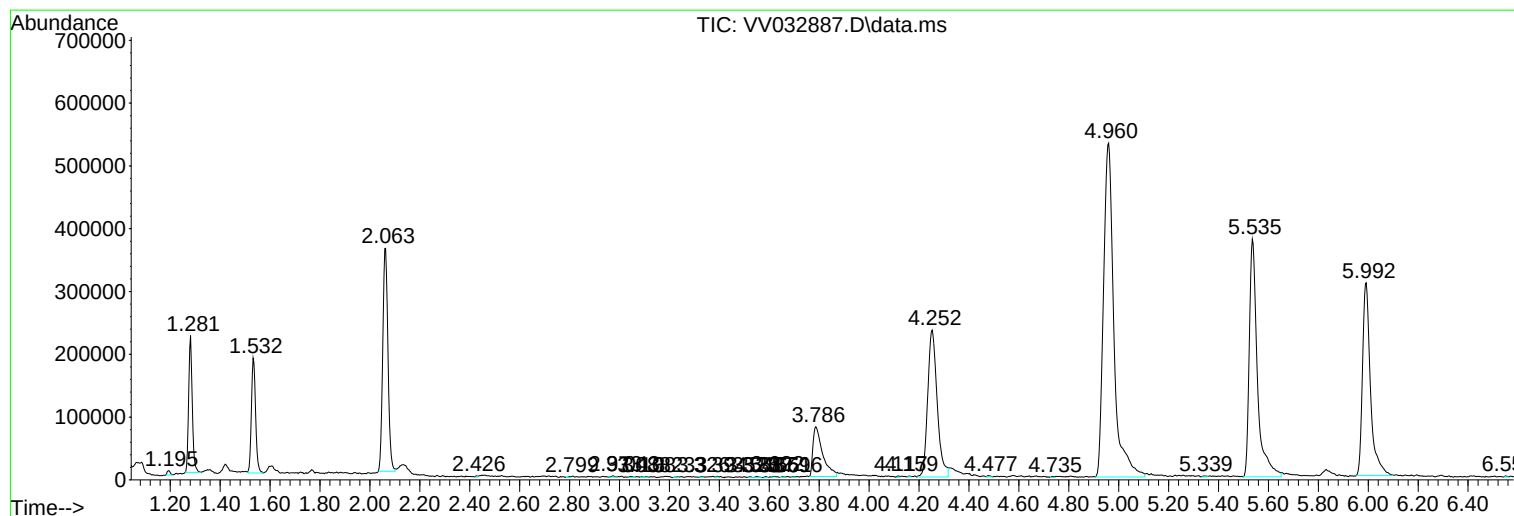

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032887.D
Acq On : 10 Nov 2023 13:21
Operator : SY/MD
Sample : 05326-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032887.D
Acq On : 10 Nov 2023 13:21
Operator : SY/MD
Sample : 05326-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------