

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032888.D
 Acq On : 10 Nov 2023 13:44
 Operator : SY/MD
 Sample : VIBLK241
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	85	rBV	188904	190973	13.42%	1.801%
2	1.535	147	154	165	rVB	180824	207089	14.55%	1.953%
3	2.063	309	318	331	rBV	323135	464284	32.62%	4.378%
4	2.667	504	506	508	rBV2	1950	860	0.06%	0.008%
5	2.725	521	524	525	rBV3	1486	921	0.06%	0.009%
6	2.802	546	548	551	rBV3	1404	753	0.05%	0.007%
7	2.870	565	569	570	rBV4	1827	941	0.07%	0.009%
8	2.902	576	579	580	rBV3	1538	1029	0.07%	0.010%
9	2.998	607	609	613	rVB4	1726	933	0.07%	0.009%
10	3.018	613	615	620	rBV5	1552	1110	0.08%	0.010%
11	3.104	639	642	644	rBV4	1962	1323	0.09%	0.012%
12	3.172	661	663	664	rBV	1181	580	0.04%	0.005%
13	3.256	687	689	698	rVB8	2427	2431	0.17%	0.023%
14	3.294	698	701	704	rBV4	2042	1329	0.09%	0.013%
15	3.310	704	706	708	rBV3	692	275	0.02%	0.003%
16	3.320	708	709	712	rVB4	1100	427	0.03%	0.004%
17	3.336	712	714	718	rBV5	1742	1532	0.11%	0.014%
18	3.410	734	737	739	rBV4	1584	1063	0.07%	0.010%
19	3.423	739	741	744	rVV4	954	774	0.05%	0.007%
20	3.474	753	757	759	rBV4	1955	1396	0.10%	0.013%
21	3.548	777	780	781	rBV3	1186	635	0.04%	0.006%
22	3.609	796	799	802	rBV5	1347	1275	0.09%	0.012%
23	3.648	810	811	815	rVB4	1149	422	0.03%	0.004%
24	3.677	815	820	822	rBV5	1428	1438	0.10%	0.014%
25	3.722	832	834	836	rBV3	1294	590	0.04%	0.006%
26	3.789	846	855	876	rBV2	86969	234135	16.45%	2.208%
27	4.252	985	999	1019	rBV	228588	589579	41.43%	5.559%
28	4.773	1158	1161	1164	rBV4	1720	1092	0.08%	0.010%
29	4.825	1175	1177	1178	rBV2	1057	296	0.02%	0.003%
30	4.870	1189	1191	1194	rBV4	1115	762	0.05%	0.007%
31	4.960	1203	1219	1236	rBV2	531860	1423209	100.00%	13.419%
32	5.349	1339	1340	1345	rBV4	1560	1288	0.09%	0.012%
33	5.535	1387	1398	1442	rBV	330084	760872	53.46%	7.174%
34	5.989	1528	1539	1572	rBV	310514	692882	48.68%	6.533%
35	6.432	1675	1677	1678	rBV2	1670	663	0.05%	0.006%
36	6.574	1719	1721	1722	rBV2	1265	425	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032888.D
 Acq On : 10 Nov 2023 13:44
 Operator : SY/MD
 Sample : VIBLK241
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.632	1737	1739	1742	rBV4	1858	1267	0.09%	0.012%
38	6.915	1817	1827	1854	rBV	158482	321498	22.59%	3.031%
39	7.246	1919	1930	1954	rBV	613852	1130074	79.40%	10.655%
40	7.554	2017	2026	2042	rBV	118297	218880	15.38%	2.064%
41	7.911	2129	2137	2147	rBV8	11337	21488	1.51%	0.203%
42	8.027	2164	2173	2208	rBV	305026	622527	43.74%	5.870%
43	8.468	2307	2310	2313	rBV3	1656	1396	0.10%	0.013%
44	8.677	2372	2375	2379	rBV4	2704	1965	0.14%	0.019%
45	8.734	2391	2393	2394	rBV2	1775	704	0.05%	0.007%
46	8.786	2399	2409	2432	rVV	577712	982340	69.02%	9.262%
47	9.181	2530	2532	2533	rBV2	1212	546	0.04%	0.005%
48	9.416	2602	2605	2606	rBV3	1854	1023	0.07%	0.010%
49	9.587	2656	2658	2659	rBV2	1082	470	0.03%	0.004%
50	9.660	2679	2681	2687	rVB6	1838	1368	0.10%	0.013%
51	9.699	2691	2693	2695	rBV3	1438	818	0.06%	0.008%
52	9.731	2700	2703	2708	rBV7	2820	2485	0.17%	0.023%
53	10.104	2816	2819	2822	rBV5	1864	1121	0.08%	0.011%
54	10.156	2824	2835	2848	rVV	470808	741334	52.09%	6.990%
55	10.422	2915	2918	2921	rBV5	1685	1412	0.10%	0.013%
56	10.458	2927	2929	2934	rBV5	1221	1064	0.07%	0.010%
57	10.609	2974	2976	2977	rBV2	1325	621	0.04%	0.006%
58	10.718	3007	3010	3011	rBV3	1692	858	0.06%	0.008%
59	10.786	3029	3031	3032	rBV2	1869	850	0.06%	0.008%
60	10.911	3069	3070	3074	rVB4	2843	1101	0.08%	0.010%
61	10.943	3074	3080	3084	rBV7	2393	2270	0.16%	0.021%
62	11.188	3145	3156	3177	rBV	556894	872356	61.30%	8.225%
63	11.564	3262	3273	3296	rVB	679980	1062462	74.65%	10.017%
64	12.075	3429	3432	3433	rBV3	1511	671	0.05%	0.006%
65	12.127	3444	3448	3451	rBV5	1678	1646	0.12%	0.016%
66	12.445	3544	3547	3548	rBV3	1467	903	0.06%	0.009%
67	12.651	3608	3611	3615	rBV5	1845	1602	0.11%	0.015%
68	12.766	3644	3647	3651	rVB4	1250	852	0.06%	0.008%
69	12.950	3702	3704	3705	rBV2	921	362	0.03%	0.003%
70	13.136	3760	3762	3765	rVB4	1890	864	0.06%	0.008%
71	13.287	3806	3809	3812	rBV4	1862	1232	0.09%	0.012%
72	13.348	3826	3828	3834	rVB7	1936	1650	0.12%	0.016%
73	13.377	3834	3837	3839	rBV4	1410	1028	0.07%	0.010%
74	13.599	3903	3906	3907	rBV3	2325	1095	0.08%	0.010%
75	13.853	3980	3985	3987	rBV6	2192	2104	0.15%	0.020%
76	14.213	4091	4097	4099	rBV7	2046	2358	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032888.D
Acq On : 10 Nov 2023 13:44
Operator : SY/MD
Sample : VIBLK241
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

77	14.477	4176	4179	4181	rBV4	1536	1169	0.08%	0.011%
78	14.712	4248	4252	4253	rBV4	2330	1549	0.11%	0.015%
79	14.811	4279	4283	4284	rBV4	2061	1240	0.09%	0.012%
80	14.866	4298	4300	4301	rBV2	1458	646	0.05%	0.006%
81	15.043	4353	4355	4360	rBV5	1681	1210	0.09%	0.011%




Sum of corrected areas: 10606065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032888.D
Acq On : 10 Nov 2023 13:44
Operator : SY/MD
Sample : VIBLK241
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

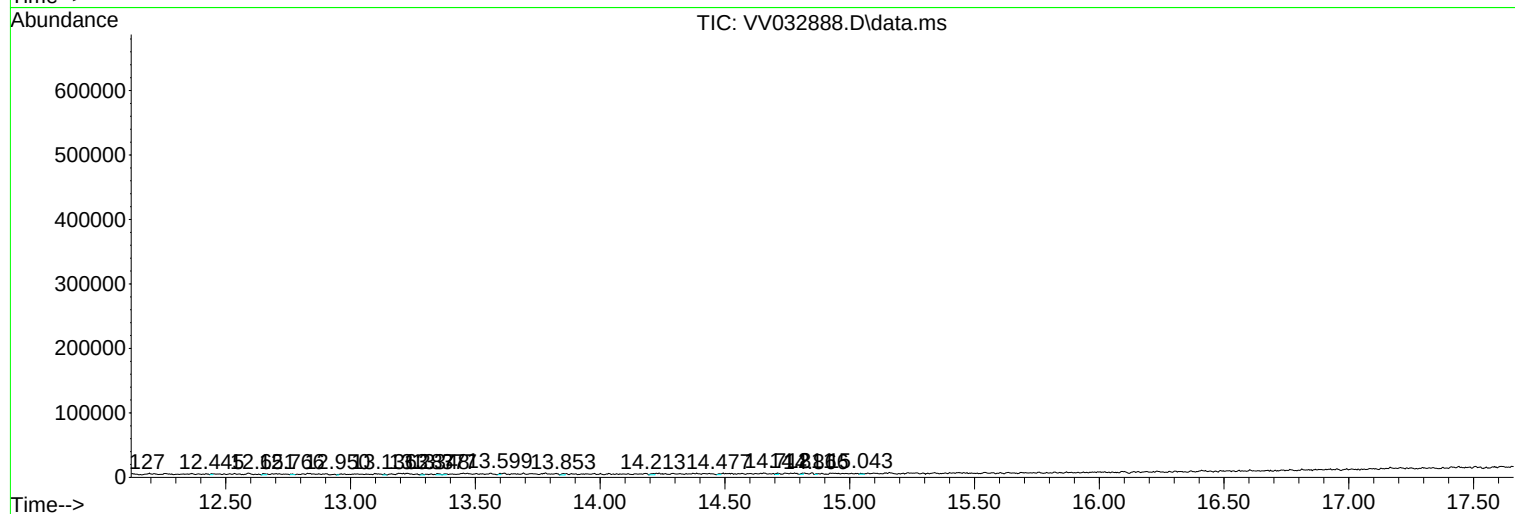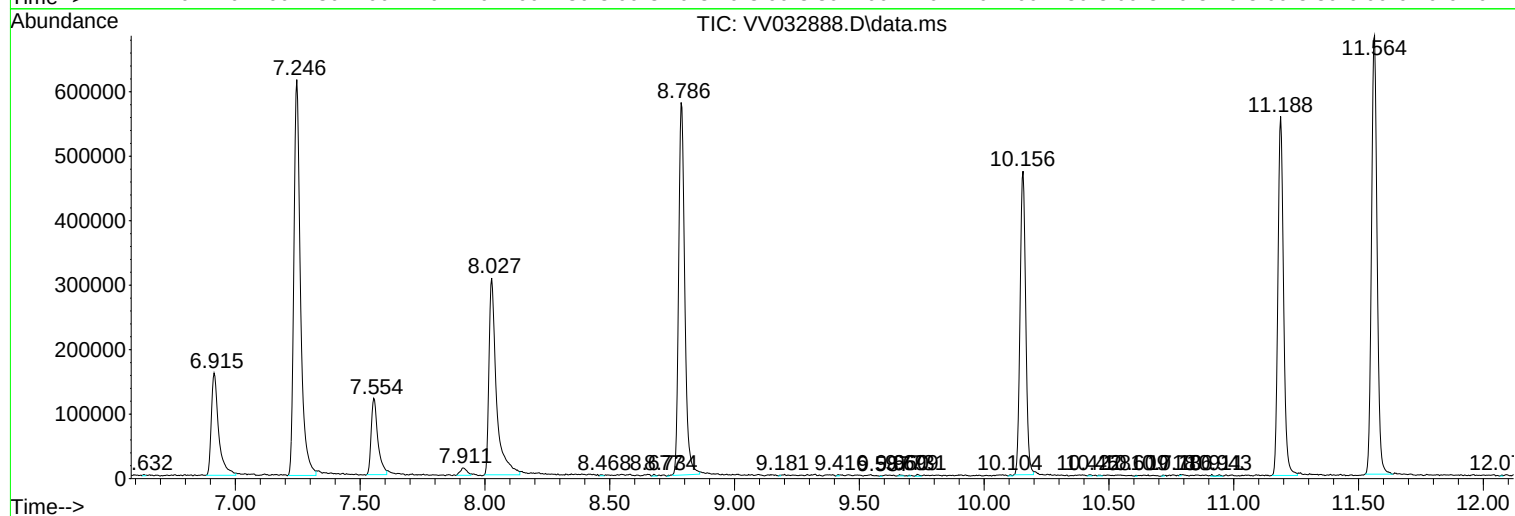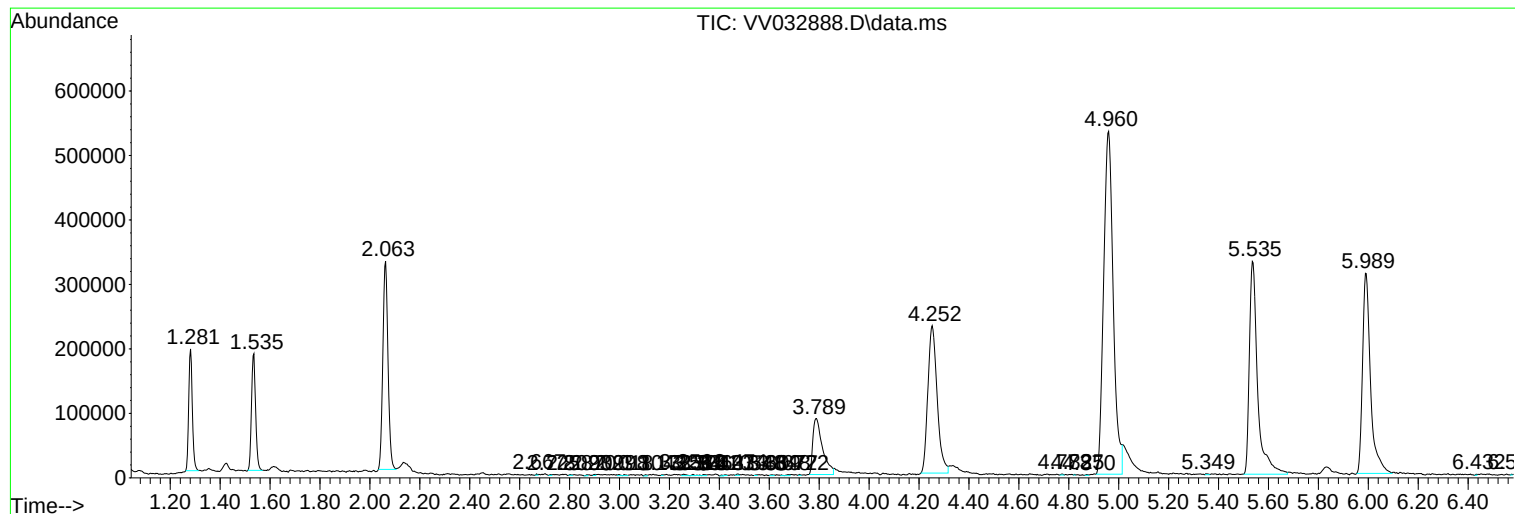

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032888.D
Acq On : 10 Nov 2023 13:44
Operator : SY/MD
Sample : VIBLK241
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032888.D
Acq On : 10 Nov 2023 13:44
Operator : SY/MD
Sample : VIBLK241
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------