

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032889.D
 Acq On : 10 Nov 2023 14:07
 Operator : SY/MD
 Sample : 05326-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rBV	205241	217857	0.60%	0.452%
2	1.536	147	154	163	rBV	183406	206363	0.57%	0.428%
3	2.063	309	318	330	rBV	358708	522133	1.44%	1.083%
4	2.378	414	416	417	rBV2	1518	612	0.00%	0.001%
5	2.429	430	432	435	rBV4	1625	788	0.00%	0.002%
6	2.446	435	437	438	rBV2	1710	652	0.00%	0.001%
7	2.581	474	479	480	rBV5	1972	1415	0.00%	0.003%
8	2.590	480	482	487	rBV5	1211	1040	0.00%	0.002%
9	2.667	502	506	508	rBV5	1796	1039	0.00%	0.002%
10	2.696	508	515	517	rBV7	4502	4695	0.01%	0.010%
11	2.783	540	542	543	rVV2	2006	739	0.00%	0.002%
12	2.790	543	544	547	rVB3	1514	608	0.00%	0.001%
13	2.812	549	551	554	rVB3	1543	819	0.00%	0.002%
14	2.831	554	557	560	rVB5	1444	1127	0.00%	0.002%
15	2.912	578	582	585	rBV6	1406	1080	0.00%	0.002%
16	2.986	603	605	607	rBV3	1517	849	0.00%	0.002%
17	3.114	641	645	646	rBV4	1715	1065	0.00%	0.002%
18	3.249	684	687	690	rBV4	1728	1547	0.00%	0.003%
19	3.317	706	708	710	rBV3	1049	643	0.00%	0.001%
20	3.375	724	726	729	rBV4	1302	841	0.00%	0.002%
21	3.391	729	731	734	rVV4	1245	631	0.00%	0.001%
22	3.468	751	755	759	rBV6	1481	1388	0.00%	0.003%
23	3.655	811	813	819	rBV5	1050	1044	0.00%	0.002%
24	3.706	827	829	833	rVB5	2024	1139	0.00%	0.002%
25	3.732	834	837	842	rBV6	1470	1318	0.00%	0.003%
26	3.786	845	854	886	rBV	82312	285521	0.79%	0.592%
27	4.076	942	944	949	rBV5	2069	1921	0.01%	0.004%
28	4.253	985	999	1020	rBV	237370	605178	1.67%	1.256%
29	4.896	1194	1199	1200	rBV5	1276	1196	0.00%	0.002%
30	4.960	1203	1219	1234	rBV2	535402	1408719	3.88%	2.923%
31	5.336	1334	1336	1338	rBV3	1724	896	0.00%	0.002%
32	5.413	1358	1360	1364	rVB5	2358	1198	0.00%	0.002%
33	5.539	1384	1399	1430	rBV	375939	882380	2.43%	1.831%
34	5.838	1481	1492	1525	rVB2	231239	521513	1.44%	1.082%
35	5.992	1529	1540	1572	rVB	308070	697954	1.92%	1.448%
36	6.365	1651	1656	1658	rBV5	1925	1828	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032889.D
 Acq On : 10 Nov 2023 14:07
 Operator : SY/MD
 Sample : 05326-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.413	1669	1671	1674	rVB4	1607	647	0.00%	0.001%
38	6.471	1685	1689	1691	rBV4	1689	1504	0.00%	0.003%
39	6.526	1704	1706	1710	rBV4	1215	1075	0.00%	0.002%
40	6.767	1778	1781	1783	rVB3	1434	757	0.00%	0.002%
41	6.838	1800	1803	1805	rBV4	1291	760	0.00%	0.002%
42	6.915	1817	1827	1846	rBV	161708	316989	0.87%	0.658%
43	7.246	1919	1930	1958	rBV	653859	1205939	3.32%	2.502%
44	7.503	2008	2010	2013	rBV4	1610	1213	0.00%	0.003%
45	7.555	2018	2026	2052	rVV2	115414	221375	0.61%	0.459%
46	7.912	2121	2137	2164	rBV	21683270	36269790	100.00%	75.260%
47	8.027	2166	2173	2207	rVB	332478	667872	1.84%	1.386%
48	8.703	2381	2383	2389	rBV6	1197	1023	0.00%	0.002%
49	8.786	2398	2409	2431	rBV	668771	1128268	3.11%	2.341%
50	9.346	2579	2583	2587	rBV6	2120	2286	0.01%	0.005%
51	9.458	2612	2618	2620	rBV6	1309	1124	0.00%	0.002%
52	9.487	2625	2627	2629	rBV3	1425	850	0.00%	0.002%
53	9.574	2647	2654	2657	rVB8	1768	2213	0.01%	0.005%
54	9.593	2657	2660	2664	rBV6	2010	1328	0.00%	0.003%
55	9.677	2684	2686	2691	rVB6	1590	1106	0.00%	0.002%
56	9.715	2696	2698	2700	rVB3	1459	618	0.00%	0.001%
57	9.731	2700	2703	2705	rBV4	1918	1294	0.00%	0.003%
58	9.770	2713	2715	2717	rBV4	1142	623	0.00%	0.001%
59	9.783	2717	2719	2721	rBV4	1934	1132	0.00%	0.002%
60	9.973	2773	2778	2787	rBV10	2423	3790	0.01%	0.008%
61	10.008	2787	2789	2793	rVB5	2242	1361	0.00%	0.003%
62	10.072	2803	2809	2811	rBV6	1561	1624	0.00%	0.003%
63	10.156	2824	2835	2850	rBV	460261	732872	2.02%	1.521%
64	10.432	2915	2921	2922	rBV5	2249	2121	0.01%	0.004%
65	10.542	2950	2955	2957	rVB6	1683	1194	0.00%	0.002%
66	10.558	2957	2960	2962	rBV4	3236	2099	0.01%	0.004%
67	10.625	2979	2981	2984	rVB4	1676	783	0.00%	0.002%
68	10.738	3013	3016	3019	rBV5	1300	873	0.00%	0.002%
69	10.831	3041	3045	3047	rBV4	1137	980	0.00%	0.002%
70	10.883	3058	3061	3062	rBV3	1407	1004	0.00%	0.002%
71	10.908	3067	3069	3070	rBV2	2545	1145	0.00%	0.002%
72	11.188	3145	3156	3180	rBV	670782	1042353	2.87%	2.163%
73	11.423	3225	3229	3231	rBV5	1703	1268	0.00%	0.003%
74	11.481	3243	3247	3249	rBV6	1626	1392	0.00%	0.003%
75	11.510	3253	3256	3259	rBV5	2302	1766	0.00%	0.004%
76	11.561	3261	3272	3294	rVV	737642	1160141	3.20%	2.407%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032889.D
 Acq On : 10 Nov 2023 14:07
 Operator : SY/MD
 Sample : 05326-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.973	3398	3400	3405	rBV6	1178	949	0.00%	0.002%
78	11.992	3405	3406	3409	rBV3	1234	670	0.00%	0.001%
79	12.037	3418	3420	3423	rVB4	1573	680	0.00%	0.001%
80	12.053	3423	3425	3427	rBV3	1779	904	0.00%	0.002%
81	12.127	3447	3448	3453	rVB5	2828	1663	0.00%	0.003%
82	12.149	3453	3455	3456	rBV2	1792	764	0.00%	0.002%
83	12.249	3481	3486	3489	rBV5	2141	1792	0.00%	0.004%
84	12.487	3558	3560	3562	rBV2	1302	675	0.00%	0.001%
85	12.577	3586	3588	3590	rBV4	1297	723	0.00%	0.002%
86	12.641	3606	3608	3615	rBV6	1789	2123	0.01%	0.004%
87	12.770	3646	3648	3650	rVB3	1476	609	0.00%	0.001%
88	12.918	3692	3694	3697	rBV4	981	671	0.00%	0.001%
89	12.960	3705	3707	3709	rBV3	1111	617	0.00%	0.001%
90	13.111	3749	3754	3757	rBV6	955	1087	0.00%	0.002%
91	13.252	3796	3798	3801	rBV4	997	639	0.00%	0.001%
92	13.284	3805	3808	3810	rBV4	2322	1730	0.00%	0.004%
93	13.526	3881	3883	3887	rVB5	1640	881	0.00%	0.002%
94	13.571	3894	3897	3898	rBV3	1636	780	0.00%	0.002%
95	13.963	4016	4019	4021	rBV3	1338	836	0.00%	0.002%
96	14.172	4081	4084	4087	rBV4	1116	949	0.00%	0.002%
97	14.220	4095	4099	4100	rBV3	1569	1318	0.00%	0.003%
98	14.458	4170	4173	4175	rBV4	2800	1508	0.00%	0.003%
99	14.693	4240	4246	4248	rBV5	2696	2653	0.01%	0.006%
100	14.908	4311	4313	4315	rBV3	1856	1057	0.00%	0.002%



Sum of corrected areas: 48192566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032889.D
Acq On : 10 Nov 2023 14:07
Operator : SY/MD
Sample : 05326-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

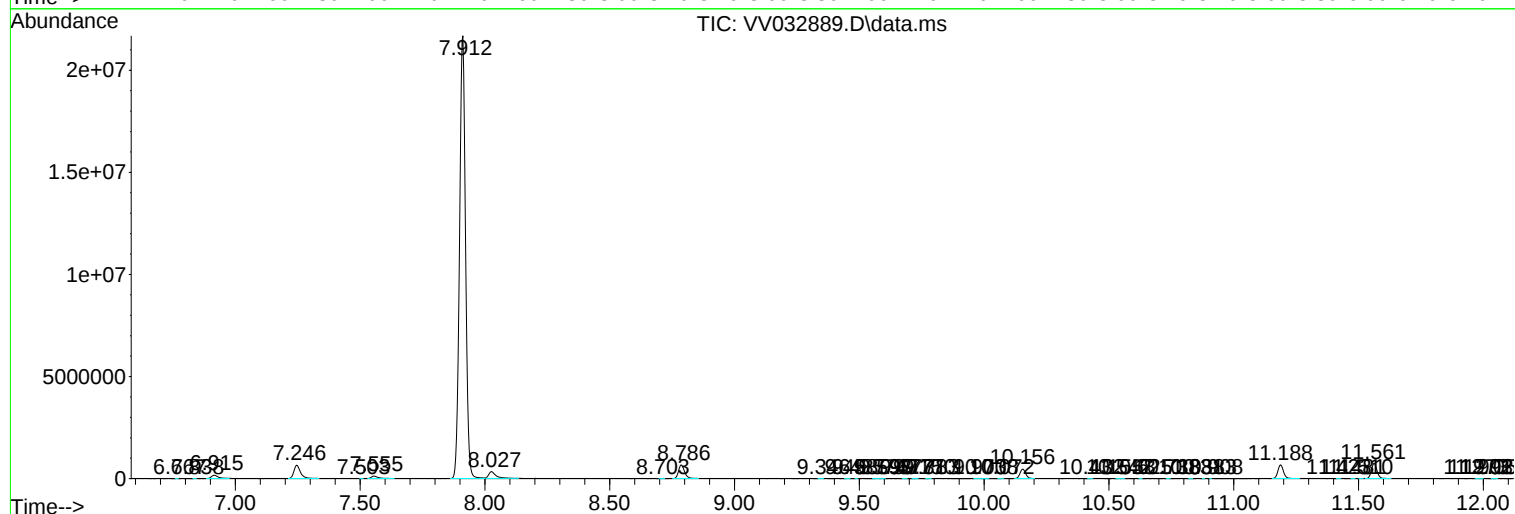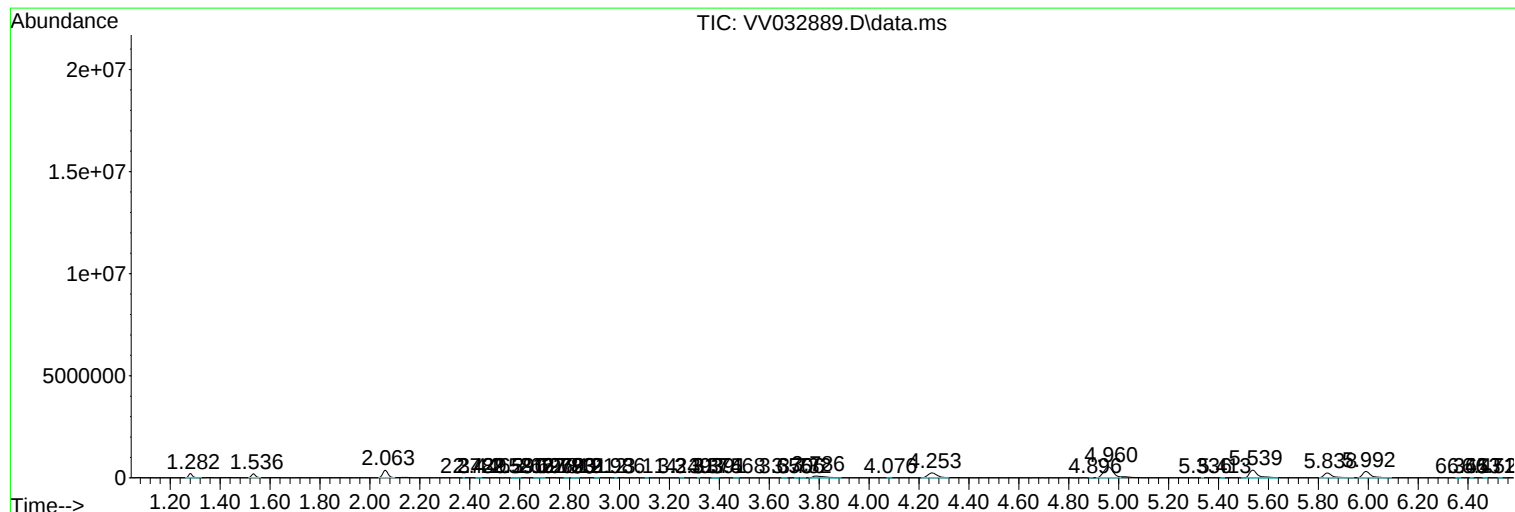

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032889.D
Acq On : 10 Nov 2023 14:07
Operator : SY/MD
Sample : 05326-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032889.D
Acq On : 10 Nov 2023 14:07
Operator : SY/MD
Sample : 05326-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc