

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032893.D
 Acq On : 10 Nov 2023 15:43
 Operator : SY/MD
 Sample : 05296-03 10X
 Misc : 5.03gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3R3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rBV	226624	249614	14.17%	1.884%
2	1.523	144	150	167	rVB	210277	255863	14.53%	1.931%
3	2.056	307	316	330	rBV	428853	618664	35.12%	4.669%
4	2.445	431	437	444	rBV9	3678	5561	0.32%	0.042%
5	2.523	459	461	465	rBV5	2635	2056	0.12%	0.016%
6	2.642	493	498	503	rBV8	1749	2073	0.12%	0.016%
7	2.667	504	506	508	rBV3	1620	863	0.05%	0.007%
8	2.693	510	514	516	rBV5	1439	903	0.05%	0.007%
9	2.735	525	527	530	rBV3	1534	453	0.03%	0.003%
10	2.777	537	540	542	rVB3	2000	1223	0.07%	0.009%
11	2.799	542	547	551	rBV8	1709	1431	0.08%	0.011%
12	2.854	561	564	569	rVB7	1550	1488	0.08%	0.011%
13	2.873	569	570	571	rBV	878	258	0.01%	0.002%
14	2.944	590	592	593	rBV	1032	556	0.03%	0.004%
15	3.008	610	612	613	rBV2	1728	786	0.04%	0.006%
16	3.047	621	624	626	rBV4	1136	671	0.04%	0.005%
17	3.111	641	644	646	rVB4	1197	685	0.04%	0.005%
18	3.124	646	648	651	rBV3	1560	1042	0.06%	0.008%
19	3.179	661	665	668	rBV6	1734	1480	0.08%	0.011%
20	3.310	703	706	710	rBV6	1799	1512	0.09%	0.011%
21	3.391	728	731	738	rVB9	1599	1683	0.10%	0.013%
22	3.416	738	739	740	rVB	957	185	0.01%	0.001%
23	3.433	740	744	750	rBV9	2462	2631	0.15%	0.020%
24	3.474	753	757	758	rBV4	1450	823	0.05%	0.006%
25	3.484	758	760	763	rVB4	1754	953	0.05%	0.007%
26	3.500	763	765	766	rBV2	771	305	0.02%	0.002%
27	3.526	770	773	776	rVB5	1320	783	0.04%	0.006%
28	3.545	776	779	781	rBV4	1130	771	0.04%	0.006%
29	3.571	784	787	789	rBV4	939	610	0.03%	0.005%
30	3.629	800	805	806	rBV5	1219	837	0.05%	0.006%
31	3.638	806	808	809	rBV2	1259	419	0.02%	0.003%
32	3.712	827	831	832	rBV3	1129	836	0.05%	0.006%
33	3.732	835	837	839	rBV3	680	364	0.02%	0.003%
34	3.783	844	853	886	rBV	94073	274699	15.59%	2.073%
35	4.188	977	979	981	rBV3	1349	683	0.04%	0.005%
36	4.249	983	998	1025	rBV	269525	714667	40.57%	5.393%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032893.D
 Acq On : 10 Nov 2023 15:43
 Operator : SY/MD
 Sample : 05296-03 10X
 Misc : 5.03gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3R3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	4.584	1098	1102	1103	rBV4	2348	1592	0.09%	0.012%
38	4.715	1139	1143	1146	rBV6	2230	2081	0.12%	0.016%
39	4.764	1156	1158	1161	rBV4	1122	610	0.03%	0.005%
40	4.883	1192	1195	1196	rBV3	1302	850	0.05%	0.006%
41	4.957	1201	1218	1263	rVV3	630927	1761534	100.00%	13.293%
42	5.535	1386	1398	1430	rBV	456665	994198	56.44%	7.503%
43	5.989	1526	1539	1572	rBV	369094	796091	45.19%	6.008%
44	6.747	1772	1775	1777	rBV4	1169	826	0.05%	0.006%
45	6.773	1781	1783	1787	rBV4	1404	871	0.05%	0.007%
46	6.857	1805	1809	1812	rBV5	2122	1671	0.09%	0.013%
47	6.915	1816	1827	1853	rVV	190802	380905	21.62%	2.875%
48	7.243	1918	1929	1958	rBV	753757	1390514	78.94%	10.494%
49	7.555	2017	2026	2042	rBV	141697	257963	14.64%	1.947%
50	7.857	2117	2120	2123	rBV5	1832	1619	0.09%	0.012%
51	7.908	2126	2136	2149	rBV5	22794	45166	2.56%	0.341%
52	8.027	2164	2173	2211	rBV	338305	666529	37.84%	5.030%
53	8.490	2315	2317	2321	rBV6	1671	1192	0.07%	0.009%
54	8.564	2339	2340	2343	rBV3	1902	1084	0.06%	0.008%
55	8.715	2386	2387	2388	rBV	1125	356	0.02%	0.003%
56	8.786	2398	2409	2434	rBV	784977	1295357	73.54%	9.775%
57	9.310	2570	2572	2573	rBV2	729	239	0.01%	0.002%
58	9.394	2595	2598	2599	rBV3	1324	657	0.04%	0.005%
59	9.464	2615	2620	2621	rBV4	1699	1368	0.08%	0.010%
60	9.677	2683	2686	2692	rBV7	2075	1576	0.09%	0.012%
61	9.780	2715	2718	2723	rBV7	2042	1930	0.11%	0.015%
62	9.821	2728	2731	2732	rBV3	956	479	0.03%	0.004%
63	9.866	2743	2745	2750	rVB5	1728	825	0.05%	0.006%
64	9.937	2764	2767	2768	rBV3	1877	867	0.05%	0.007%
65	9.966	2772	2776	2777	rBV3	1376	845	0.05%	0.006%
66	10.030	2794	2796	2800	rBV5	1081	634	0.04%	0.005%
67	10.153	2820	2834	2858	rBV	521877	838563	47.60%	6.328%
68	10.432	2919	2921	2924	rVB4	1245	586	0.03%	0.004%
69	10.474	2931	2934	2937	rBV4	1545	1143	0.06%	0.009%
70	10.844	3046	3049	3050	rBV4	1912	1109	0.06%	0.008%
71	10.892	3062	3064	3065	rBV2	1454	525	0.03%	0.004%
72	10.969	3085	3088	3089	rBV3	1505	880	0.05%	0.007%
73	11.188	3145	3156	3176	rBV	811568	1257216	71.37%	9.488%
74	11.503	3252	3254	3256	rVB3	1980	556	0.03%	0.004%
75	11.561	3261	3272	3295	rBV	862851	1381440	78.42%	10.425%
76	11.786	3340	3342	3346	rVB6	1660	728	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032893.D
Acq On : 10 Nov 2023 15:43
Operator : SY/MD
Sample : 05296-03 10X
Misc : 5.03gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3R3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

77	11.831	3353	3356	3357	rBV3	2226	1110	0.06%	0.008%
78	11.963	3395	3397	3400	rBV4	2111	1005	0.06%	0.008%
79	12.332	3511	3512	3513	rBV	1373	514	0.03%	0.004%
80	12.509	3561	3567	3572	rVB9	1759	2042	0.12%	0.015%
81	12.660	3612	3614	3616	rBV3	1178	595	0.03%	0.004%
82	12.699	3622	3626	3627	rBV4	1533	972	0.06%	0.007%
83	12.728	3632	3635	3637	rBV3	2008	1163	0.07%	0.009%
84	13.168	3769	3772	3777	rBV6	2394	2133	0.12%	0.016%




Sum of corrected areas: 13251140

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032893.D
Acq On : 10 Nov 2023 15:43
Operator : SY/MD
Sample : 05296-03 10X
Misc : 5.03gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3R3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

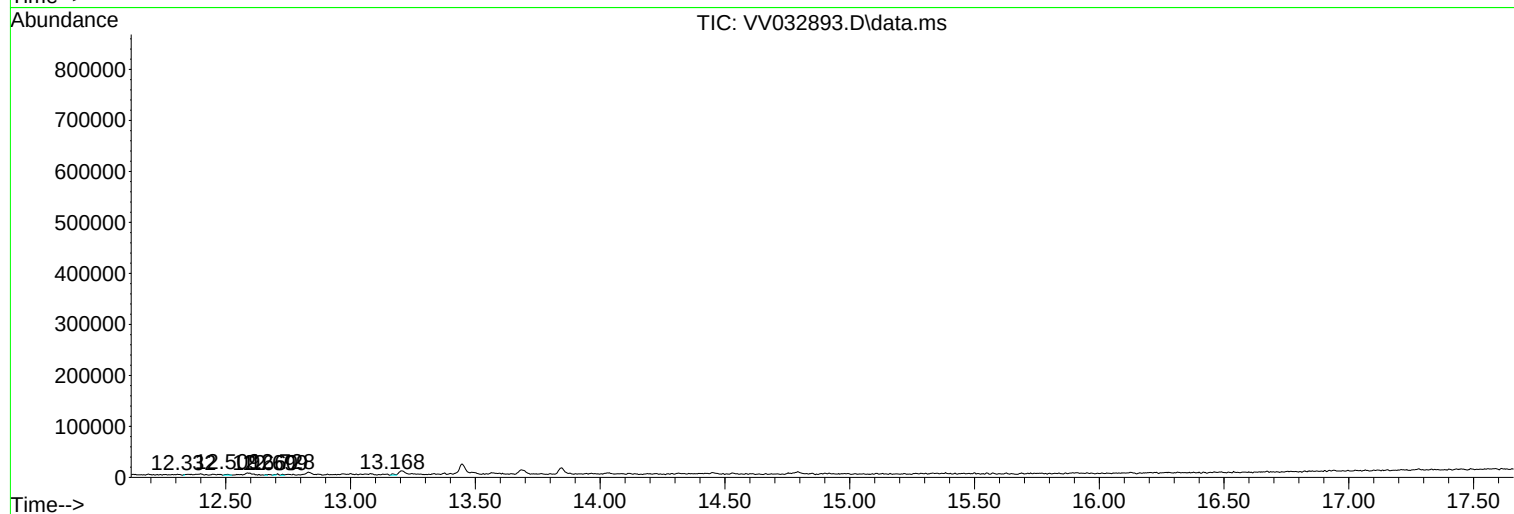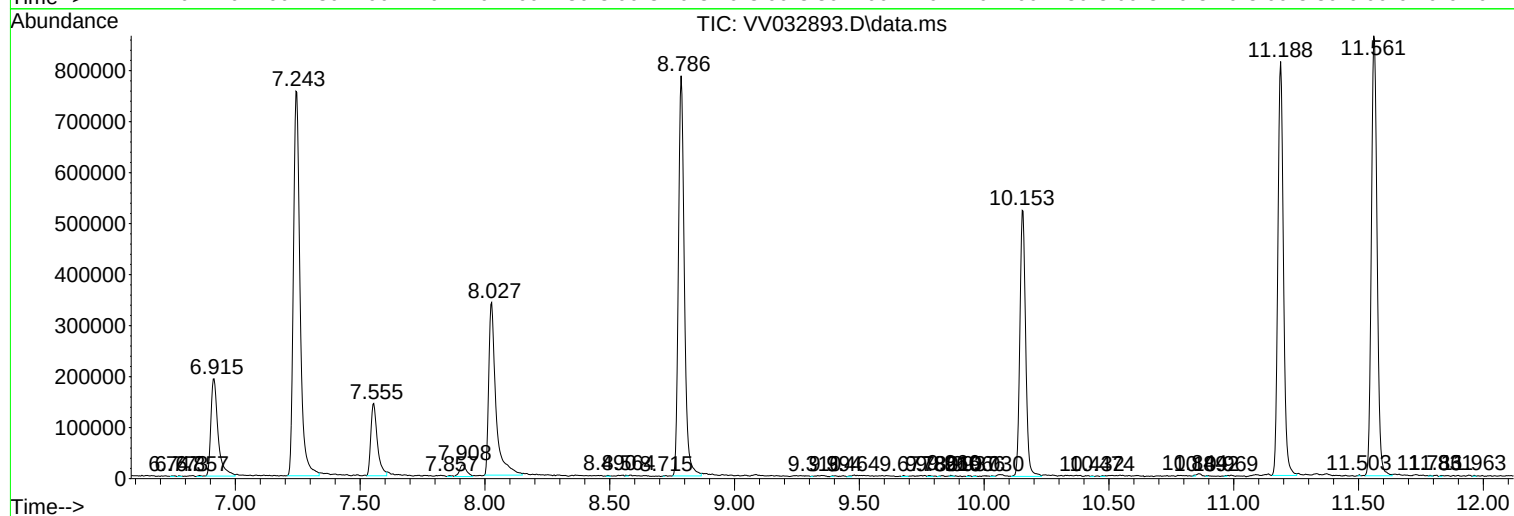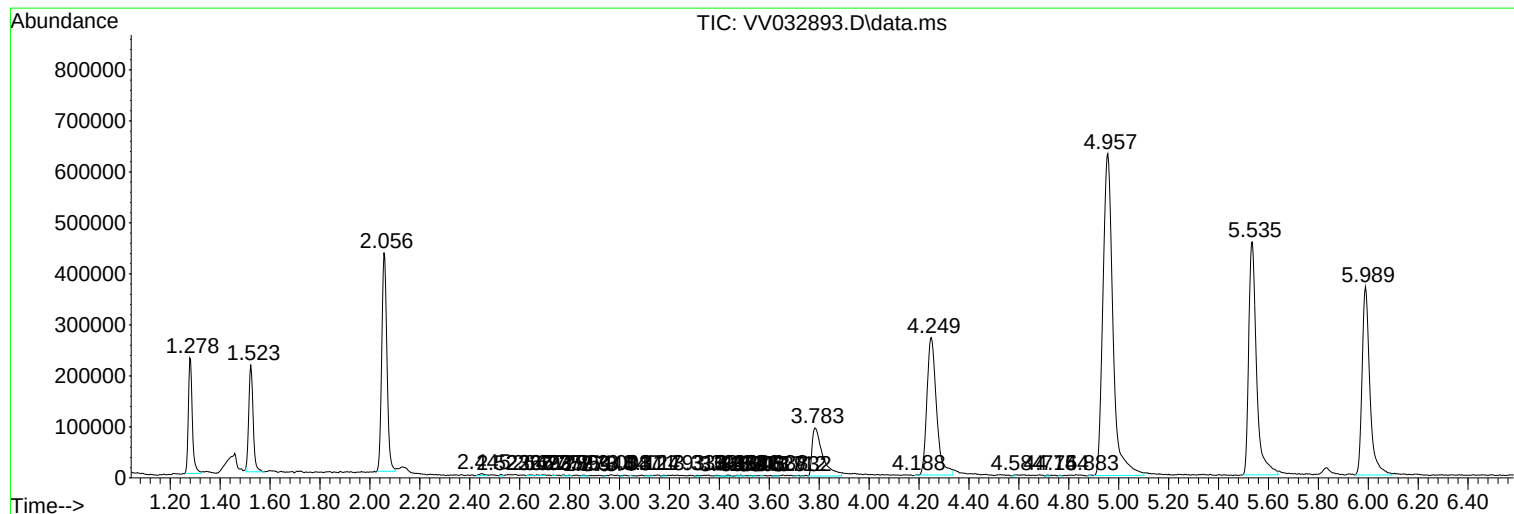

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032893.D
Acq On : 10 Nov 2023 15:43
Operator : SY/MD
Sample : 05296-03 10X
Misc : 5.03gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3R3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032893.D
Acq On : 10 Nov 2023 15:43
Operator : SY/MD
Sample : 05296-03 10X
Misc : 5.03gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3R3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------