

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032899.D
 Acq On : 10 Nov 2023 18:03
 Operator : SY/MD
 Sample : 05296-16 10X
 Misc : 5.45gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rBV	187881	208328	14.12%	1.847%
2	1.523	144	150	163	rVB	180096	210211	14.24%	1.864%
3	2.056	308	316	333	rBV	357775	513990	34.83%	4.557%
4	2.404	422	424	425	rBV2	1237	362	0.02%	0.003%
5	2.825	554	555	557	rBV3	1709	645	0.04%	0.006%
6	2.847	560	562	564	rBV3	1396	814	0.06%	0.007%
7	2.905	578	580	583	rBV5	1341	1085	0.07%	0.010%
8	2.957	593	596	599	rBV5	1439	1094	0.07%	0.010%
9	3.015	610	614	616	rBV5	1436	991	0.07%	0.009%
10	3.027	616	618	619	rBV2	1026	522	0.04%	0.005%
11	3.076	625	633	635	rBV9	2089	2229	0.15%	0.020%
12	3.114	639	645	646	rBV5	1090	864	0.06%	0.008%
13	3.150	654	656	662	rBV6	1113	1038	0.07%	0.009%
14	3.272	691	694	698	rBV5	1701	1407	0.10%	0.012%
15	3.413	737	738	739	rBV	1328	302	0.02%	0.003%
16	3.445	747	748	752	rBV4	1080	729	0.05%	0.006%
17	3.465	752	754	756	rVB3	1948	790	0.05%	0.007%
18	3.490	759	762	766	rBV5	1988	1575	0.11%	0.014%
19	3.532	772	775	777	rBV4	1798	1013	0.07%	0.009%
20	3.552	779	781	782	rBV2	484	160	0.01%	0.001%
21	3.568	782	786	787	rBV4	1776	1149	0.08%	0.010%
22	3.625	802	804	805	rBV2	737	260	0.02%	0.002%
23	3.645	808	810	811	rVV2	696	197	0.01%	0.002%
24	3.696	823	826	828	rBV3	1805	940	0.06%	0.008%
25	3.728	834	836	837	rVB2	762	247	0.02%	0.002%
26	3.786	845	854	881	rBV	83781	240306	16.28%	2.130%
27	4.249	984	998	1021	rBV	231834	600013	40.66%	5.319%
28	4.638	1116	1119	1121	rBV4	1302	819	0.06%	0.007%
29	4.879	1193	1194	1197	rBV3	1129	653	0.04%	0.006%
30	4.957	1203	1218	1261	rBV2	535909	1475749	100.00%	13.083%
31	5.535	1387	1398	1424	rBV	409129	872642	59.13%	7.736%
32	5.989	1528	1539	1572	rBV	310540	675323	45.76%	5.987%
33	6.368	1655	1657	1661	rBV5	1561	1026	0.07%	0.009%
34	6.410	1668	1670	1672	rBV3	1882	1244	0.08%	0.011%
35	6.648	1740	1744	1746	rBV5	1296	1056	0.07%	0.009%
36	6.674	1750	1752	1755	rBV3	1899	955	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032899.D
 Acq On : 10 Nov 2023 18:03
 Operator : SY/MD
 Sample : 05296-16 10X
 Misc : 5.45gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.715	1763	1765	1766	rBV2	1547	532	0.04%	0.005%
38	6.915	1818	1827	1849	rBV	155567	304889	20.66%	2.703%
39	7.104	1884	1886	1889	rBV4	2197	1378	0.09%	0.012%
40	7.156	1899	1902	1906	rBV5	1888	1658	0.11%	0.015%
41	7.246	1918	1930	1956	rBV	637029	1170699	79.33%	10.378%
42	7.555	2017	2026	2047	rBV2	117893	216246	14.65%	1.917%
43	7.911	2129	2137	2149	rBV9	9461	18023	1.22%	0.160%
44	8.027	2163	2173	2209	rBV	287872	595153	40.33%	5.276%
45	8.654	2366	2368	2369	rBV2	1174	374	0.03%	0.003%
46	8.786	2398	2409	2432	rBV	698973	1154864	78.26%	10.238%
47	9.387	2593	2596	2599	rVB4	2501	1773	0.12%	0.016%
48	9.416	2601	2605	2607	rBV4	1285	1078	0.07%	0.010%
49	9.577	2651	2655	2657	rBV4	2394	1843	0.12%	0.016%
50	9.625	2668	2670	2671	rBV2	1289	466	0.03%	0.004%
51	9.815	2723	2729	2731	rBV7	2664	2894	0.20%	0.026%
52	9.966	2772	2776	2780	rBV7	1519	1154	0.08%	0.010%
53	10.156	2824	2835	2852	rBV	452534	716577	48.56%	6.353%
54	10.474	2929	2934	2937	rBV6	1328	1268	0.09%	0.011%
55	10.622	2977	2980	2982	rBV4	2070	1354	0.09%	0.012%
56	10.657	2987	2991	2994	rBV5	2119	1591	0.11%	0.014%
57	10.963	3084	3086	3089	rVB2	1124	482	0.03%	0.004%
58	10.979	3089	3091	3095	rVB5	1385	942	0.06%	0.008%
59	11.188	3145	3156	3178	rBV	704866	1104382	74.84%	9.791%
60	11.561	3262	3272	3292	rBV	735413	1143547	77.49%	10.138%
61	11.853	3361	3363	3365	rBV3	1415	685	0.05%	0.006%
62	11.898	3376	3377	3379	rVB2	1578	543	0.04%	0.005%
63	11.915	3381	3382	3384	rBV2	1219	425	0.03%	0.004%
64	12.143	3451	3453	3456	rVB3	1632	854	0.06%	0.008%
65	12.403	3529	3534	3536	rBV6	1778	1803	0.12%	0.016%
66	12.554	3580	3581	3582	rBV	835	288	0.02%	0.003%
67	12.725	3633	3634	3639	rVB5	1748	1249	0.08%	0.011%
68	12.767	3645	3647	3651	rBV4	1516	1135	0.08%	0.010%
69	12.818	3660	3663	3665	rBV3	1832	1161	0.08%	0.010%
70	12.982	3710	3714	3723	rVB9	3078	3338	0.23%	0.030%
71	13.496	3872	3874	3875	rBV2	1016	375	0.03%	0.003%
72	14.352	4138	4140	4142	rBV3	1538	736	0.05%	0.007%
73	14.394	4150	4153	4156	rBV4	1692	1037	0.07%	0.009%
74	14.467	4174	4176	4180	rBV4	2197	1075	0.07%	0.010%
75	15.310	4435	4438	4441	rBV5	1926	1464	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032899.D
Acq On : 10 Nov 2023 18:03
Operator : SY/MD
Sample : 05296-16 10X
Misc : 5.45gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis




Sum of corrected areas: 11280063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032899.D
Acq On : 10 Nov 2023 18:03
Operator : SY/MD
Sample : 05296-16 10X
Misc : 5.45gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

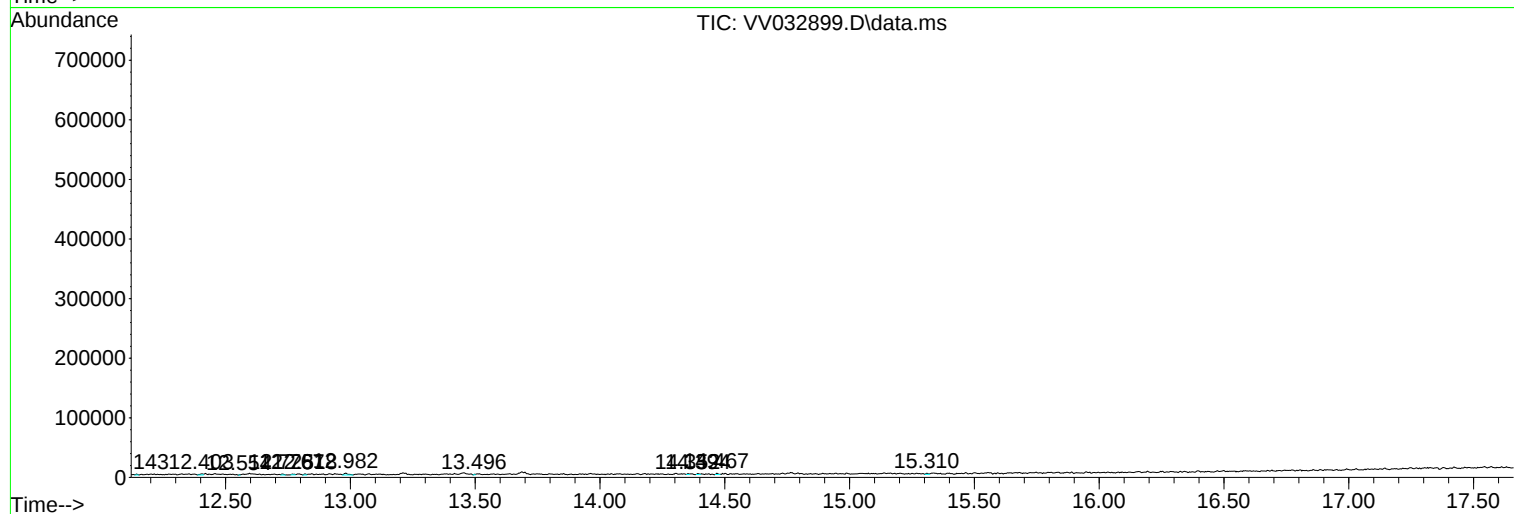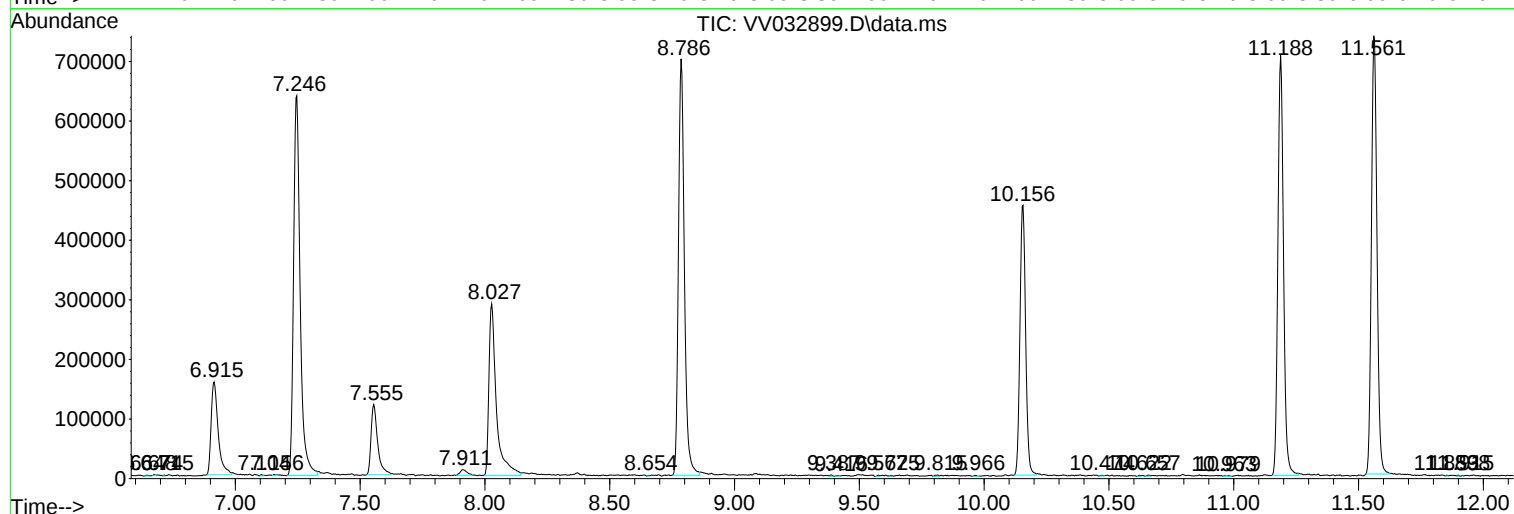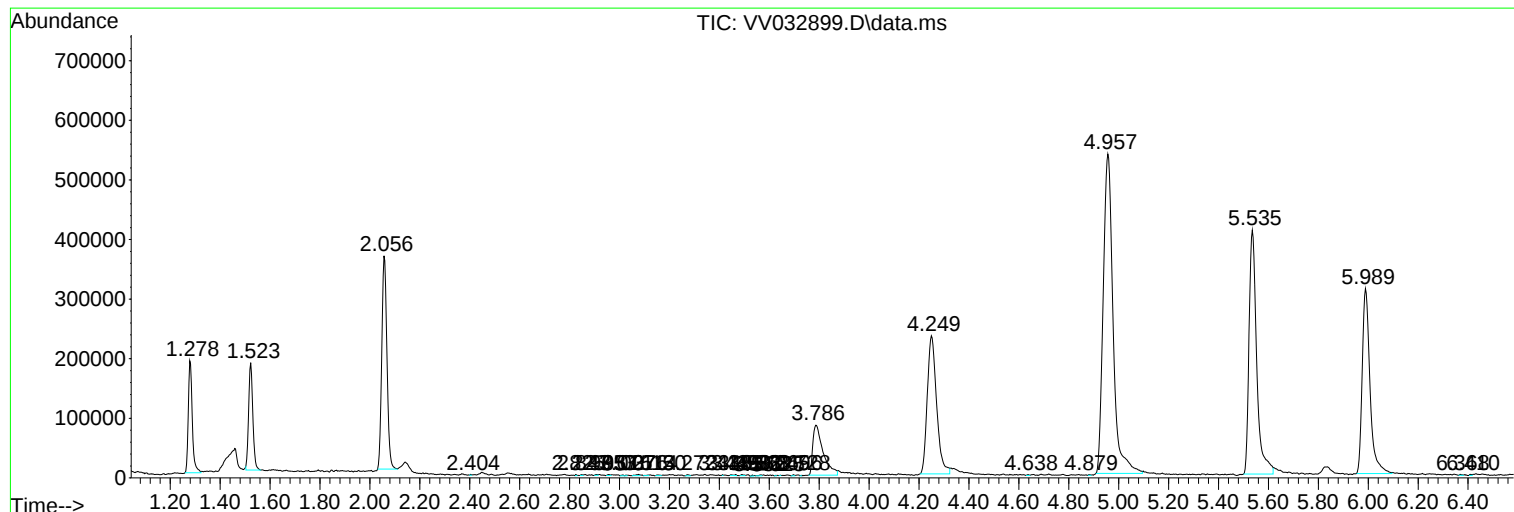

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032899.D
Acq On : 10 Nov 2023 18:03
Operator : SY/MD
Sample : 05296-16 10X
Misc : 5.45gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032899.D
Acq On : 10 Nov 2023 18:03
Operator : SY/MD
Sample : 05296-16 10X
Misc : 5.45gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc