

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032902.D
 Acq On : 10 Nov 2023 19:59
 Operator : SY/MD
 Sample : VV1110MBL02
 Misc : 5.00gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK216

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV	233133	246837	14.89%	2.051%
2	1.532	147	153	166	rVB	200050	230864	13.93%	1.918%
3	2.063	309	318	331	rBV	401249	576371	34.78%	4.789%
4	2.529	461	463	465	rBV3	2055	1372	0.08%	0.011%
5	2.732	525	526	531	rVB5	1938	1315	0.08%	0.011%
6	2.838	557	559	560	rBV2	736	297	0.02%	0.002%
7	2.899	576	578	579	rBV2	1250	353	0.02%	0.003%
8	3.037	618	621	624	rBV3	1387	865	0.05%	0.007%
9	3.085	634	636	637	rVB2	1075	277	0.02%	0.002%
10	3.095	637	639	642	rVB3	1370	753	0.05%	0.006%
11	3.114	642	645	648	rBV5	1561	1285	0.08%	0.011%
12	3.175	662	664	668	rVB3	2031	1282	0.08%	0.011%
13	3.192	668	669	670	rVB	778	150	0.01%	0.001%
14	3.201	670	672	673	rBV	877	422	0.03%	0.004%
15	3.217	674	677	678	rBV2	1082	628	0.04%	0.005%
16	3.246	684	686	688	rBV3	1214	546	0.03%	0.005%
17	3.298	699	702	704	rBV4	1284	789	0.05%	0.007%
18	3.307	704	705	706	rBV	847	242	0.01%	0.002%
19	3.375	722	726	729	rBV6	1266	1037	0.06%	0.009%
20	3.413	734	738	739	rBV4	1679	1031	0.06%	0.009%
21	3.442	745	747	748	rBV3	1355	622	0.04%	0.005%
22	3.474	752	757	760	rBV7	1859	1655	0.10%	0.014%
23	3.513	766	769	773	rBV6	1170	778	0.05%	0.006%
24	3.587	790	792	794	rBV2	793	327	0.02%	0.003%
25	3.651	809	812	813	rBV3	1148	587	0.04%	0.005%
26	3.716	829	832	834	rBV4	927	513	0.03%	0.004%
27	3.786	846	854	882	rBV	89630	256507	15.48%	2.131%
28	4.253	985	999	1019	rBV	250652	648412	39.13%	5.388%
29	4.677	1129	1131	1134	rBV4	1368	597	0.04%	0.005%
30	4.690	1134	1135	1137	rBV2	1270	718	0.04%	0.006%
31	4.822	1174	1176	1180	rBV5	1433	1013	0.06%	0.008%
32	4.892	1197	1198	1200	rBV3	652	212	0.01%	0.002%
33	4.960	1202	1219	1264	rVV2	574577	1657221	100.00%	13.770%
34	5.535	1387	1398	1435	rBV	383585	862025	52.02%	7.163%
35	5.992	1527	1540	1577	rBV	331571	746611	45.05%	6.204%
36	6.584	1722	1724	1726	rBV3	1458	709	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032902.D
 Acq On : 10 Nov 2023 19:59
 Operator : SY/MD
 Sample : VV1110MBL02
 Misc : 5.00gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK216

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.638	1739	1741	1743	rBV2	1544	522	0.03%	0.004%
38	6.777	1782	1784	1785	rVB2	1022	223	0.01%	0.002%
39	6.831	1799	1801	1803	rBV3	1406	748	0.05%	0.006%
40	6.915	1817	1827	1855	rBV	172653	347269	20.95%	2.885%
41	7.246	1917	1930	1957	rBV	703403	1305851	78.80%	10.850%
42	7.555	2017	2026	2051	rBV	125616	241680	14.58%	2.008%
43	7.822	2107	2109	2112	rBV5	2017	1061	0.06%	0.009%
44	8.027	2163	2173	2204	rBV	308591	639184	38.57%	5.311%
45	8.529	2328	2329	2331	rBV2	1460	427	0.03%	0.004%
46	8.786	2398	2409	2431	rBV	662763	1114531	67.25%	9.261%
47	9.217	2541	2543	2547	rVB4	3013	1572	0.09%	0.013%
48	9.236	2547	2549	2551	rBV2	570	284	0.02%	0.002%
49	9.317	2570	2574	2577	rVB6	2166	1413	0.09%	0.012%
50	9.330	2577	2578	2579	rBV	1414	378	0.02%	0.003%
51	9.375	2591	2592	2594	rBV2	1231	601	0.04%	0.005%
52	9.519	2635	2637	2642	rBV4	2089	1430	0.09%	0.012%
53	9.568	2650	2652	2653	rBV2	1258	423	0.03%	0.004%
54	9.622	2666	2669	2670	rBV3	1697	1050	0.06%	0.009%
55	9.712	2692	2697	2700	rBV6	1885	1522	0.09%	0.013%
56	9.805	2725	2726	2728	rBV2	1300	432	0.03%	0.004%
57	9.944	2766	2769	2771	rBV4	917	576	0.03%	0.005%
58	10.043	2796	2800	2804	rBV7	2366	3072	0.19%	0.026%
59	10.088	2812	2814	2818	rBV5	1713	1286	0.08%	0.011%
60	10.156	2824	2835	2860	rVB	478692	768126	46.35%	6.382%
61	10.574	2963	2965	2968	rBV3	1085	388	0.02%	0.003%
62	10.683	2997	2999	3003	rVB4	2085	1018	0.06%	0.008%
63	10.735	3013	3015	3016	rBV2	1131	389	0.02%	0.003%
64	10.793	3030	3033	3035	rBV3	2127	1542	0.09%	0.013%
65	10.953	3081	3083	3085	rBV3	1080	477	0.03%	0.004%
66	11.011	3099	3101	3104	rBV4	1037	471	0.03%	0.004%
67	11.188	3145	3156	3178	rBV	663579	1048098	63.24%	8.709%
68	11.522	3256	3260	3261	rBV4	1532	1293	0.08%	0.011%
69	11.561	3261	3272	3289	rVV	769040	1214236	73.27%	10.089%
70	11.863	3363	3366	3368	rBV4	1378	1003	0.06%	0.008%
71	11.886	3370	3373	3375	rBV3	1748	1027	0.06%	0.009%
72	12.056	3424	3426	3429	rBV4	1505	853	0.05%	0.007%
73	12.079	3429	3433	3437	rBV7	1939	2447	0.15%	0.020%
74	12.137	3447	3451	3452	rBV3	1817	1344	0.08%	0.011%
75	12.185	3463	3466	3468	rBV4	1918	1149	0.07%	0.010%
76	12.275	3491	3494	3495	rBV3	1101	568	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032902.D
 Acq On : 10 Nov 2023 19:59
 Operator : SY/MD
 Sample : VV1110MBL02
 Misc : 5.00gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK216

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.323	3504	3509	3511	rBV5	2501	1984	0.12%	0.016%
78	12.538	3571	3576	3579	rBV6	1798	1620	0.10%	0.013%
79	12.558	3579	3582	3584	rBV4	1413	1000	0.06%	0.008%
80	12.593	3585	3593	3600	rVV8	5144	8156	0.49%	0.068%
81	12.873	3676	3680	3681	rBV3	1704	1265	0.08%	0.011%
82	12.960	3703	3707	3711	rBV7	2070	1988	0.12%	0.017%
83	13.043	3731	3733	3734	rBV2	1175	422	0.03%	0.004%
84	13.069	3738	3741	3742	rBV3	1328	694	0.04%	0.006%
85	13.172	3771	3773	3774	rVB2	1028	290	0.02%	0.002%
86	13.207	3774	3784	3792	rBV2	8895	16911	1.02%	0.141%
87	13.278	3802	3806	3808	rBV5	1980	1413	0.09%	0.012%
88	13.349	3827	3828	3831	rBV3	1345	665	0.04%	0.006%
89	13.384	3837	3839	3843	rVB5	1925	1147	0.07%	0.010%
90	13.445	3848	3858	3868	rBV	20755	36173	2.18%	0.301%
91	13.763	3954	3957	3959	rBV4	1311	839	0.05%	0.007%
92	13.812	3968	3972	3973	rBV5	1370	823	0.05%	0.007%
93	14.056	4047	4048	4051	rVB3	1790	568	0.03%	0.005%
94	14.136	4071	4073	4076	rBV3	1506	993	0.06%	0.008%
95	14.210	4093	4096	4097	rBV3	1106	688	0.04%	0.006%
96	14.805	4279	4281	4282	rBV2	1250	472	0.03%	0.004%
97	15.127	4379	4381	4386	rVB6	2598	1693	0.10%	0.014%




Sum of corrected areas: 12034991

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032902.D
Acq On : 10 Nov 2023 19:59
Operator : SY/MD
Sample : VV1110MBL02
Misc : 5.00gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

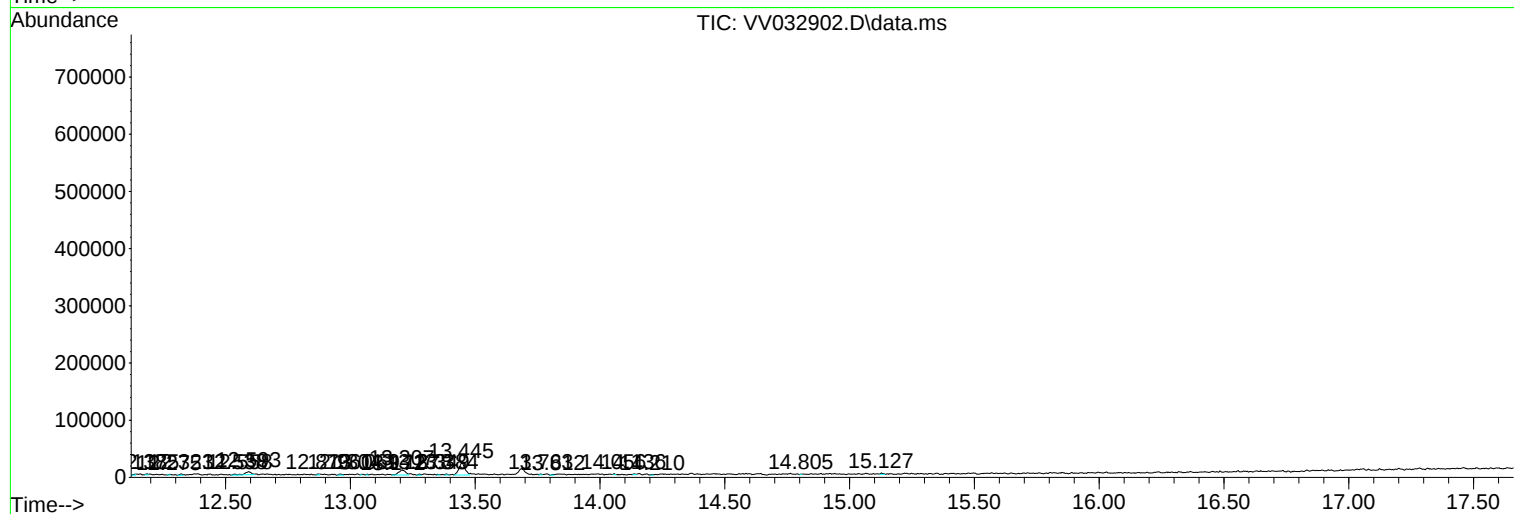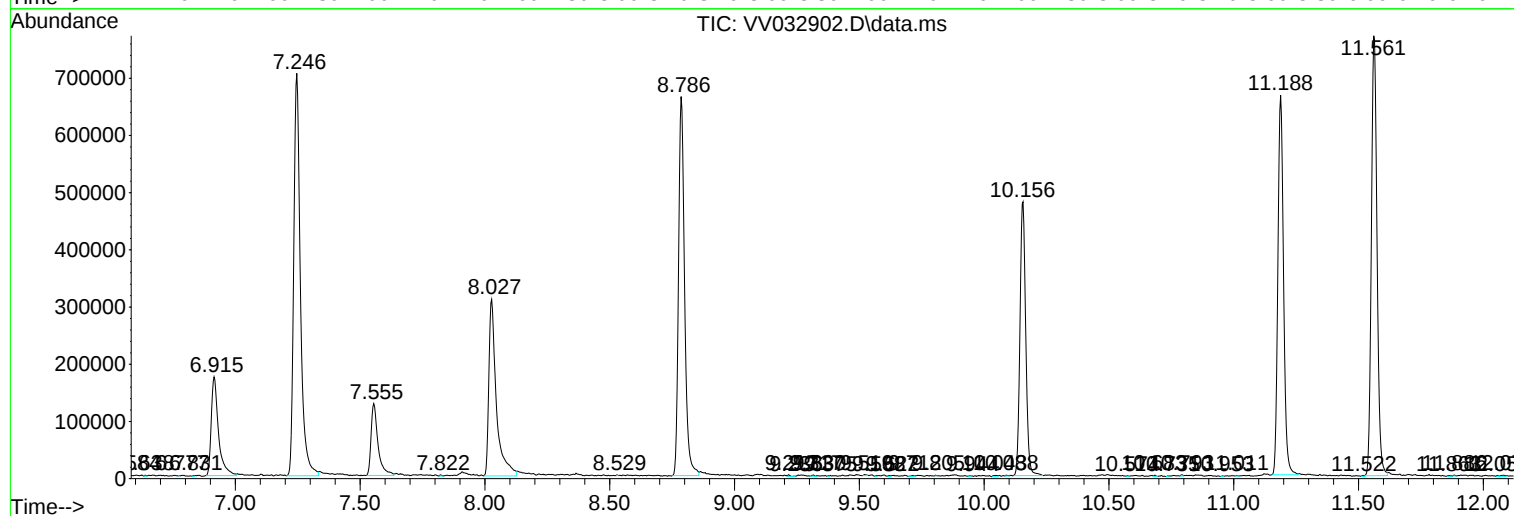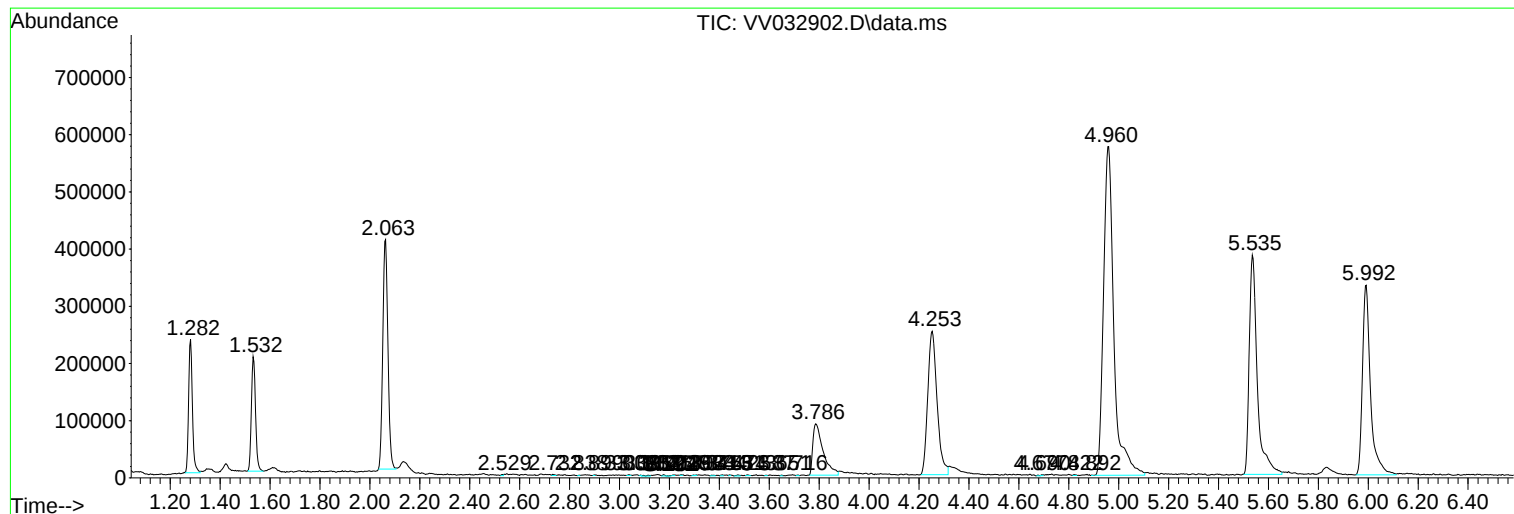

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032902.D
Acq On : 10 Nov 2023 19:59
Operator : SY/MD
Sample : VV1110MBL02
Misc : 5.00gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032902.D
Acq On : 10 Nov 2023 19:59
Operator : SY/MD
Sample : VV1110MBL02
Misc : 5.00gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc