

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032917.D
 Acq On : 11 Nov 2023 01:48
 Operator : SY/MD
 Sample : VIBLK244
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	188642	193394	13.05%	1.693%
2	1.532	147	153	169	rVB	174282	209528	14.13%	1.834%
3	2.063	309	318	333	rBV	339392	491216	33.14%	4.299%
4	2.314	394	396	397	rBV2	1617	669	0.05%	0.006%
5	2.449	431	438	439	rBV6	4546	4433	0.30%	0.039%
6	2.645	497	499	500	rBV2	1104	623	0.04%	0.005%
7	2.834	554	558	559	rBV4	1903	1294	0.09%	0.011%
8	2.886	571	574	576	rBV3	1081	597	0.04%	0.005%
9	2.921	583	585	587	rBV3	1683	939	0.06%	0.008%
10	2.992	603	607	611	rBV5	1937	2143	0.14%	0.019%
11	3.027	615	618	620	rBV4	816	572	0.04%	0.005%
12	3.053	623	626	629	rBV5	1210	847	0.06%	0.007%
13	3.082	633	635	639	rBV6	1925	1569	0.11%	0.014%
14	3.114	644	645	647	rBV2	674	326	0.02%	0.003%
15	3.175	658	664	665	rBV6	1504	1320	0.09%	0.012%
16	3.233	678	682	684	rBV4	1745	1424	0.10%	0.012%
17	3.387	728	730	731	rBV2	916	368	0.02%	0.003%
18	3.397	731	733	735	rVV3	1372	602	0.04%	0.005%
19	3.436	740	745	747	rBV6	1251	1332	0.09%	0.012%
20	3.497	762	764	766	rVB3	1217	396	0.03%	0.003%
21	3.516	766	770	774	rBV7	1769	1740	0.12%	0.015%
22	3.548	779	780	782	rBV2	931	493	0.03%	0.004%
23	3.670	815	818	819	rBV3	1091	505	0.03%	0.004%
24	3.715	830	832	834	rVB3	960	483	0.03%	0.004%
25	3.741	836	840	844	rBV6	1271	1473	0.10%	0.013%
26	3.789	846	855	879	rBV	86033	234762	15.84%	2.055%
27	4.252	985	999	1026	rBV	233770	601726	40.59%	5.266%
28	4.612	1108	1111	1112	rBV2	1908	1102	0.07%	0.010%
29	4.686	1132	1134	1141	rVB8	2268	1850	0.12%	0.016%
30	4.715	1141	1143	1147	rBV4	1228	879	0.06%	0.008%
31	4.857	1186	1187	1189	rVB2	1240	418	0.03%	0.004%
32	4.960	1202	1219	1248	rBV2	544764	1482345	100.00%	12.973%
33	5.535	1386	1398	1425	rBV	467157	967004	65.23%	8.463%
34	5.992	1528	1540	1566	rBV	320344	670535	45.23%	5.868%
35	6.400	1665	1667	1671	rVB3	1612	723	0.05%	0.006%
36	6.419	1671	1673	1674	rBV2	2042	802	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032917.D
 Acq On : 11 Nov 2023 01:48
 Operator : SY/MD
 Sample : VIBLK244
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.513	1700	1702	1706	rBV5	1616	876	0.06%	0.008%
38	6.693	1755	1758	1761	rBV5	1727	835	0.06%	0.007%
39	6.731	1767	1770	1773	rBV5	2311	1574	0.11%	0.014%
40	6.915	1817	1827	1856	rBV	166384	318165	21.46%	2.784%
41	7.120	1889	1891	1895	rBV5	1563	1239	0.08%	0.011%
42	7.246	1919	1930	1953	rBV	625149	1120937	75.62%	9.810%
43	7.554	2016	2026	2053	rBV	117717	219983	14.84%	1.925%
44	7.776	2092	2095	2097	rBV4	1906	1055	0.07%	0.009%
45	7.821	2105	2109	2111	rBV5	1674	1274	0.09%	0.011%
46	7.982	2156	2159	2163	rBV6	2429	2440	0.16%	0.021%
47	8.027	2164	2173	2201	rVV	293343	577873	38.98%	5.057%
48	8.448	2302	2304	2307	rBV4	1228	592	0.04%	0.005%
49	8.471	2309	2311	2313	rBV4	1651	833	0.06%	0.007%
50	8.554	2336	2337	2341	rBV4	1618	1197	0.08%	0.010%
51	8.593	2347	2349	2353	rVB5	1880	1218	0.08%	0.011%
52	8.731	2390	2392	2394	rBV3	1147	631	0.04%	0.006%
53	8.744	2394	2396	2397	rBV2	1285	622	0.04%	0.005%
54	8.786	2398	2409	2431	rVV	739712	1217496	82.13%	10.655%
55	9.140	2518	2519	2522	rVB3	1552	643	0.04%	0.006%
56	9.223	2543	2545	2551	rBV6	1525	1526	0.10%	0.013%
57	9.326	2571	2577	2579	rBV7	1669	1351	0.09%	0.012%
58	9.606	2662	2664	2667	rVB5	1377	747	0.05%	0.007%
59	9.680	2685	2687	2689	rBV2	617	284	0.02%	0.002%
60	9.699	2689	2693	2694	rBV4	1546	1027	0.07%	0.009%
61	9.853	2739	2741	2744	rBV4	1869	1022	0.07%	0.009%
62	9.876	2746	2748	2750	rVV3	1396	550	0.04%	0.005%
63	10.011	2788	2790	2793	rVB4	2022	1036	0.07%	0.009%
64	10.030	2794	2796	2797	rVB2	1039	277	0.02%	0.002%
65	10.066	2804	2807	2809	rBV4	1652	1081	0.07%	0.009%
66	10.082	2809	2812	2815	rVB5	1621	1101	0.07%	0.010%
67	10.101	2815	2818	2820	rBV4	1322	762	0.05%	0.007%
68	10.156	2822	2835	2853	rBV	445975	721375	48.66%	6.313%
69	10.381	2902	2905	2906	rBV3	1713	967	0.07%	0.008%
70	10.496	2939	2941	2943	rBV3	1364	938	0.06%	0.008%
71	10.532	2949	2952	2954	rBV3	1792	1295	0.09%	0.011%
72	10.734	3013	3015	3016	rBV2	1237	571	0.04%	0.005%
73	10.841	3046	3048	3050	rBV3	948	327	0.02%	0.003%
74	10.873	3056	3058	3063	rBV6	1700	1364	0.09%	0.012%
75	10.956	3082	3084	3087	rBV3	1039	582	0.04%	0.005%
76	10.972	3087	3089	3090	rBV2	869	311	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032917.D
 Acq On : 11 Nov 2023 01:48
 Operator : SY/MD
 Sample : VIBLK244
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.005	3097	3099	3100	rBV3	702	311	0.02%	0.003%
78	11.120	3133	3135	3136	rBV2	1379	622	0.04%	0.005%
79	11.130	3136	3138	3139	rVV2	1992	630	0.04%	0.006%
80	11.188	3145	3156	3180	rBV	757014	1180691	79.65%	10.333%
81	11.291	3186	3188	3190	rBV3	1964	998	0.07%	0.009%
82	11.519	3256	3259	3260	rBV3	1780	999	0.07%	0.009%
83	11.564	3261	3273	3291	rVV	702626	1130073	76.24%	9.890%
84	11.789	3341	3343	3351	rBV8	1503	1427	0.10%	0.012%
85	11.908	3377	3380	3381	rBV3	1076	535	0.04%	0.005%
86	11.966	3397	3398	3402	rBV4	1161	622	0.04%	0.005%
87	12.294	3498	3500	3502	rBV3	727	390	0.03%	0.003%
88	12.316	3502	3507	3511	rBV8	1491	1929	0.13%	0.017%
89	12.361	3517	3521	3524	rBV6	2321	2206	0.15%	0.019%
90	12.390	3529	3530	3534	rBV4	1003	553	0.04%	0.005%
91	12.667	3615	3616	3618	rBV2	1323	523	0.04%	0.005%
92	12.696	3618	3625	3631	rVV10	2175	3333	0.22%	0.029%
93	12.754	3640	3643	3649	rBV7	1784	1176	0.08%	0.010%
94	12.914	3690	3693	3695	rBV4	1548	1167	0.08%	0.010%
95	13.053	3734	3736	3737	rBV2	1708	741	0.05%	0.006%
96	13.085	3745	3746	3751	rVB5	1612	730	0.05%	0.006%
97	13.271	3802	3804	3807	rBV4	1470	891	0.06%	0.008%
98	13.397	3842	3843	3846	rBV3	1259	601	0.04%	0.005%
99	13.847	3974	3983	3988	rBV3	3339	5380	0.36%	0.047%
100	14.226	4099	4101	4105	rBV5	2213	1512	0.10%	0.013%




Sum of corrected areas: 11426449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032917.D
Acq On : 11 Nov 2023 01:48
Operator : SY/MD
Sample : VIBLK244
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

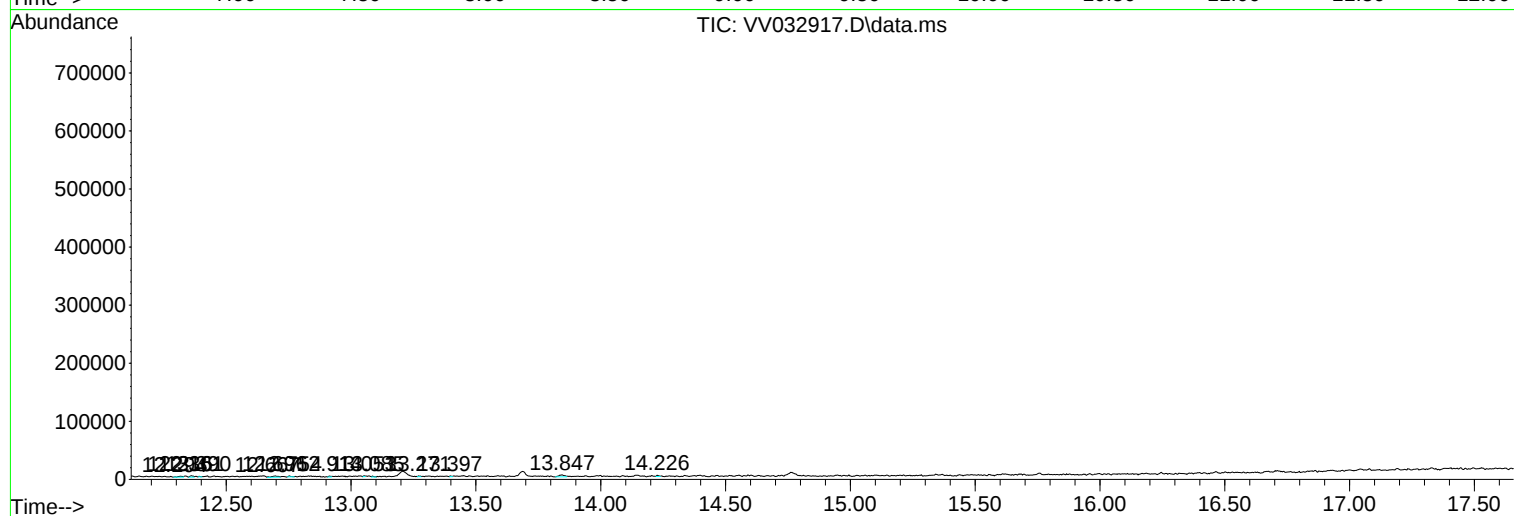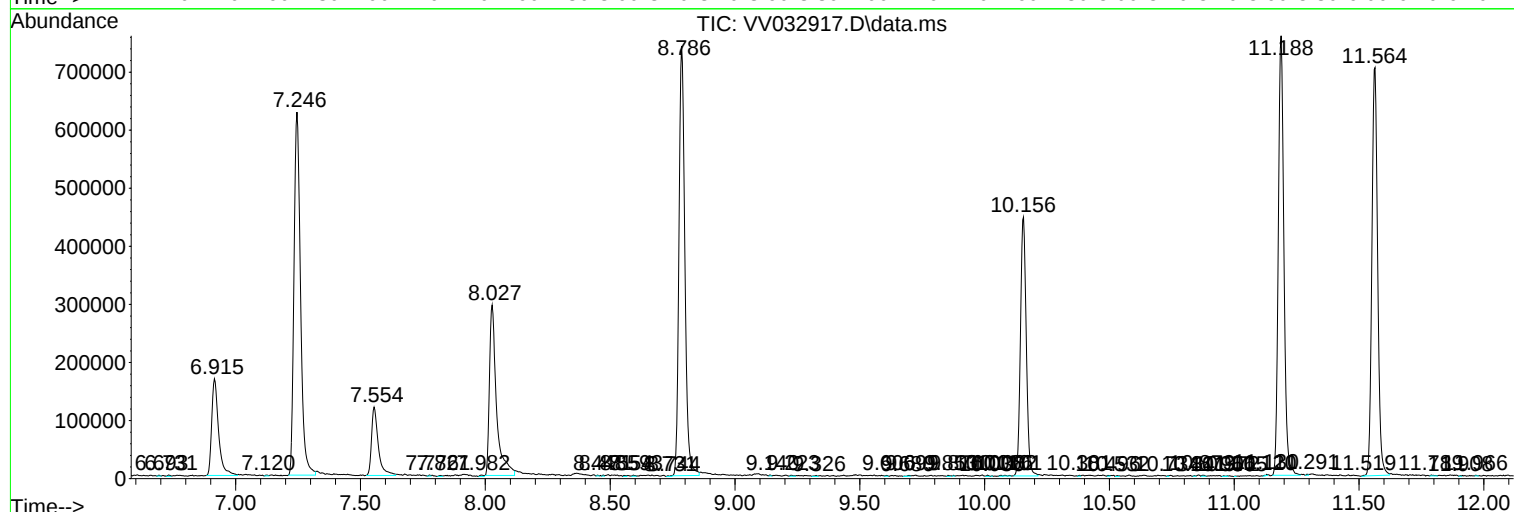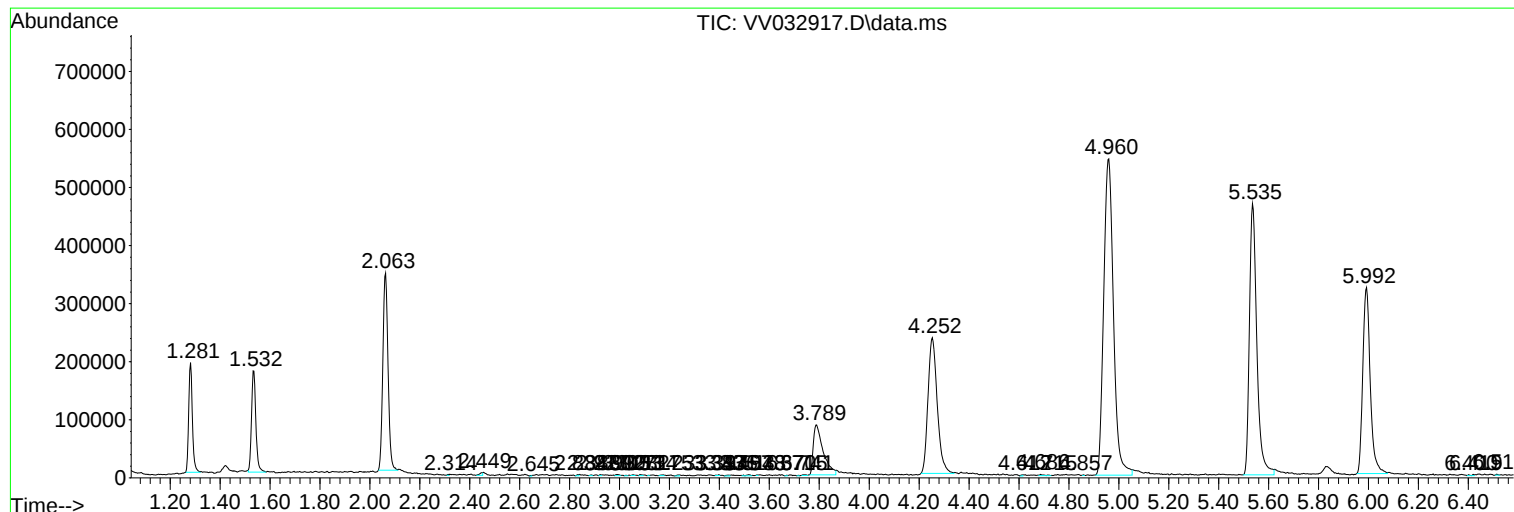

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032917.D
Acq On : 11 Nov 2023 01:48
Operator : SY/MD
Sample : VIBLK244
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032917.D
Acq On : 11 Nov 2023 01:48
Operator : SY/MD
Sample : VIBLK244
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc