
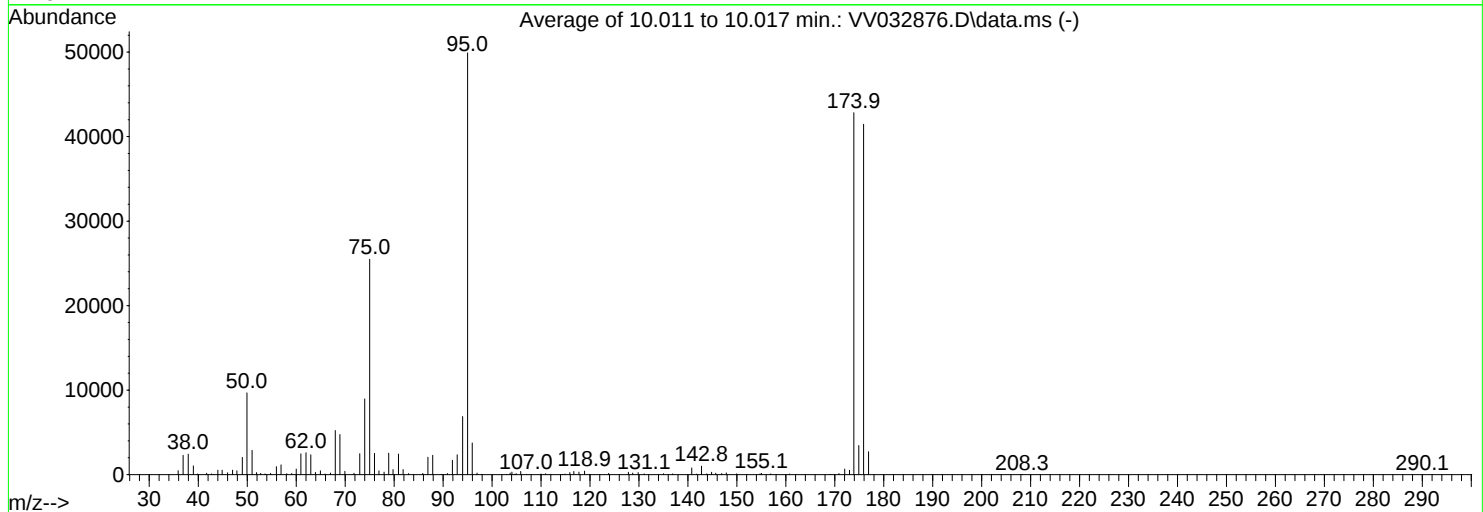


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032876.D
Acq On : 10 Nov 2023 07:38
Operator : SY/MD
Sample : BFB230
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB230

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Title : VOC Analysis
Last Update : Wed Nov 08 01:37:19 2023

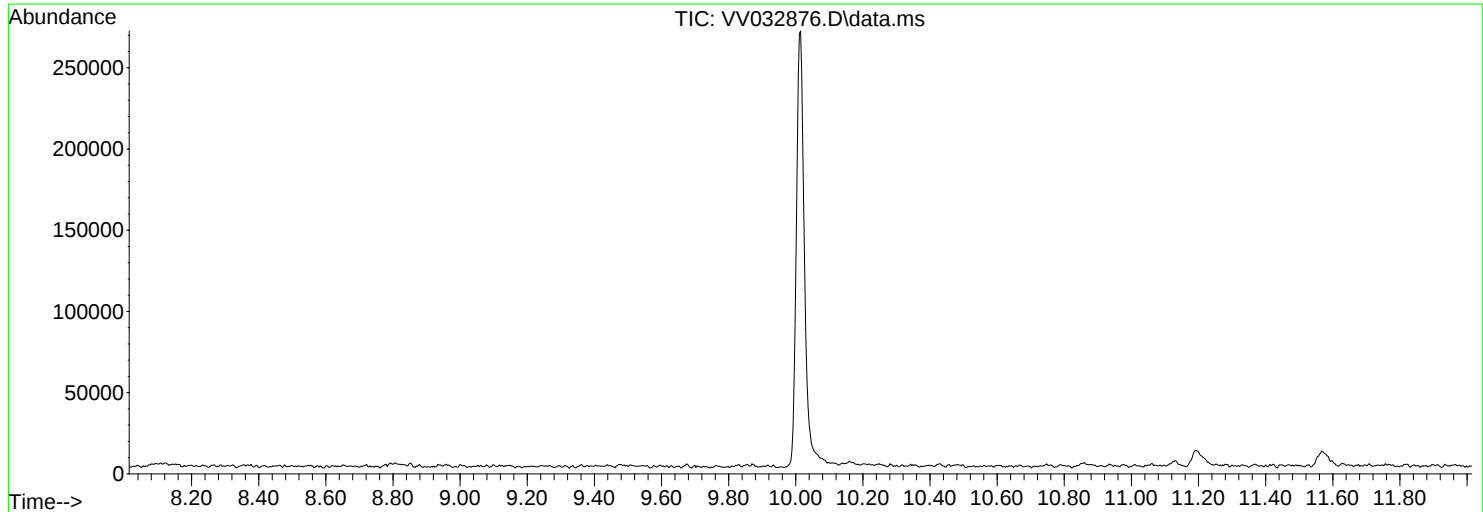

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	9678	PASS
75	95	30	80	51.1	25491	PASS
95	95	100	100	100.0	49912	PASS
96	95	5	9	7.5	3746	PASS
173	174	0.00	2	1.2	510	PASS
174	95	50	120	85.8	42837	PASS
175	174	5	9	8.0	3448	PASS
176	174	95	105	96.8	41469	PASS
177	176	5	10	6.5	2704	PASS

m/z	Abundance
35.20	131.0
35.90	154.0
36.80	133.0
37.60	192.0
38.40	237.0
39.00	137.0
40.00	236.0
40.60	113.0
41.30	186.0
42.30	128.0
43.20	118.0
44.10	350.0
45.30	140.0
46.30	125.0
49.00	117.0
49.80	119.0
50.30	155.0
54.20	100.0
54.80	139.0
56.80	132.0
57.10	128.0
61.10	126.0
63.90	129.0
68.60	125.0
69.70	104.0
71.70	134.0
76.50	144.0
83.20	114.0
91.00	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	714.0
37.00	2686.0
38.00	2505.0
39.00	1215.0
39.90	287.0
41.10	116.0
41.70	144.0
42.40	135.0
43.20	223.0
44.00	936.0
44.90	672.0
46.00	192.0
47.00	472.0
47.90	487.0
49.00	2250.0
50.00	9935.0
51.00	3008.0
51.90	248.0
52.70	161.0
54.90	329.0
56.00	1041.0
56.90	1428.0
58.10	107.0
59.10	139.0
60.00	637.0
61.00	2818.0
62.00	2806.0
63.00	2669.0
64.10	416.0
64.90	516.0
65.90	106.0
67.00	185.0
68.00	5536.0
69.00	5066.0
70.00	437.0
72.00	272.0
73.00	2657.0
74.00	9149.0
75.00	26896.0
76.00	2848.0
76.90	373.0
77.90	325.0
78.90	2550.0
79.80	616.0
80.90	2440.0
81.90	643.0
83.00	138.0
85.90	168.0
86.90	2098.0
87.90	2364.0
89.70	115.0
90.90	242.0
91.90	1727.0
92.90	2388.0
94.00	7366.0
95.00	51208.0
95.90	4021.0
96.90	122.0
104.00	305.0
105.00	156.0
105.80	388.0
107.00	113.0
111.00	100.0
115.90	291.0
116.70	379.0
117.80	312.0
118.90	411.0
123.80	158.0
127.80	311.0
128.90	155.0
129.80	289.0
135.00	193.0
136.90	164.0
140.70	806.0
142.80	1107.0
143.80	183.0
144.90	313.0
145.70	206.0
146.90	112.0
147.90	208.0
149.90	140.0
154.70	143.0
155.10	150.0
160.80	117.0
169.10	101.0
170.90	214.0
172.10	647.0
173.90	43776.0
174.90	3599.0
175.90	41520.0
176.90	2746.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	638.0
36.90	2473.0
37.90	2557.0
39.00	1204.0
39.90	336.0
41.20	142.0
41.70	171.0
42.70	133.0
43.30	262.0
44.00	892.0
44.90	523.0
46.00	225.0
47.00	545.0
47.90	467.0
49.00	2284.0
50.00	10230.0
51.00	2940.0
51.90	245.0
52.80	151.0
53.60	136.0
54.80	282.0
55.90	989.0
56.90	1449.0
58.10	116.0
59.10	127.0
60.00	705.0
61.00	2701.0
62.00	2635.0
63.00	2375.0
64.00	383.0
65.00	447.0
67.00	184.0
68.00	5398.0
69.00	4848.0
70.00	412.0
71.90	303.0
73.00	2555.0
74.00	9216.0
75.00	26304.0
76.00	2548.0
76.90	479.0
77.90	334.0
78.90	2658.0
79.80	613.0
80.90	2482.0
81.90	618.0
82.90	153.0
85.90	143.0
86.90	2054.0
87.90	2411.0
90.90	249.0
91.90	1741.0
92.90	2411.0
94.00	7068.0
95.00	51640.0
95.90	3928.0
96.90	189.0
103.70	305.0
104.00	308.0
104.90	161.0
105.90	391.0
110.00	114.0
110.90	115.0
114.90	110.0
115.90	234.0
116.70	401.0
117.80	296.0
118.90	437.0
123.90	164.0
127.90	301.0
128.70	197.0
129.80	241.0
131.10	115.0
135.00	134.0
136.90	145.0
140.80	808.0
141.70	107.0
142.80	1055.0
143.90	126.0
144.90	293.0
145.70	167.0
146.90	140.0
147.80	234.0
150.00	126.0
154.80	152.0
155.10	155.0
157.00	127.0
160.80	102.0
170.80	159.0
172.10	691.0
173.00	764.0
173.90	44208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

174.90	3584.0
175.90	42776.0
176.90	2797.0
208.30	103.0
290.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
35.90	518.0
36.90	2135.0
37.90	2202.0
39.00	1093.0
39.90	332.0
41.30	172.0
41.70	182.0
42.70	125.0
44.00	819.0
44.90	411.0
46.00	284.0
47.00	600.0
47.90	394.0
49.00	1972.0
50.00	9225.0
51.00	2663.0
51.90	273.0
52.80	166.0
53.70	139.0
54.70	242.0
55.90	833.0
56.90	1389.0
58.10	144.0
59.10	112.0
60.00	645.0
60.90	2270.0
62.00	2330.0
63.00	2008.0
63.90	364.0
65.00	427.0
65.90	110.0
67.00	211.0
68.00	4728.0
68.90	4321.0
69.90	357.0
71.80	331.0
73.00	2245.0
74.00	8497.0
75.00	23272.0
76.00	2158.0
76.90	538.0
78.00	266.0
78.90	2431.0
79.80	574.0
80.90	2430.0
81.80	532.0
82.90	122.0
84.00	126.0
85.80	124.0
86.90	2030.0
87.90	2117.0
90.90	212.0
91.90	1641.0
92.90	2227.0
94.00	6187.0
95.00	46888.0
96.00	3288.0
97.00	237.0
97.90	109.0
103.00	104.0
103.70	279.0
104.10	317.0
104.70	147.0
105.90	341.0
110.00	122.0
110.90	141.0
112.00	133.0
114.40	126.0
114.90	130.0
115.90	196.0
116.70	349.0
117.70	297.0
118.90	434.0
119.90	106.0
123.90	142.0
127.90	248.0
128.70	224.0
129.90	199.0
131.10	143.0
140.90	784.0
141.80	147.0
142.80	876.0
144.80	256.0
145.70	131.0
146.90	132.0
147.80	196.0
155.00	171.0
156.90	157.0
172.00	680.0
173.00	765.0
173.90	40528.0
174.90	3162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

175.9040112.0

176.902570.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230