


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV111119\
 Data File : VV013574.D
 Acq On : 11 Nov 2019 09:23
 Operator : SY/MD
 Sample : BFB58
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB58

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Nov 13 04:27:44 2019

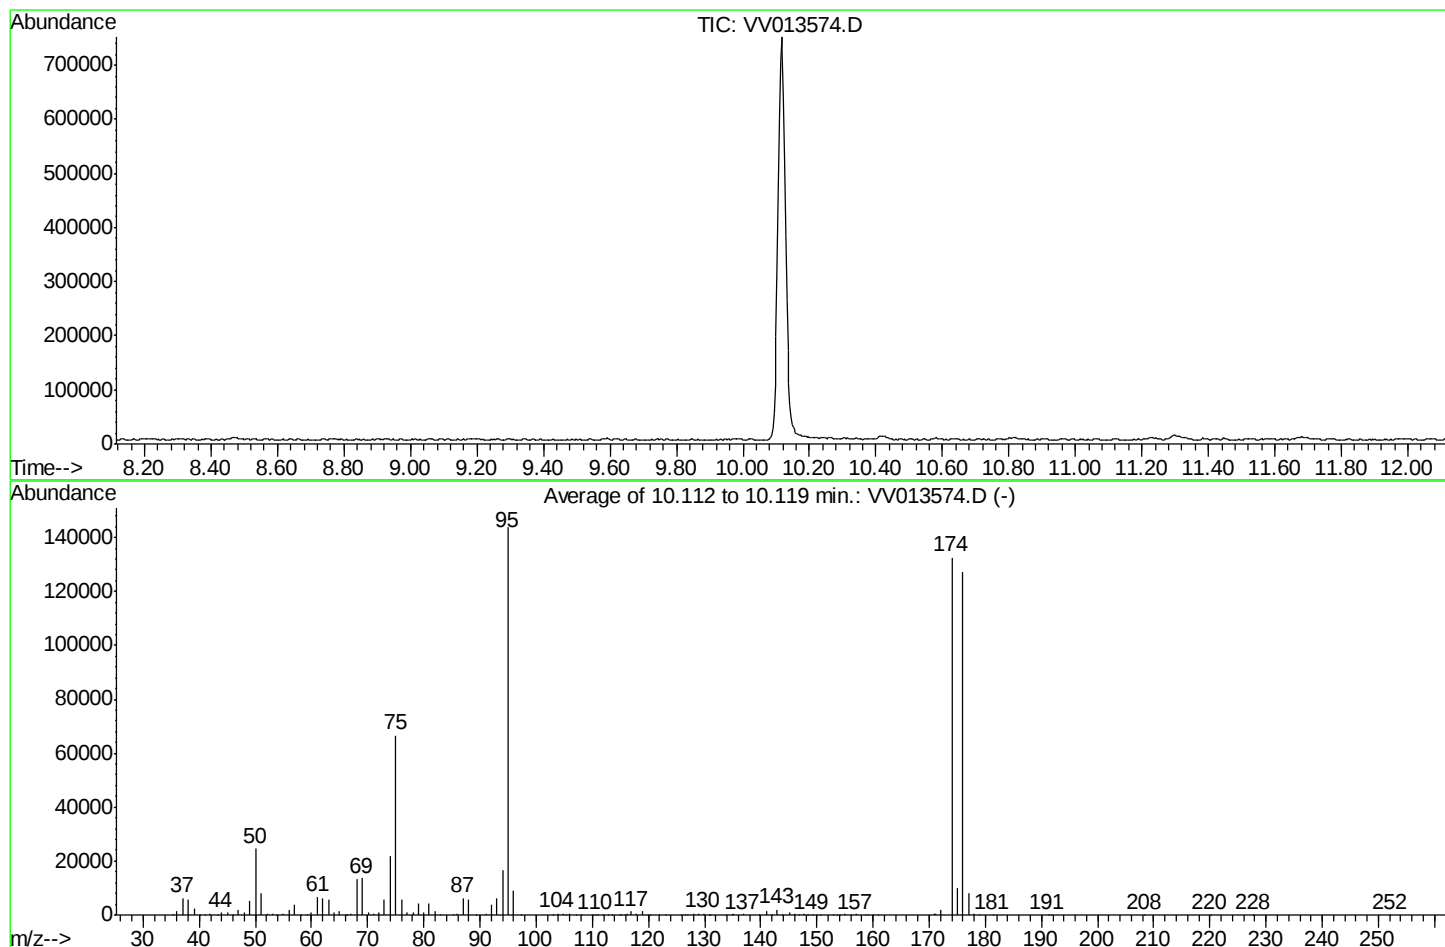

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	24534	PASS
75	95	30	80	46.4	66688	PASS
95	95	100	100	100.0	143786	PASS
96	95	5	9	6.3	9052	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.2	132602	PASS
175	174	5	9	7.4	9876	PASS
176	174	95	101	96.0	127250	PASS
177	176	5	9	6.4	8197	PASS

m/z	Abundance
35.20	123.0
36.00	1542.0
37.00	6087.0
38.10	6010.0
39.10	2563.0
40.00	1245.0
41.90	276.0
42.60	142.0
43.20	187.0
44.00	1871.0
45.00	1062.0
45.90	245.0
47.00	1823.0
47.90	965.0
49.00	5631.0
50.00	24536.0
51.00	7765.0
52.10	500.0
53.00	281.0
54.90	488.0
56.00	1912.0
57.00	3662.0
58.10	228.0
60.00	1214.0
61.10	7237.0
62.00	5872.0
63.00	5663.0
64.00	1134.0
65.00	1390.0
66.00	178.0
66.90	467.0
68.00	13081.0
69.00	13677.0
70.10	1271.0
71.00	259.0
71.90	735.0
73.00	5632.0
74.00	20960.0
75.00	65904.0
76.10	5657.0
77.10	890.0
78.00	808.0
79.00	4254.0
79.90	1196.0
80.90	4349.0
82.00	1226.0
83.00	124.0
85.20	101.0
86.00	372.0
87.00	5920.0
88.00	5733.0
91.10	579.0
92.00	3705.0
93.00	6125.0
94.00	16182.0
95.00	139520.0
96.00	9000.0
97.20	288.0
102.90	117.0
103.90	523.0
104.80	385.0
105.90	500.0
107.10	235.0
108.10	124.0
111.00	180.0
111.90	103.0
112.80	146.0
113.30	128.0
114.80	298.0
116.10	581.0
117.00	1309.0
117.80	487.0
118.90	1240.0
119.90	126.0
120.40	136.0
122.90	154.0
125.80	161.0
126.50	130.0
126.90	129.0
128.00	485.0
128.90	312.0
129.80	532.0
130.80	311.0
133.70	169.0
135.00	282.0
136.90	223.0
139.70	181.0
140.90	1507.0
141.90	226.0
142.90	2121.0
143.80	194.0
145.10	889.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

145.90	373.0
146.80	239.0
147.70	464.0
148.30	270.0
149.20	140.0
149.90	193.0
150.70	105.0
152.90	159.0
153.50	131.0
154.10	205.0
154.90	391.0
157.00	305.0
159.10	189.0
160.90	202.0
170.90	419.0
171.10	439.0
171.90	1673.0
174.00	127280.0
175.00	9582.0
176.00	120512.0
177.00	7848.0
178.10	271.0
181.40	119.0
191.10	114.0
191.60	108.0
208.30	108.0
220.10	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
36.00	1393.0
37.00	6436.0
38.10	5847.0
39.10	2559.0
40.00	1227.0
40.90	226.0
41.90	285.0
42.50	142.0
43.20	226.0
43.90	1773.0
45.00	1362.0
45.90	442.0
47.00	2030.0
47.90	1016.0
49.00	5783.0
50.00	25448.0
51.00	8230.0
52.10	459.0
53.00	335.0
55.00	540.0
56.00	1903.0
57.00	3775.0
58.10	248.0
59.20	104.0
60.00	1442.0
61.00	6971.0
62.10	6443.0
63.00	5978.0
63.90	1197.0
65.00	1315.0
66.00	177.0
66.90	476.0
68.00	13655.0
69.10	14218.0
70.10	1185.0
71.00	287.0
71.90	845.0
73.00	6251.0
74.00	22864.0
75.00	68824.0
76.10	5693.0
77.00	920.0
78.10	876.0
79.00	4313.0
80.00	1234.0
80.90	4717.0
82.00	1303.0
83.00	201.0
85.90	353.0
87.00	6486.0
88.00	6198.0
89.20	107.0
91.10	626.0
92.00	3956.0
93.00	6646.0
94.00	17384.0
95.00	148544.0
96.00	9325.0
97.20	396.0
102.90	158.0
103.80	557.0
104.80	325.0
105.90	534.0
107.00	244.0
108.10	135.0
110.00	104.0
110.60	140.0
111.10	198.0
112.70	162.0
113.30	113.0
114.90	262.0
116.10	626.0
117.00	1348.0
117.80	585.0
118.90	1351.0
119.80	132.0
121.90	127.0
123.00	132.0
125.80	172.0
126.90	156.0
128.00	498.0
128.90	270.0
129.80	579.0
130.80	318.0
133.70	118.0
135.00	284.0
135.10	286.0
136.90	305.0
139.80	160.0
140.90	1661.0
141.90	206.0
142.90	2144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

143.80	184.0
145.10	949.0
146.00	397.0
146.80	220.0
147.70	455.0
149.20	157.0
149.90	127.0
150.70	164.0
152.90	120.0
154.10	194.0
154.90	332.0
156.00	107.0
156.90	342.0
158.60	147.0
159.20	168.0
161.00	237.0
171.00	551.0
171.90	1800.0
174.00	137024.0
175.00	10213.0
176.00	131024.0
177.00	8562.0
178.00	295.0
179.00	103.0
191.10	113.0
208.40	184.0
227.70	145.0
252.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
35.30	104.0
36.00	1308.0
37.00	6055.0
38.10	5491.0
39.10	2438.0
40.00	1131.0
40.90	212.0
41.90	243.0
43.20	239.0
43.90	1612.0
45.00	1495.0
45.90	531.0
47.00	1941.0
48.00	960.0
49.00	5340.0
50.00	23936.0
51.00	8021.0
52.10	390.0
53.00	304.0
53.80	116.0
55.10	529.0
56.00	1642.0
57.00	3542.0
58.10	255.0
59.20	118.0
60.00	1435.0
61.00	6145.0
62.10	6154.0
63.00	5500.0
63.90	1181.0
65.00	1229.0
66.20	187.0
66.90	503.0
68.00	12809.0
69.10	13448.0
70.10	940.0
71.00	256.0
71.90	798.0
73.00	6244.0
74.00	22448.0
75.00	65336.0
76.00	5553.0
76.90	960.0
78.10	761.0
79.00	4075.0
80.00	1168.0
80.90	4507.0
82.00	1197.0
83.00	245.0
85.80	353.0
87.00	6527.0
88.00	5840.0
90.90	597.0
92.00	4010.0
93.10	6157.0
94.00	16400.0
95.00	143296.0
96.00	8832.0
97.20	429.0
102.90	152.0
103.80	570.0
104.70	304.0
105.20	240.0
106.00	544.0
107.00	257.0
108.10	154.0
109.90	108.0
110.60	144.0
111.10	176.0
112.70	162.0
113.40	102.0
115.10	206.0
115.80	588.0
116.90	1349.0
117.80	625.0
118.90	1241.0
119.80	103.0
121.80	132.0
125.90	142.0
126.90	152.0
128.10	452.0
129.00	229.0
129.90	496.0
131.00	319.0
134.80	291.0
136.90	322.0
141.00	1565.0
141.90	198.0
142.90	2082.0
145.00	815.0
146.00	350.0
146.80	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

147.80	455.0
149.10	166.0
150.70	162.0
152.90	121.0
154.00	162.0
154.90	252.0
156.00	105.0
156.80	347.0
158.60	186.0
159.20	170.0
160.00	128.0
160.90	233.0
170.90	608.0
172.00	1846.0
174.00	133504.0
175.00	9834.0
176.00	130216.0
176.90	8181.0
178.00	298.0
208.40	186.0
227.70	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
35.60	209.0
36.10	121.0
37.30	123.0
38.70	209.0
40.00	1179.0
41.40	148.0
42.70	153.0
43.90	995.0
45.20	120.0
46.10	155.0
47.60	135.0
48.10	167.0
48.90	134.0
50.20	106.0
51.30	102.0
54.90	170.0
60.00	206.0
60.70	159.0
61.50	133.0
62.00	121.0
64.10	178.0
65.60	133.0
67.00	140.0
67.70	157.0
68.90	150.0
73.00	181.0
77.10	112.0
79.70	108.0
85.50	141.0
97.30	129.0
102.10	133.0
124.90	103.0
130.20	146.0
131.30	144.0
189.10	102.0
194.90	103.0
206.80	140.0
234.70	109.0
252.90	103.0
286.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58