
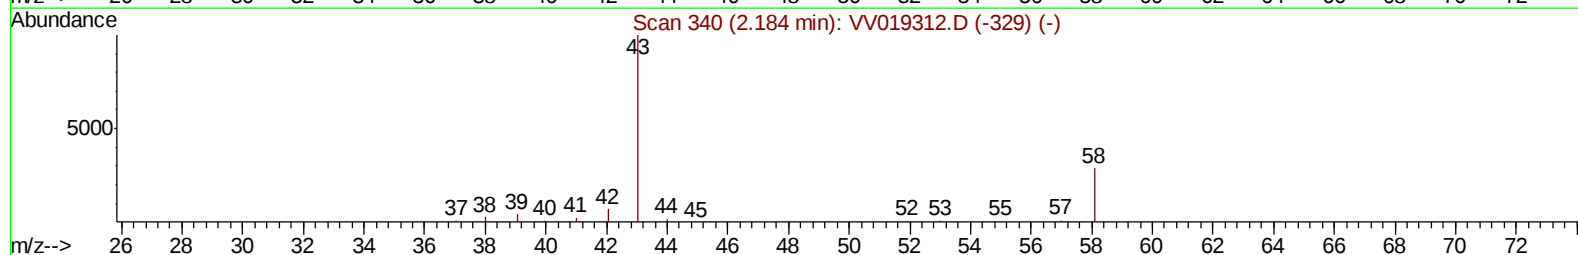
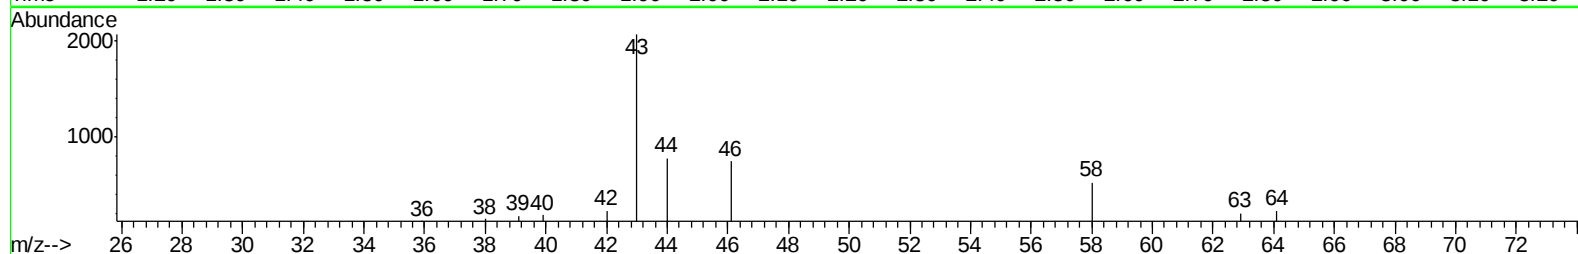


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111120\
 Data File : VV019337.D
 Acq On : 11 Nov 2020 14:14
 Operator : SY/MD
 Sample : L4693-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Nov 12 00:49:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 12 00:41:49 2020
 Response via : Initial Calibration

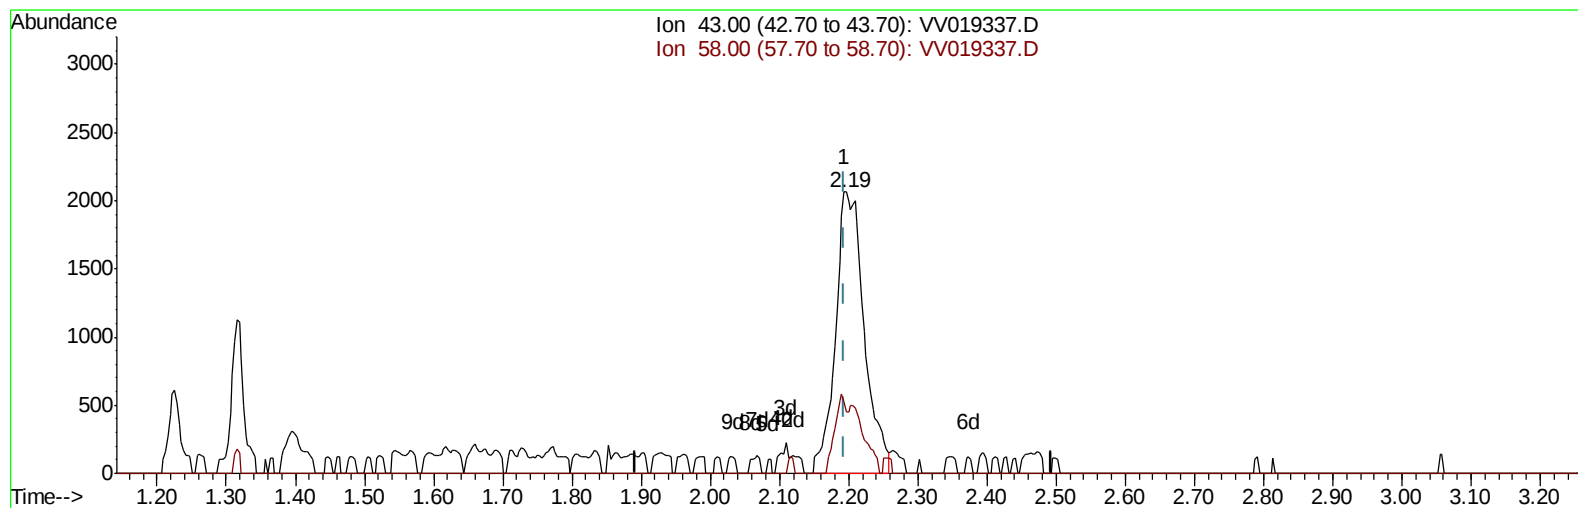

TIC: VV019337.D

(13) Acetone (T)

2.193min (-0.000) 5.05ug/L m

response 5962

Ion	Exp%	Act%
43.00	100	100
58.00	29.70	12.50
0.00	0.00	0.00
0.00	0.00	0.00