

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111120\
 Data File : VV019337.D
 Acq On : 11 Nov 2020 14:14
 Operator : SY/MD
 Sample : L4693-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4C8

Manual Integrations
 APPROVED

MMDadoda
 11/16/2020 2:26:34 PM

Quant Time: Nov 12 00:49:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 12 00:41:49 2020
 Response via : Initial Calibration

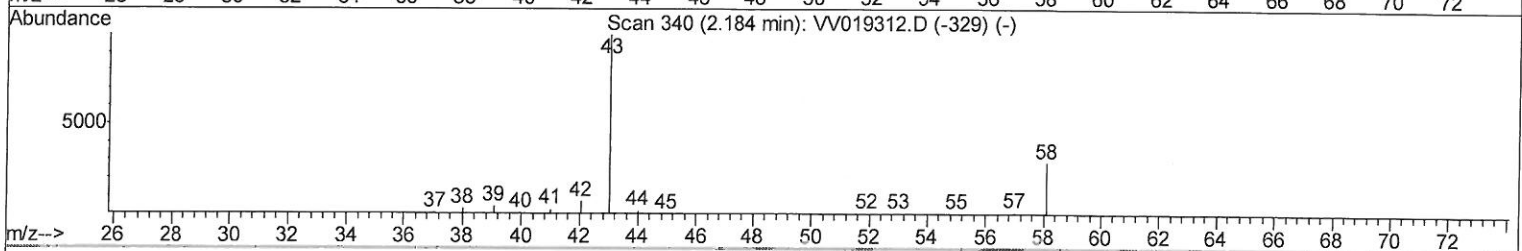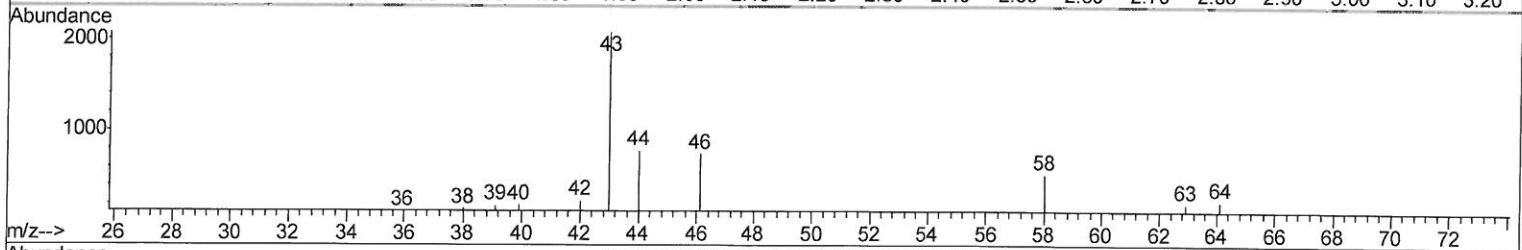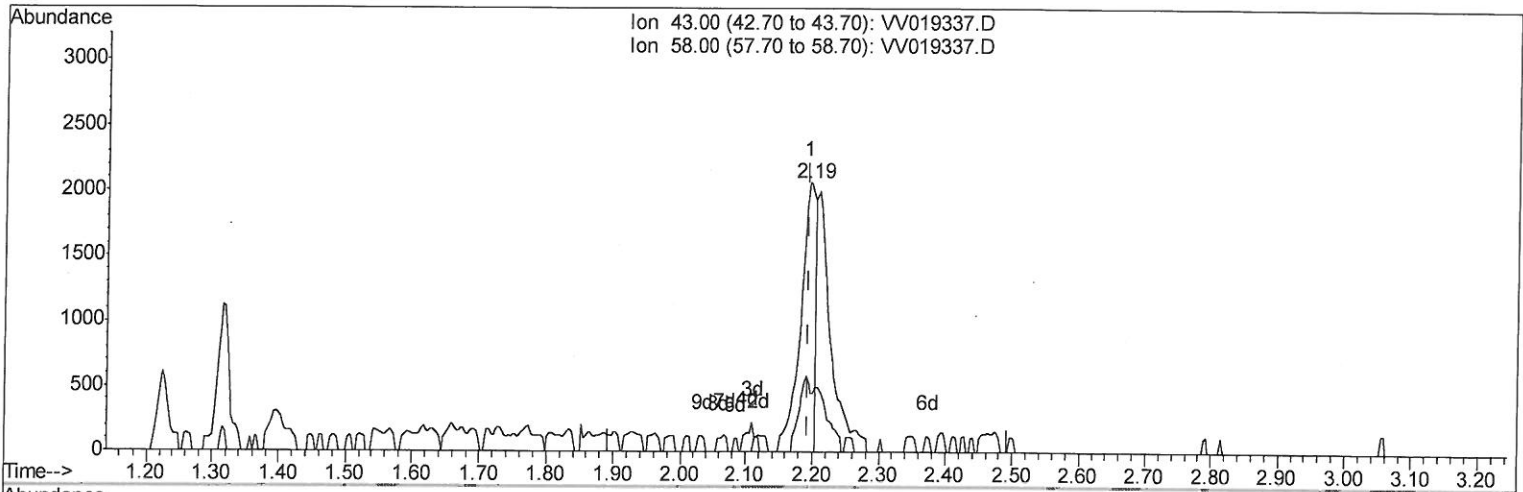

TIC: VV019337.D

(13) Acetone (T)

2.193min (-0.000) 2.71ug/L

response 3199

Ion	Exp%	Act%
43.00	100	100
58.00	29.70	23.29
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111120\
 Data File : VV019337.D
 Acq On : 11 Nov 2020 14:14
 Operator : SY/MD
 Sample : L4693-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4C8

Manual Integrations
 APPROVED

MMDadoda
 11/16/2020 2:26:34 PM

Quant Time: Nov 12 00:49:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 12 00:41:49 2020
 Response via : Initial Calibration

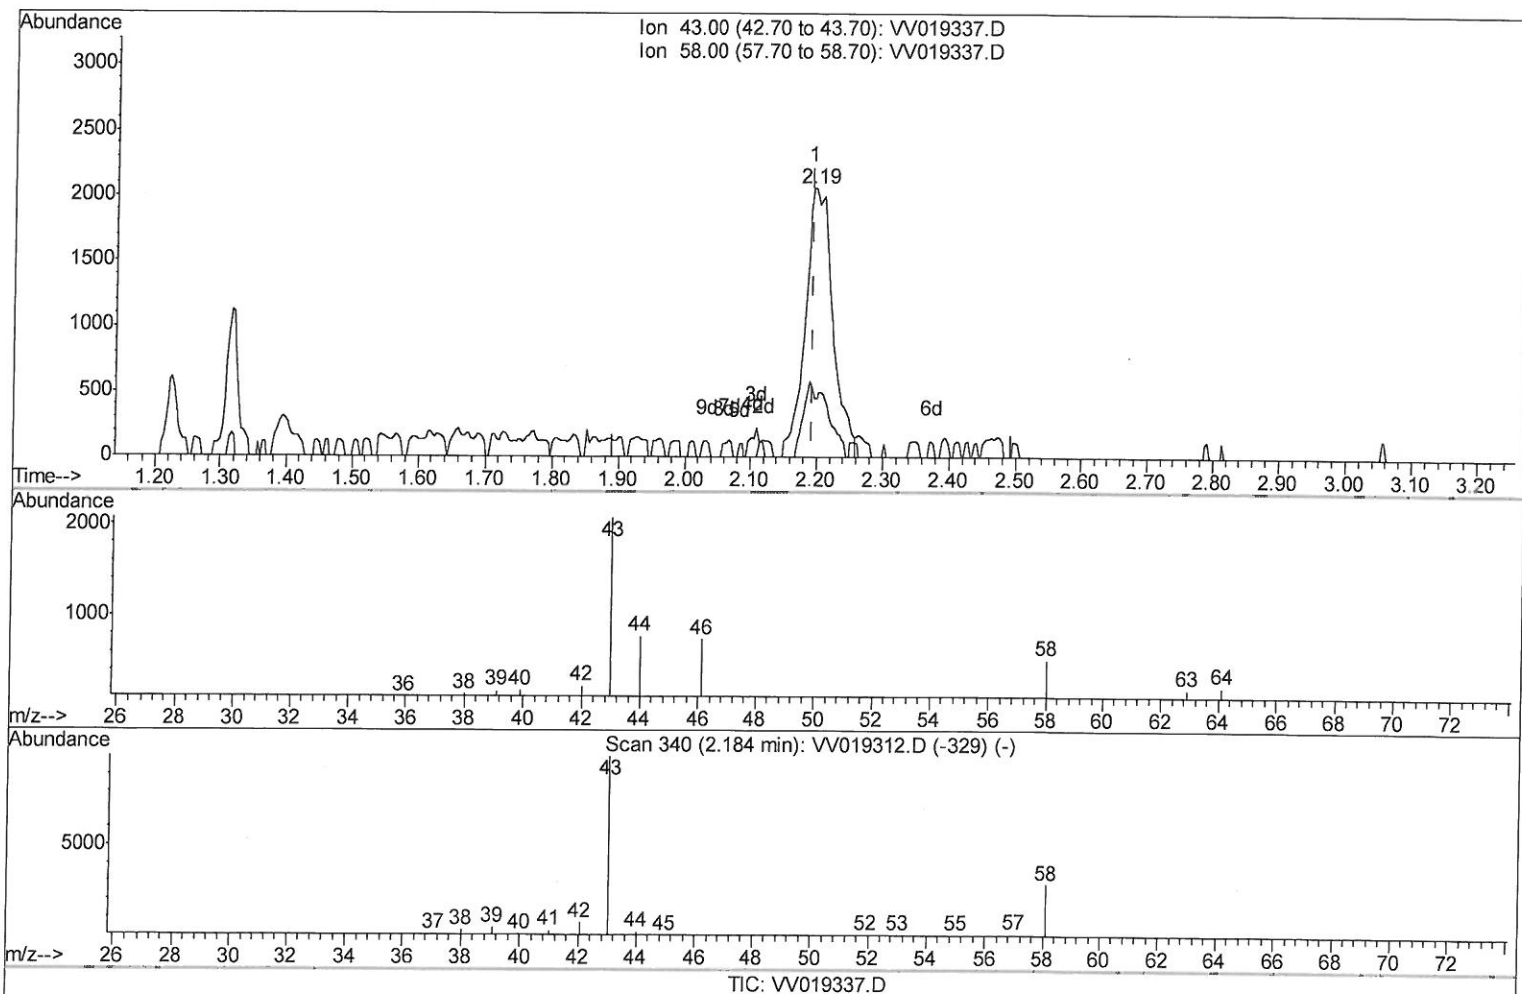

(13) Acetone (T)

2.193min (-0.000) 5.05ug/L m

response 5962

Ion	Exp%	Act%
43.00	100	100
58.00	29.70	12.50
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111120\
 Data File : VV019337.D
 Acq On : 11 Nov 2020 14:14
 Operator : SY/MD
 Sample : L4693-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4C8

Manual Integrations
 APPROVED

MMDadoda
 11/16/2020 2:26:34 PM

Quant Time: Nov 12 01:26:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 12 00:41:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	260909	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	255775	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	123174	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	106671	51.45	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	102.90%		
7) Chloroethane-d5	1.58	69	86036	53.41	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	106.82%		
11) 1,1-Dichloroethene-d2	2.12	63	152841	38.75	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.50%		
21) 2-Butanone-d5	3.92	46	119825	94.36	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	94.36%		
24) Chloroform-d	4.38	84	178617	46.31	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.62%		
26) 1,2-Dichloroethane-d4	5.06	65	123729	46.04	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.08%		
32) Benzene-d6	5.07	84	343987	47.41	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.82%		
36) 1,2-Dichloropropane-d6	6.09	67	108327	50.07	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.14%		
41) Toluene-d8	7.34	98	304871	43.74	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.48%		
43) trans-1,3-Dichloropropene-	7.64	79	52575	42.00	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.00%		
47) 2-Hexanone-d5	8.11	63	68480	73.09	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	73.09%		
57) 1,1,2,2-Tetrachloroethane-	10.23	84	120997	41.48	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.96%		
64) 1,2-Dichlorobenzene-d4	11.65	152	125546	48.51	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.02%		
Target Compounds						
13) Acetone	2.19	43	5962m	5.053	ug/L	Ovalue
48) 2-Hexanone	8.16	43	8064	4.016	ug/L	# 65

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111120\
Data File : VV019337.D
Acq On : 11 Nov 2020 14:14
Operator : SY/MD
Sample : L4693-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4C8

Manual Integrations
APPROVED

MMDadoda
11/16/2020 2:26:34 PM

Quant Time: Nov 12 01:26:39 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 12 00:41:49 2020
Response via : Initial Calibration

