

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111120\
 Data File : VV019334.D
 Acq On : 11 Nov 2020 11:14
 Operator : SY/MD
 Sample : L4659-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	182863	183625	16.59%	2.239%
2	1.579	144	152	165	rBV	152549	169866	15.35%	2.071%
3	2.123	310	321	348	rVB	294594	445041	40.21%	5.427%
4	2.373	396	399	403	rVB2	366	285	0.03%	0.003%
5	2.434	414	418	421	rVB2	333	262	0.02%	0.003%
6	2.454	421	424	426	rBV	293	136	0.01%	0.002%
7	2.489	432	435	438	rBV2	224	161	0.01%	0.002%
8	2.528	443	447	455	rVB3	881	989	0.09%	0.012%
9	2.637	479	481	484	rVB3	189	103	0.01%	0.001%
10	2.717	500	506	512	rBV2	239	371	0.03%	0.005%
11	2.859	548	550	557	rVB2	196	96	0.01%	0.001%
12	3.020	597	600	602	rBV2	161	102	0.01%	0.001%
13	3.155	640	642	646	rBV	188	108	0.01%	0.001%
14	3.177	646	649	651	rVV2	168	101	0.01%	0.001%
15	3.190	651	653	656	rVV	116	67	0.01%	0.001%
16	3.251	667	672	673	rBV	148	113	0.01%	0.001%
17	3.286	681	683	685	rVB2	158	42	0.00%	0.001%
18	3.299	685	687	689	rVB	63	25	0.00%	0.000%
19	3.315	689	692	693	rBV	75	44	0.00%	0.001%
20	3.389	710	715	717	rBV	270	201	0.02%	0.002%
21	3.476	739	742	747	rBV2	181	180	0.02%	0.002%
22	3.499	747	749	754	rVB2	140	102	0.01%	0.001%
23	3.524	754	757	759	rBV	148	100	0.01%	0.001%
24	3.540	759	762	765	rVV	261	147	0.01%	0.002%
25	3.553	765	766	771	rVB	198	85	0.01%	0.001%
26	3.576	771	773	775	rBV2	80	41	0.00%	0.000%
27	3.637	791	792	793	rVB	208	40	0.00%	0.000%
28	3.685	804	807	810	rVB	155	91	0.01%	0.001%
29	3.740	821	824	825	rBV	81	46	0.00%	0.001%
30	3.913	867	878	912	rBV	71253	214977	19.42%	2.622%
31	4.315	1000	1003	1005	rBV2	303	186	0.02%	0.002%
32	4.376	1005	1022	1049	rBV	180290	443626	40.08%	5.410%
33	4.640	1102	1104	1111	rVB3	233	181	0.02%	0.002%
34	4.669	1111	1113	1114	rBV3	191	86	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111120\
 Data File : VV019334.D
 Acq On : 11 Nov 2020 11:14
 Operator : SY/MD
 Sample : L4659-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	4.714	1124	1127	1129	rBV	292	170	0.02%	0.002%
36	4.740	1132	1135	1137	rBV	149	112	0.01%	0.001%
37	4.807	1154	1156	1159	rBV2	190	101	0.01%	0.001%
38	4.865	1171	1174	1176	rBV2	79	59	0.01%	0.001%
39	4.897	1180	1184	1186	rBV	271	162	0.01%	0.002%
40	4.913	1186	1189	1195	rVB2	300	219	0.02%	0.003%
41	4.942	1195	1198	1199	rBV2	177	100	0.01%	0.001%
42	4.955	1199	1202	1205	rVB	176	98	0.01%	0.001%
43	5.016	1217	1221	1222	rBV	385	248	0.02%	0.003%
44	5.071	1222	1238	1276	rVV2	429964	1106876	100.00%	13.498%
45	5.505	1366	1373	1377	rBV2	244	256	0.02%	0.003%
46	5.550	1384	1387	1391	rVB3	234	168	0.02%	0.002%
47	5.598	1400	1402	1403	rVB	158	58	0.01%	0.001%
48	5.640	1403	1415	1444	rBV	309653	619158	55.94%	7.550%
49	5.926	1493	1504	1522	rBV3	19592	42286	3.82%	0.516%
50	6.029	1534	1536	1539	rVB	258	91	0.01%	0.001%
51	6.093	1542	1556	1578	rBV	247858	501748	45.33%	6.119%
52	6.376	1641	1644	1647	rBV	167	136	0.01%	0.002%
53	6.405	1651	1653	1656	rVV2	146	84	0.01%	0.001%
54	6.421	1656	1658	1663	rVB2	236	154	0.01%	0.002%
55	6.460	1667	1670	1672	rBV	120	85	0.01%	0.001%
56	6.643	1726	1727	1728	rBV	95	22	0.00%	0.000%
57	6.656	1728	1731	1733	rBV2	312	231	0.02%	0.003%
58	6.685	1739	1740	1741	rBV2	136	43	0.00%	0.001%
59	6.714	1746	1749	1751	rBV	175	118	0.01%	0.001%
60	7.007	1829	1840	1864	rBV	133958	244997	22.13%	2.988%
61	7.199	1897	1900	1903	rBV3	453	288	0.03%	0.004%
62	7.267	1919	1921	1926	rBV2	379	299	0.03%	0.004%
63	7.338	1931	1943	1962	rBV	497693	850061	76.80%	10.366%
64	7.592	2017	2022	2026	rBV3	474	482	0.04%	0.006%
65	7.643	2028	2038	2063	rVV2	95641	169836	15.34%	2.071%
66	7.884	2111	2113	2114	rBV2	203	97	0.01%	0.001%
67	7.917	2121	2123	2126	rBV	226	112	0.01%	0.001%
68	7.994	2145	2147	2152	rBV2	249	225	0.02%	0.003%
69	8.029	2155	2158	2160	rBV2	215	129	0.01%	0.002%
70	8.109	2172	2183	2218	rBV2	232883	457966	41.37%	5.585%
71	8.479	2296	2298	2303	rVB2	296	213	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111120\
 Data File : VV019334.D
 Acq On : 11 Nov 2020 11:14
 Operator : SY/MD
 Sample : L4659-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	8.505	2303	2306	2311	rBV	362	321	0.03%	0.004%
73	8.592	2331	2333	2337	rVB	320	129	0.01%	0.002%
74	8.614	2337	2340	2342	rBV	287	219	0.02%	0.003%
75	8.675	2357	2359	2362	rVB2	165	72	0.01%	0.001%
76	8.826	2403	2406	2407	rBV	220	106	0.01%	0.001%
77	8.871	2409	2420	2446	rBV	482278	777081	70.20%	9.476%
78	9.238	2531	2534	2537	rBV2	331	184	0.02%	0.002%
79	9.267	2540	2543	2544	rBV	226	114	0.01%	0.001%
80	9.769	2697	2699	2702	rBV2	194	121	0.01%	0.001%
81	9.846	2721	2723	2728	rBV2	246	158	0.01%	0.002%
82	10.006	2769	2773	2776	rBV	190	189	0.02%	0.002%
83	10.151	2813	2818	2823	rVB3	722	682	0.06%	0.008%
84	10.235	2832	2844	2866	rBV	283620	448024	40.48%	5.464%
85	10.334	2872	2875	2880	rBV2	298	290	0.03%	0.004%
86	10.357	2880	2882	2883	rBV2	208	85	0.01%	0.001%
87	10.936	3058	3062	3068	rVB2	776	901	0.08%	0.011%
88	11.270	3154	3166	3192	rBV	475956	730672	66.01%	8.910%
89	11.646	3271	3283	3305	rBV	495770	781030	70.56%	9.524%
90	11.968	3378	3383	3385	rBV2	350	325	0.03%	0.004%
91	13.547	3872	3874	3876	rBV2	481	193	0.02%	0.002%
92	13.588	3883	3887	3889	rBV2	323	277	0.03%	0.003%


Sum of corrected areas: 8200287

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111120\
Data File : VV019334.D
Acq On : 11 Nov 2020 11:14
Operator : SY/MD
Sample : L4659-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

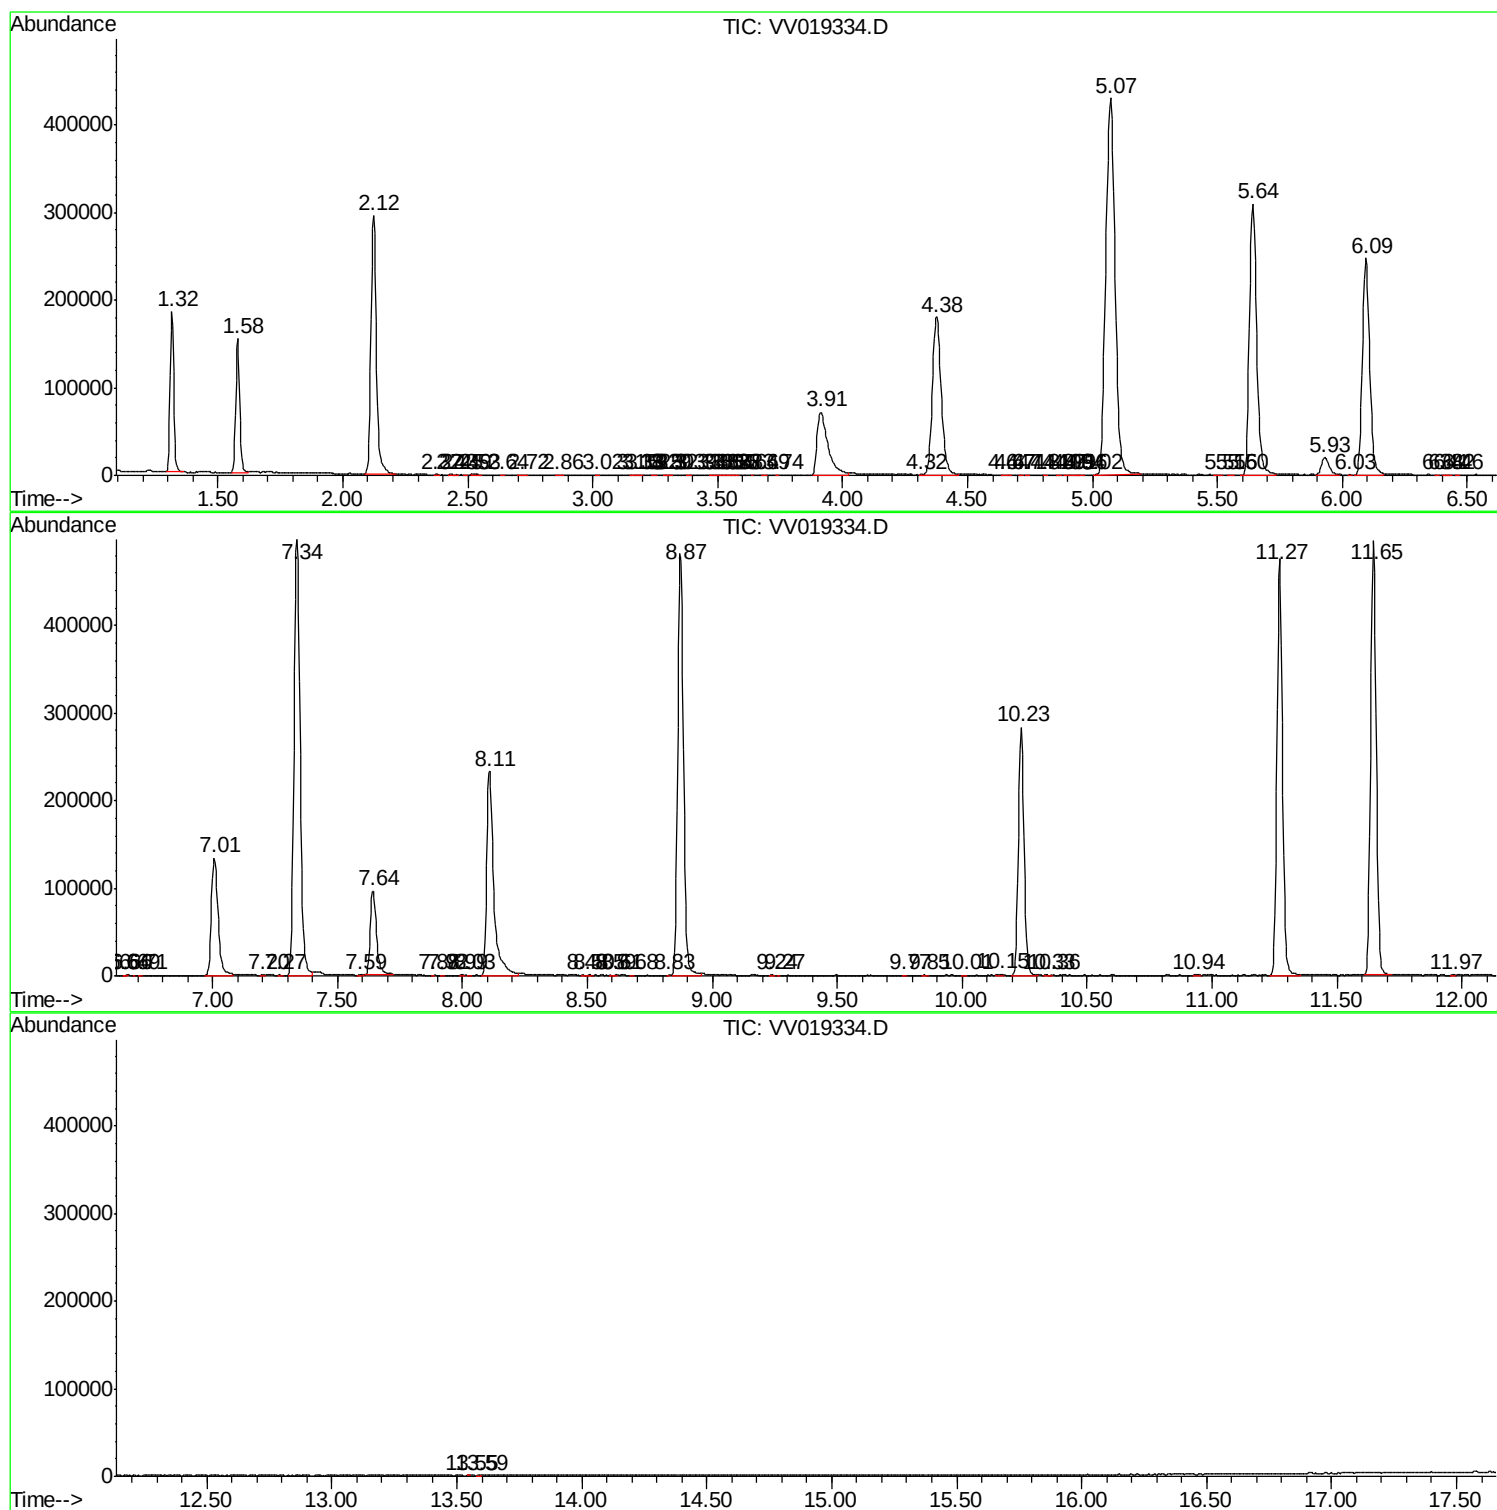

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV111120\
Data File : VV019334.D
Acq On : 11 Nov 2020 11:14
Operator : SY/MD
Sample : L4659-21
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111120\
Data File : VV019334.D
Acq On : 11 Nov 2020 11:14
Operator : SY/MD
Sample : L4659-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc