


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV111120\
 Data File : VV019330.D
 Acq On : 11 Nov 2020 08:46
 Operator : SY/MD
 Sample : BFB92
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB92

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis
 Last Update : Thu Nov 12 00:51:38 2020

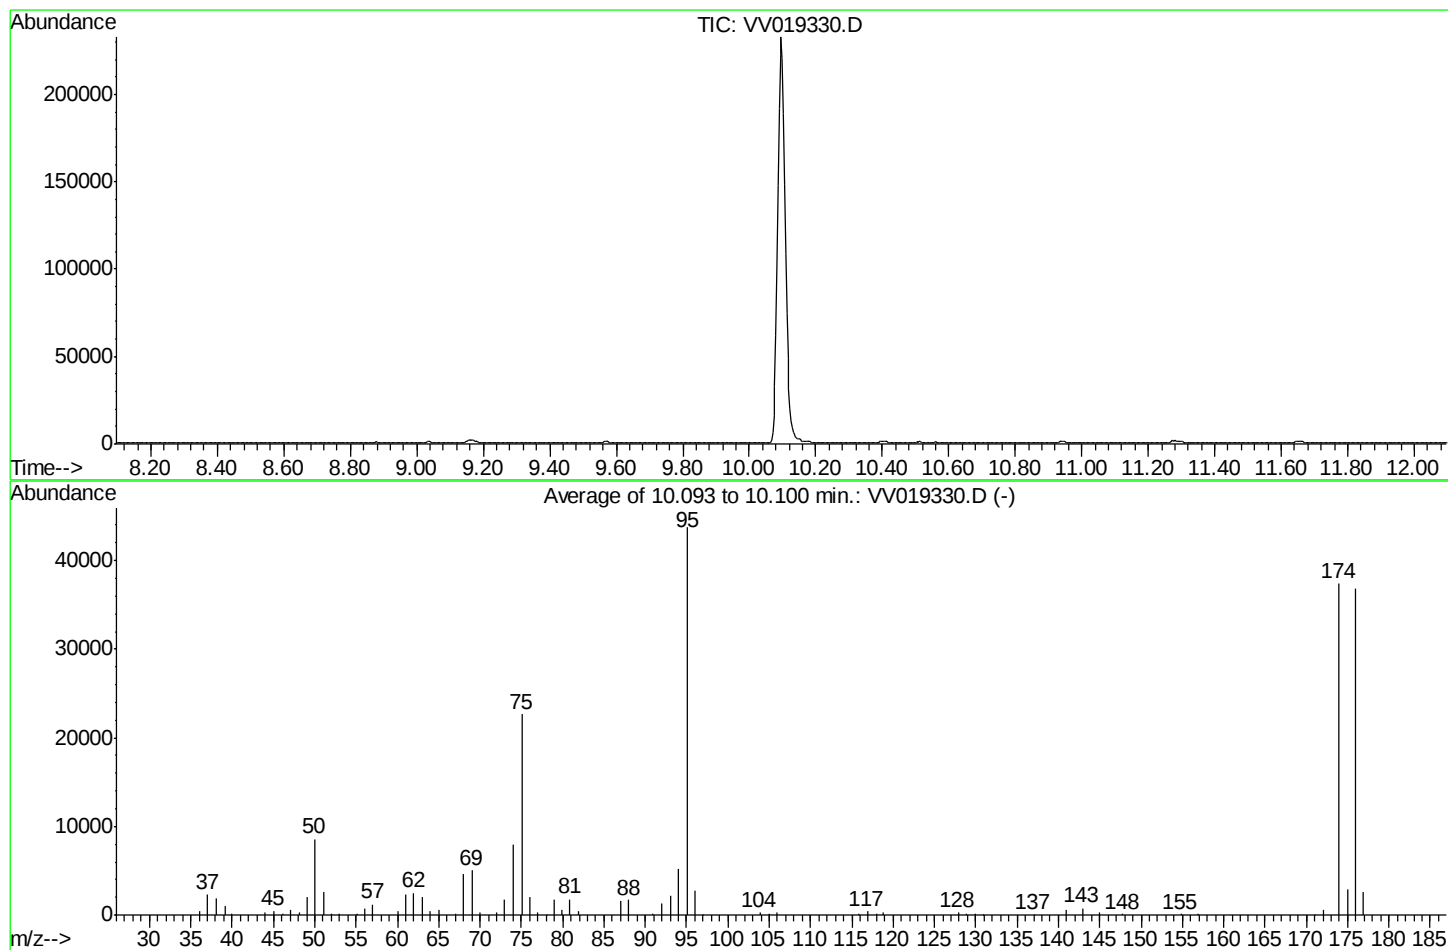

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	8584	PASS
75	95	30	80	51.8	22669	PASS
95	95	100	100	100.0	43757	PASS
96	95	5	9	6.3	2769	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.5	37413	PASS
175	174	5	9	7.8	2918	PASS
176	174	95	101	98.5	36842	PASS
177	176	5	9	6.9	2556	PASS

m/z	Abundance
36.00	449.0
37.00	2227.0
38.10	1990.0
39.10	1091.0
40.00	326.0
44.00	717.0
45.00	488.0
46.10	142.0
47.10	606.0
48.00	306.0
49.00	2083.0
50.00	8580.0
51.10	2728.0
52.10	181.0
55.10	163.0
56.00	685.0
57.00	1161.0
60.00	473.0
61.00	2269.0
62.00	2465.0
63.10	2005.0
64.00	397.0
65.00	569.0
66.90	153.0
68.00	4572.0
69.00	4876.0
70.00	391.0
71.90	281.0
73.00	1747.0
74.00	7892.0
75.10	22872.0
76.00	2088.0
77.00	318.0
78.90	1736.0
79.90	585.0
80.90	1801.0
81.90	534.0
87.00	1703.0
88.00	1715.0
90.90	238.0
92.00	1304.0
93.00	2091.0
94.00	5102.0
95.10	43616.0
96.00	2766.0
97.00	103.0
103.90	254.0
104.90	127.0
105.90	197.0
115.80	206.0
116.90	393.0
118.00	205.0
118.90	333.0
127.90	266.0
128.90	139.0
129.90	172.0
130.90	118.0
140.90	474.0
142.90	724.0
145.00	364.0
147.80	117.0
154.80	113.0
156.90	112.0
172.00	455.0
174.00	36232.0
175.00	2923.0
176.00	35688.0
176.90	2559.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
36.00	467.0
37.00	2349.0
38.10	2022.0
39.10	1098.0
40.00	331.0
44.00	684.0
45.00	471.0
46.10	162.0
47.10	617.0
48.10	284.0
49.00	2117.0
50.00	8860.0
51.10	2680.0
52.00	215.0
52.90	125.0
55.10	128.0
56.00	729.0
57.00	1250.0
60.00	449.0
61.00	2422.0
62.00	2576.0
63.10	2096.0
64.00	388.0
65.00	618.0
67.00	156.0
68.00	4828.0
69.00	5165.0
70.00	341.0
72.00	297.0
73.00	1810.0
74.00	8203.0
75.10	23424.0
76.00	2051.0
77.00	309.0
78.90	1871.0
79.90	648.0
80.90	1805.0
81.90	500.0
87.00	1709.0
88.00	1780.0
90.90	221.0
92.00	1305.0
93.00	2277.0
94.00	5345.0
95.10	45280.0
96.00	2899.0
97.00	113.0
103.90	236.0
105.00	139.0
105.90	238.0
115.80	230.0
116.90	429.0
118.00	234.0
118.80	335.0
127.90	233.0
128.90	152.0
129.90	199.0
140.90	595.0
142.90	769.0
145.00	352.0
147.80	119.0
154.90	125.0
157.00	106.0
172.00	535.0
174.00	38664.0
175.00	3044.0
176.00	38064.0
176.90	2630.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
36.00	463.0
37.00	2262.0
38.10	1807.0
39.10	1001.0
40.00	307.0
44.00	680.0
45.00	386.0
46.10	166.0
47.00	559.0
48.20	222.0
49.00	1849.0
50.00	8313.0
51.00	2384.0
52.00	202.0
53.00	151.0
56.00	696.0
57.00	1183.0
60.00	369.0
61.00	2283.0
62.00	2376.0
63.00	1993.0
64.00	318.0
65.00	562.0
67.10	151.0
68.00	4494.0
69.00	4976.0
70.00	298.0
72.00	268.0
73.00	1745.0
74.00	7563.0
75.10	21712.0
76.00	1830.0
77.00	248.0
78.10	164.0
78.90	1827.0
79.90	667.0
80.90	1643.0
82.00	455.0
87.00	1529.0
88.00	1700.0
90.90	166.0
92.00	1254.0
93.00	2289.0
94.00	5062.0
95.10	42376.0
96.00	2644.0
103.90	203.0
105.00	117.0
106.00	254.0
115.80	203.0
116.90	454.0
117.90	215.0
118.80	326.0
127.80	195.0
128.90	151.0
129.90	239.0
137.00	110.0
140.90	641.0
142.90	763.0
144.90	295.0
147.80	109.0
154.90	111.0
157.00	107.0
171.00	102.0
172.00	637.0
174.00	37344.0
175.00	2788.0
176.00	36776.0
177.00	2479.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

Scan 2789 (10.058 min): VV019330.D
BFB92

m/z	Abundance
40.10	185.0
44.00	384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92