




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

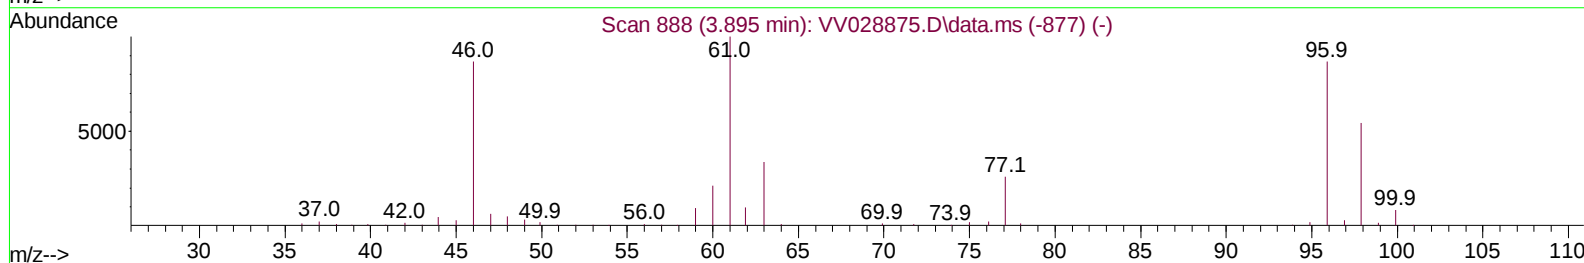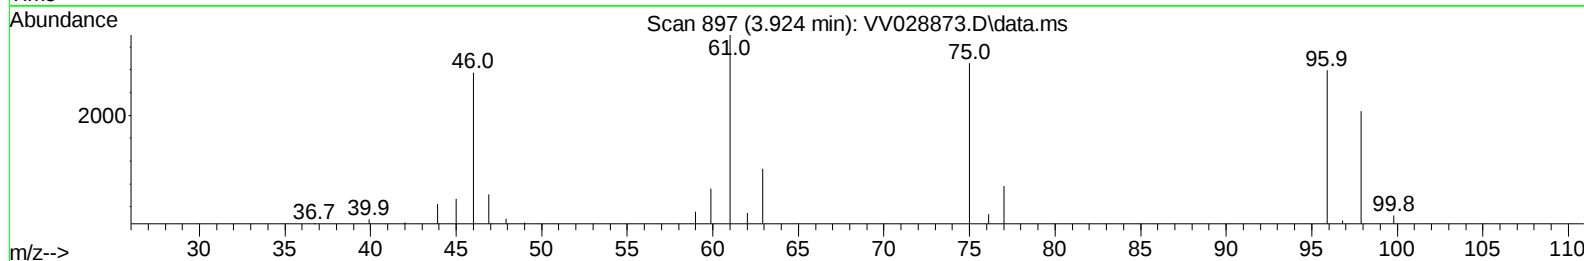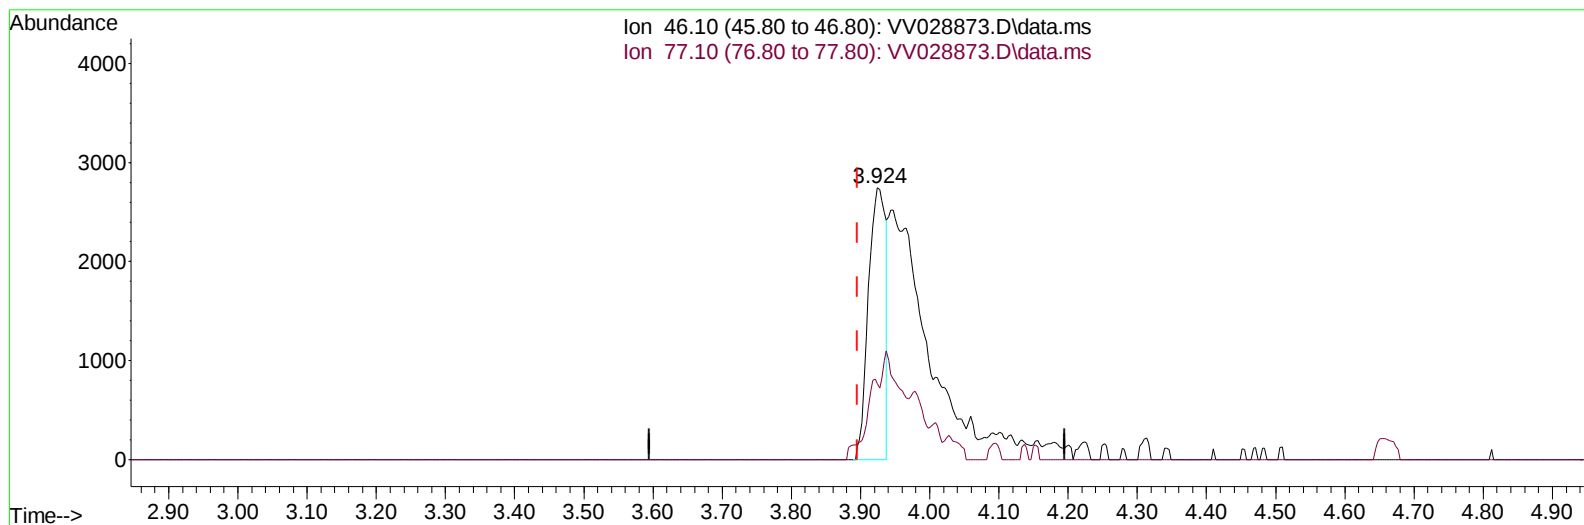

TIC: VV028873.D\data.ms

(20) 2-Butanone-d5 (S)

3.924min (+ 0.029) 1.52 ug/L

response 4725

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.70	24.47
0.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028873.D
Acq On : 11 Nov 2022 13:30
Operator : SY/MD
Sample : VSTD0.577
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5277

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:54:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 11 21:54:17 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/14/2022
Supervised By :Mahesh Dadoda 11/15/2022

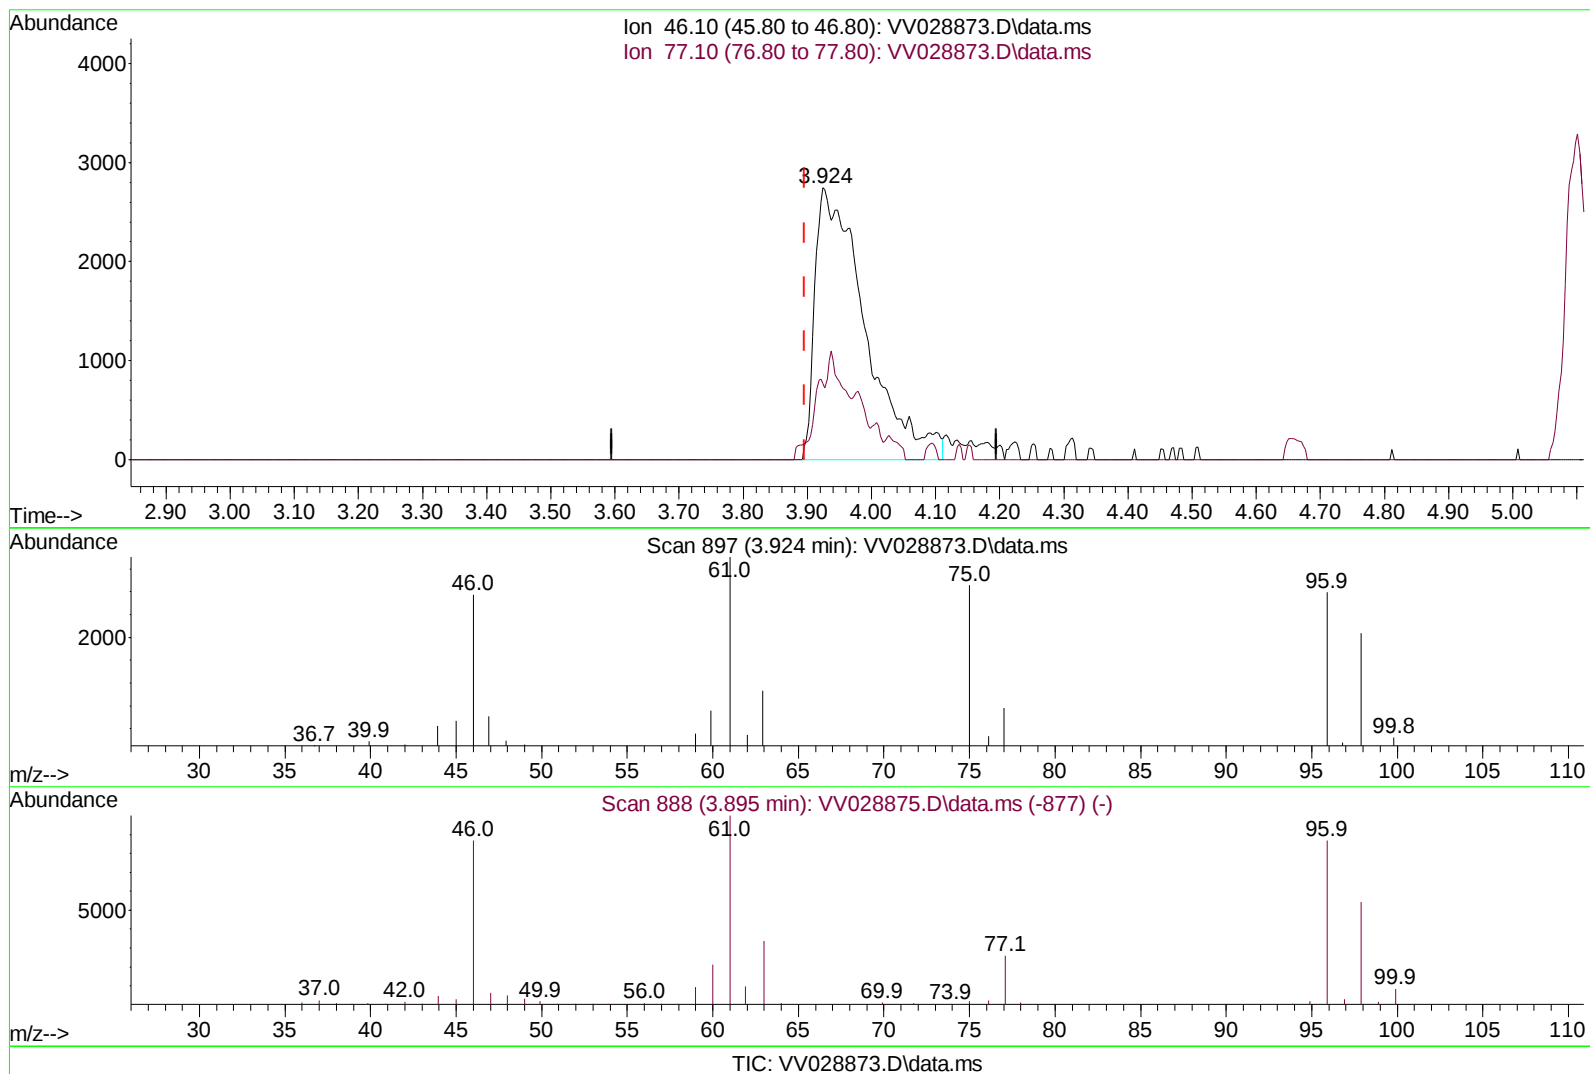

(20) 2-Butanone-d5 (S)

3.924min (+ 0.029) 4.79 ug/L m

response 14839

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.70	7.79#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

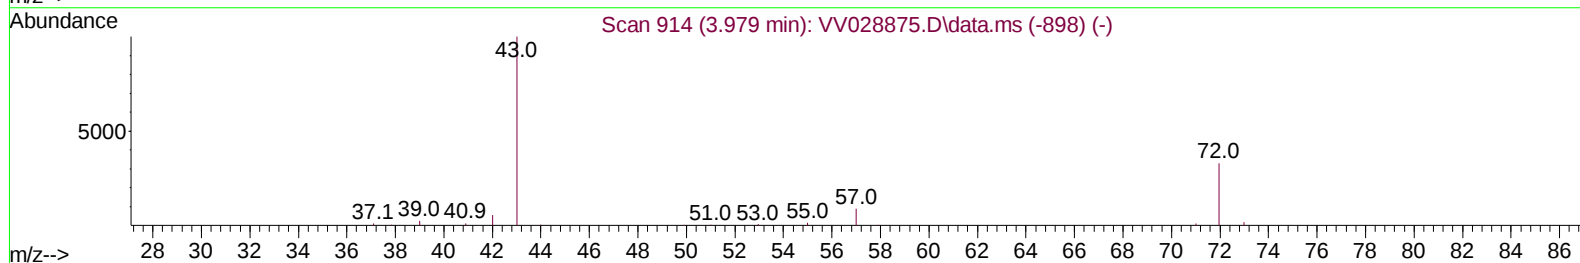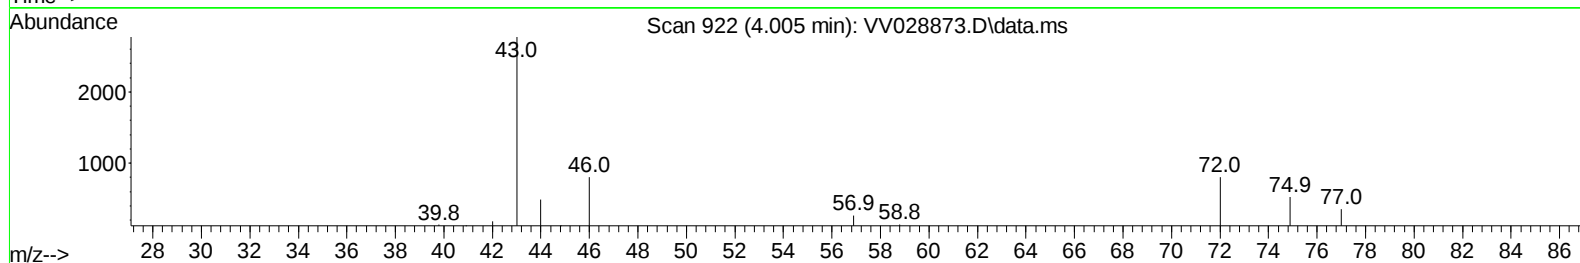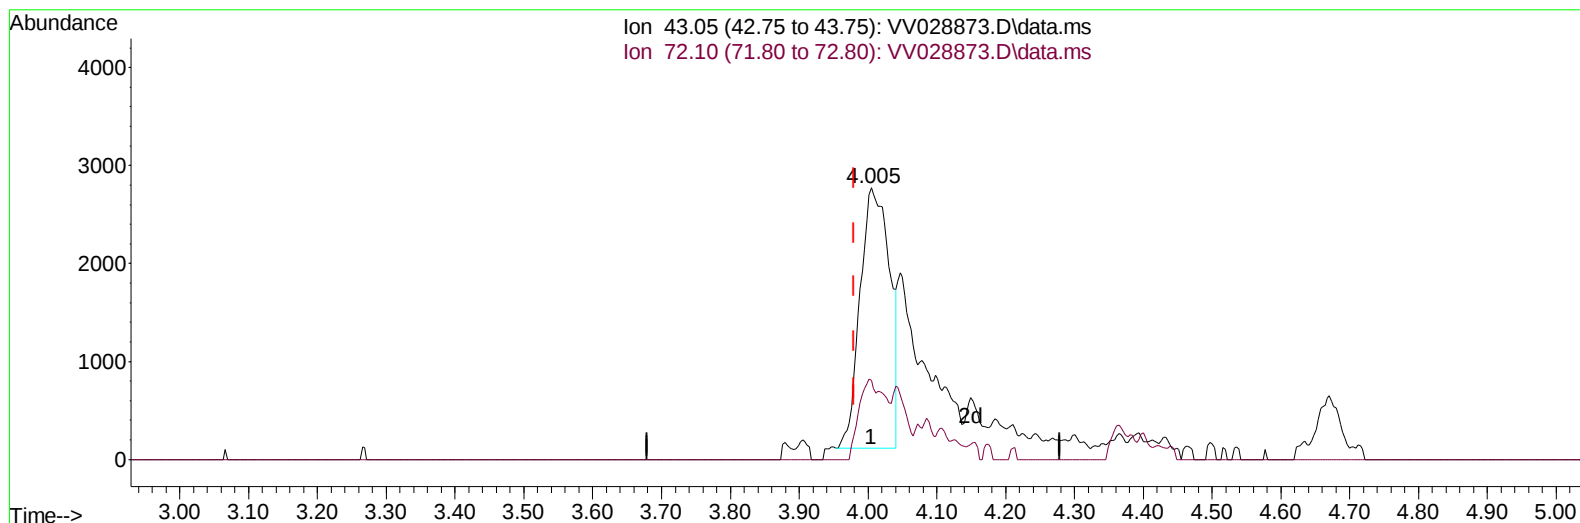

TIC: VV028873.D\data.ms

(21) 2-Butanone (T)

4.005min (+ 0.026) 2.60 ug/L

response 7925

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.90	27.91
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

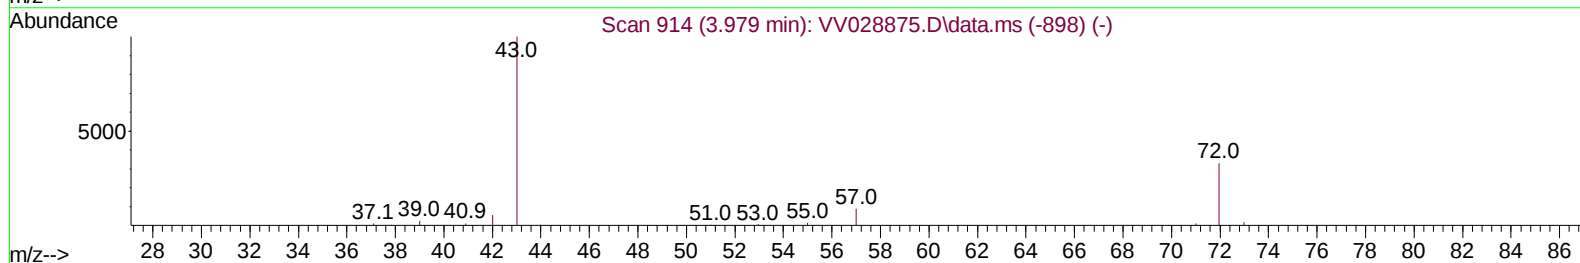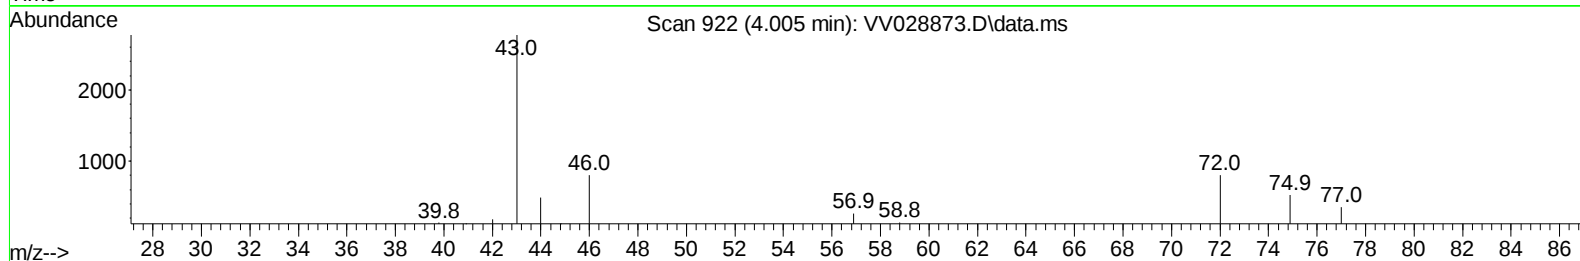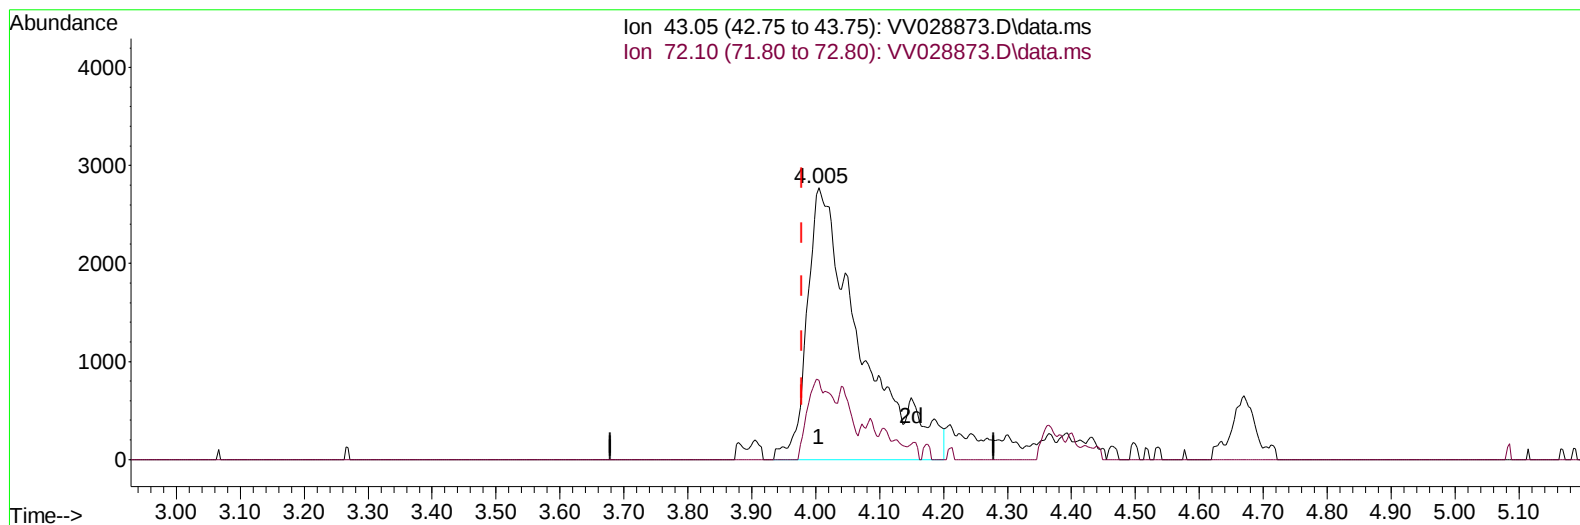

TIC: VV028873.D\data.ms

(21) 2-Butanone (T)

4.005min (+ 0.026) 5.22 ug/L m

response 15918

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.90	13.90
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

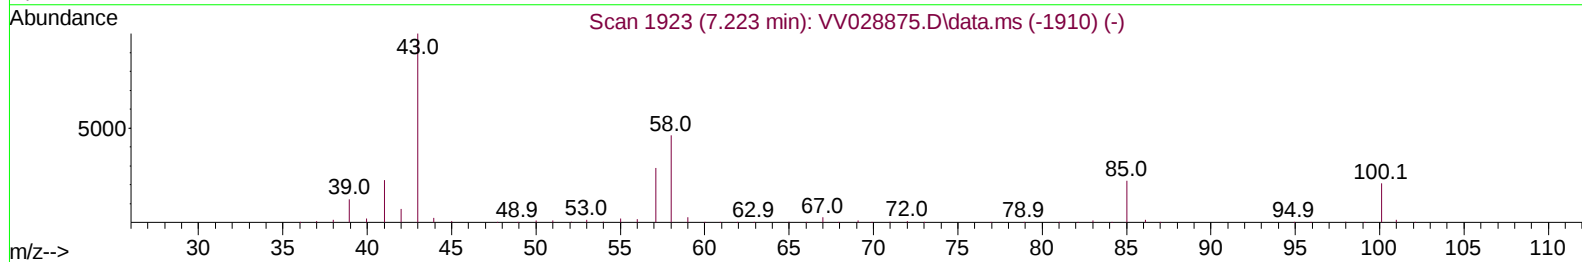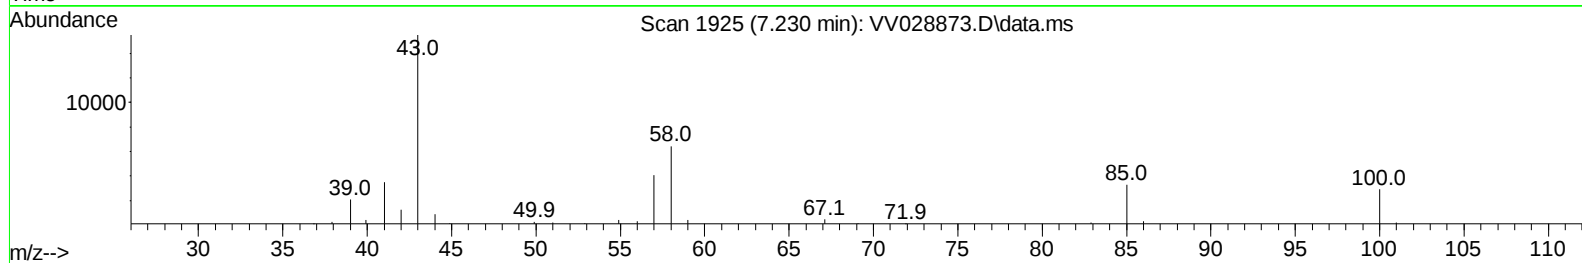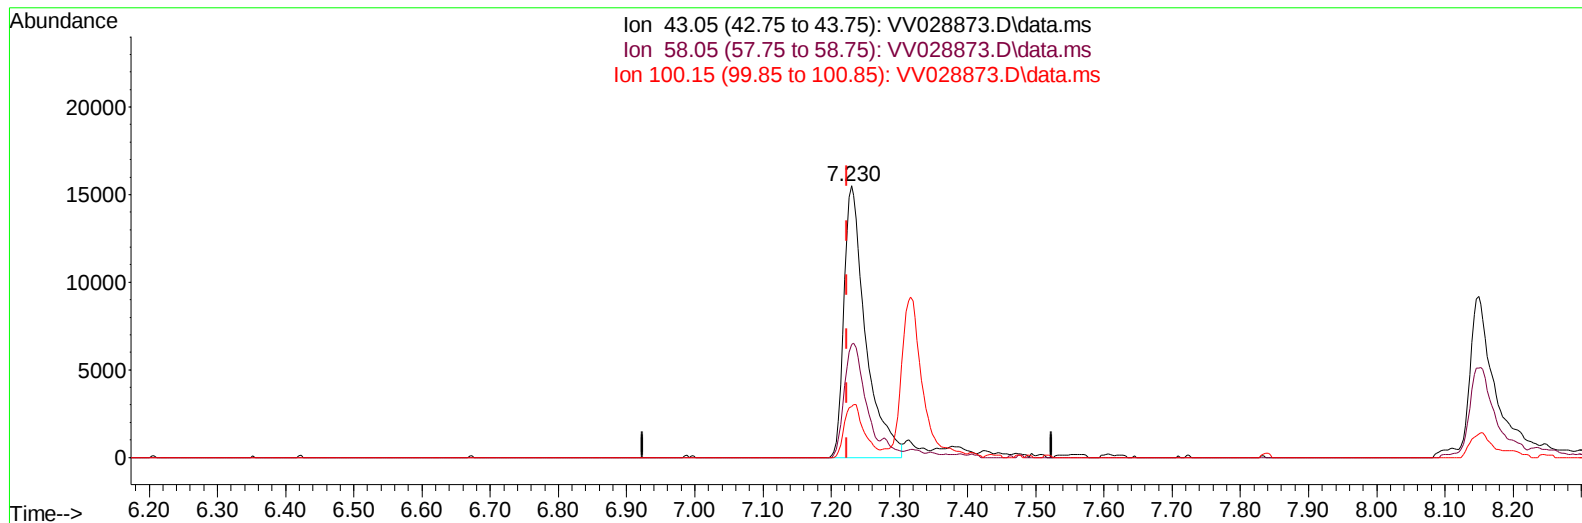

TIC: VV028873.D\data.ms

(40) 4-Methyl-2-pentanone (T)

7.230min (+ 0.006) 3.99 ug/L

response 33936

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	45.80	40.58
100.15	18.10	18.11
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

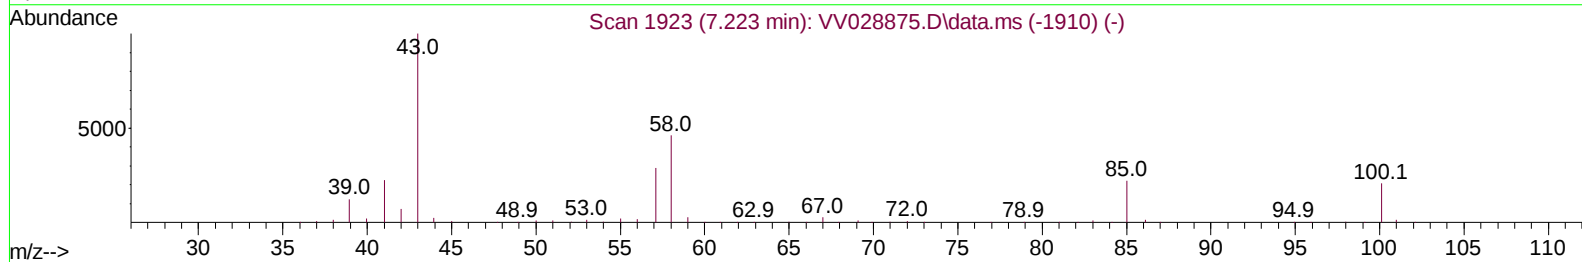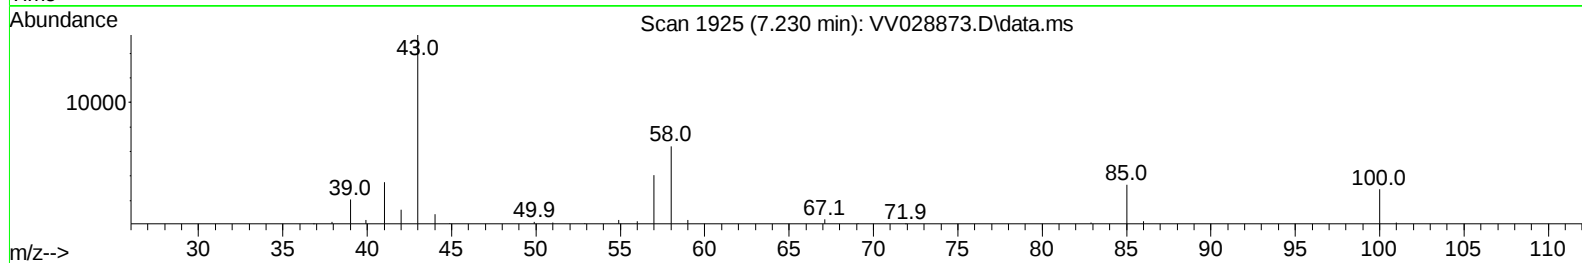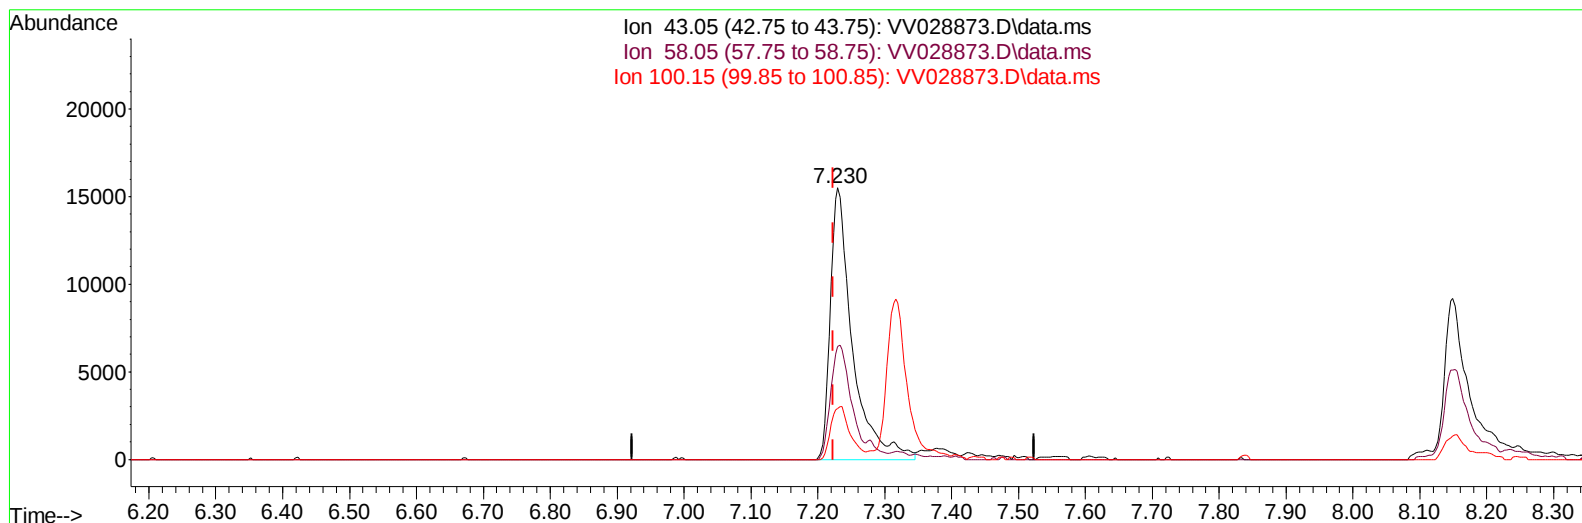

TIC: VV028873.D\data.ms

(40) 4-Methyl-2-pentanone (T)

7.230min (+ 0.006) 4.18 ug/L m

response 35525

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	45.80	38.76
100.15	18.10	17.30
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

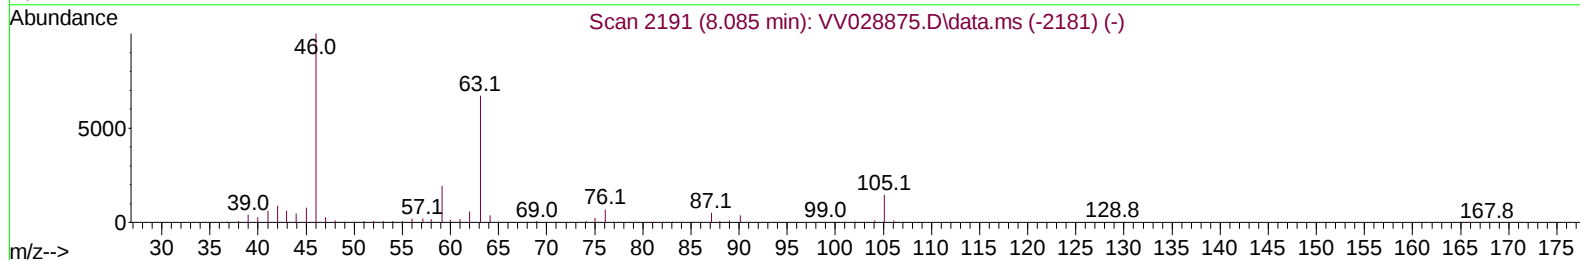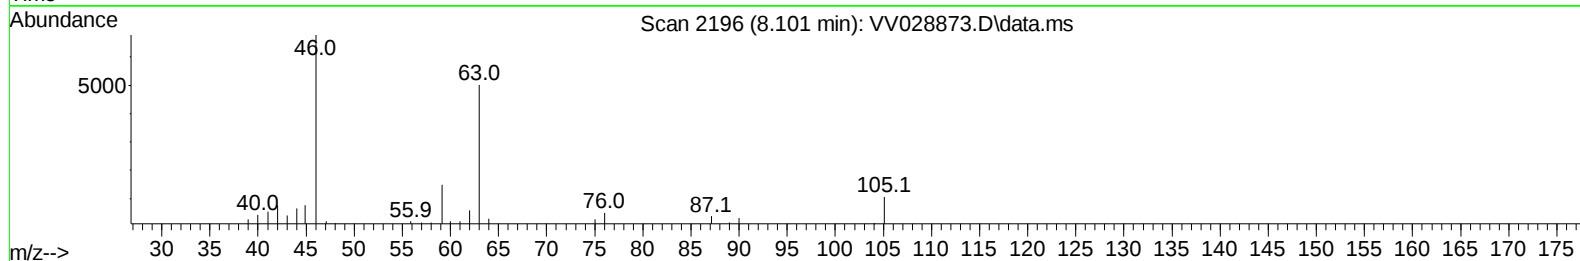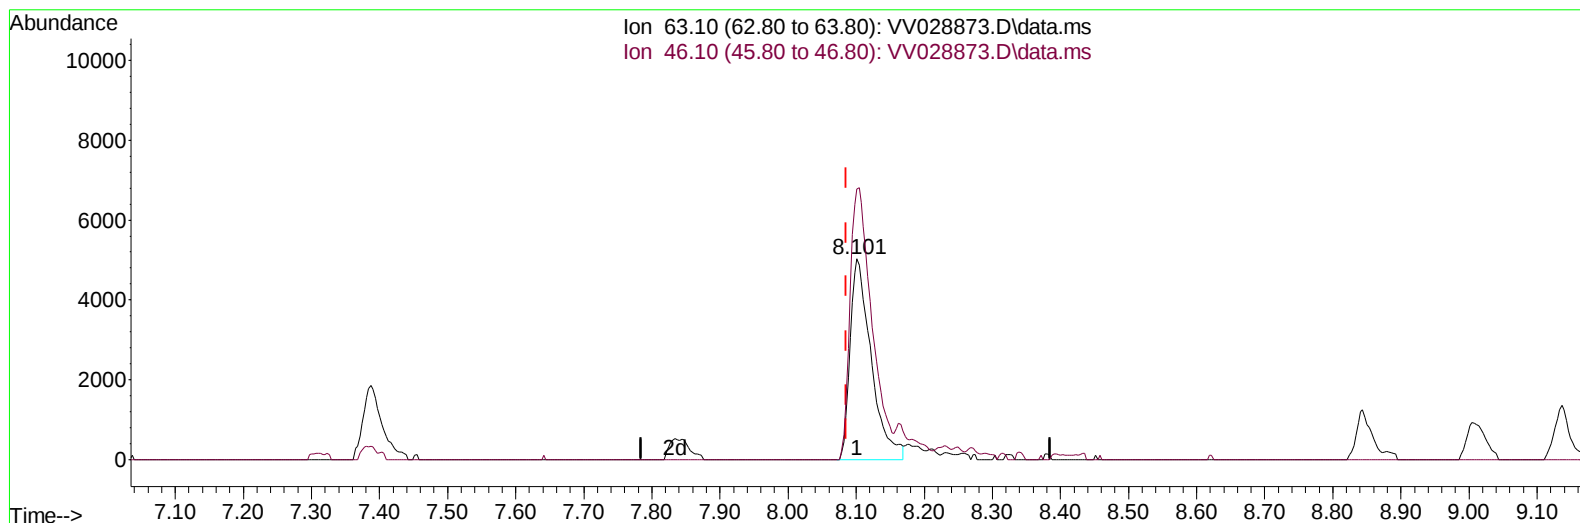

TIC: VV028873.D\data.ms

(46) 2-Hexanone-d5 (S)

8.101min (+ 0.016) 3.35 ug/L

response 10809

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	153.40	141.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

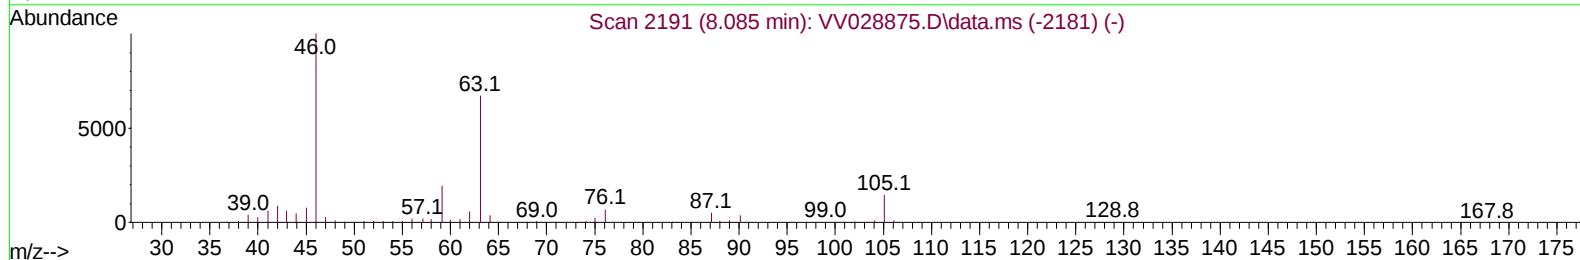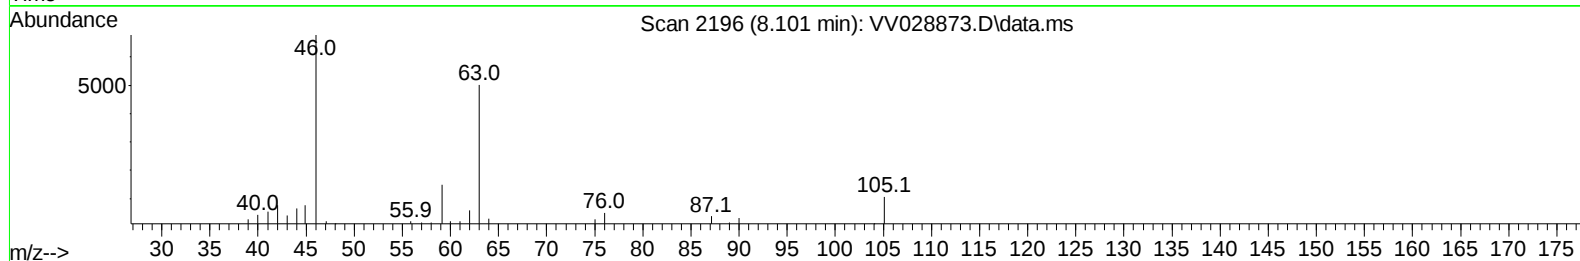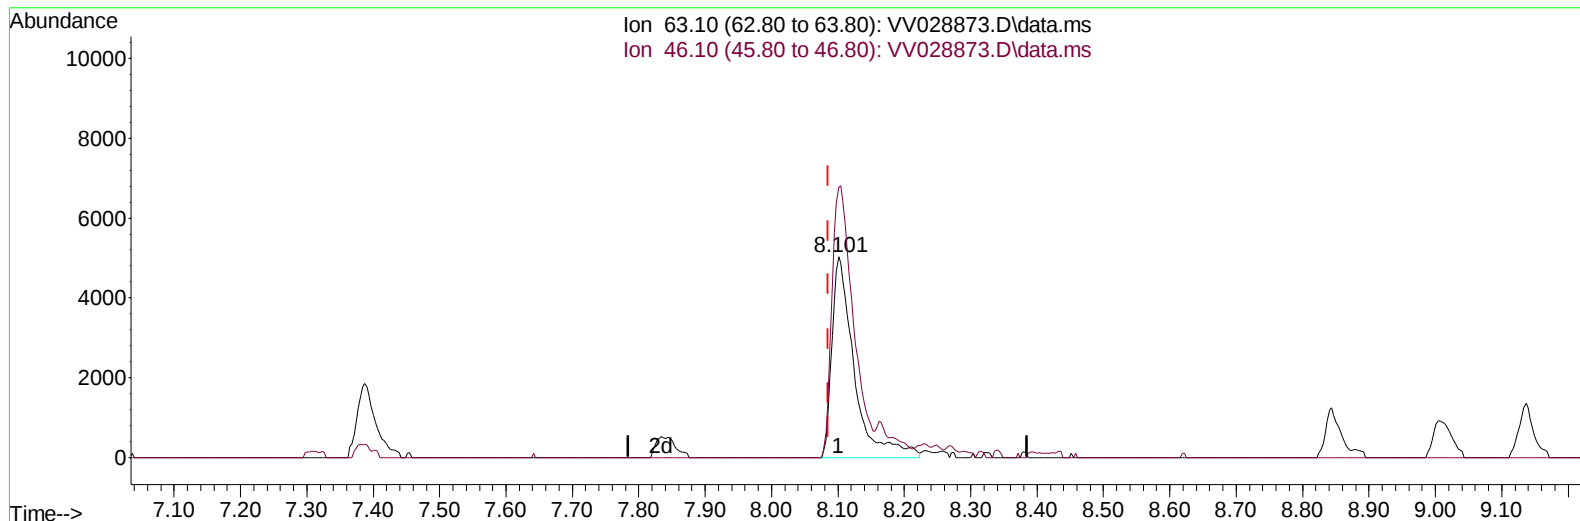

TIC: VV028873.D\data.ms

(46) 2-Hexanone-d5 (S)

8.101min (+ 0.016) 3.63 ug/L m

response 11694

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	153.40	130.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

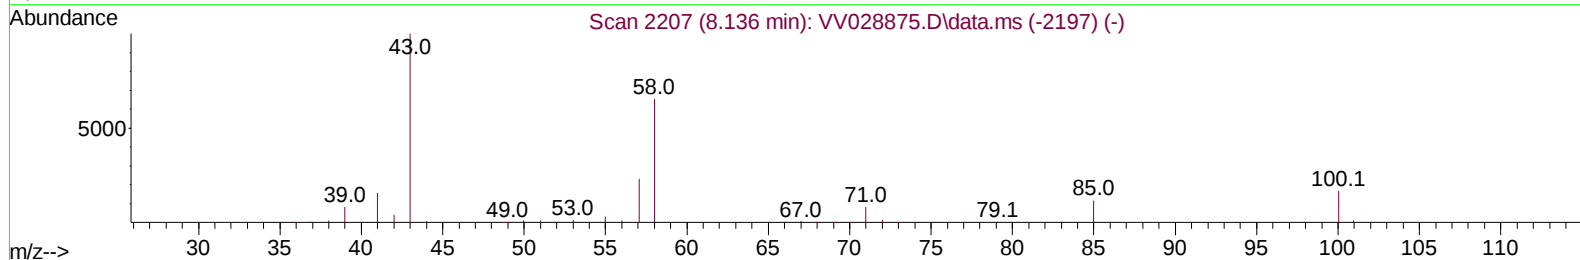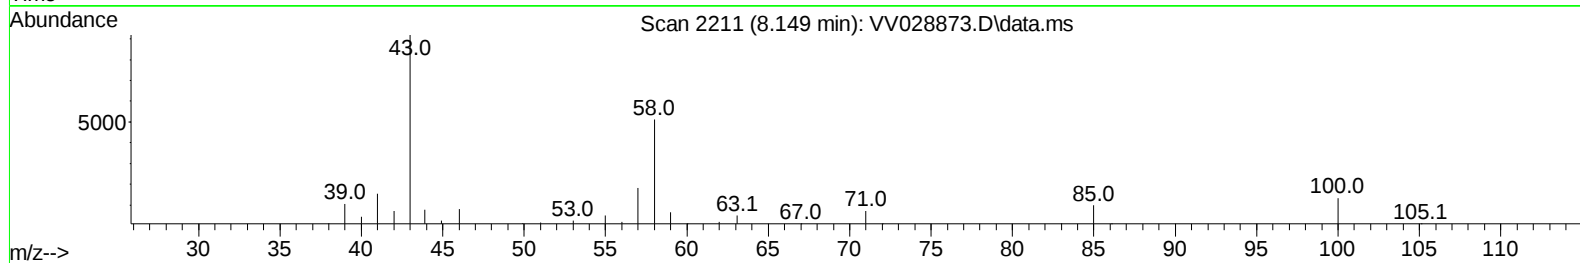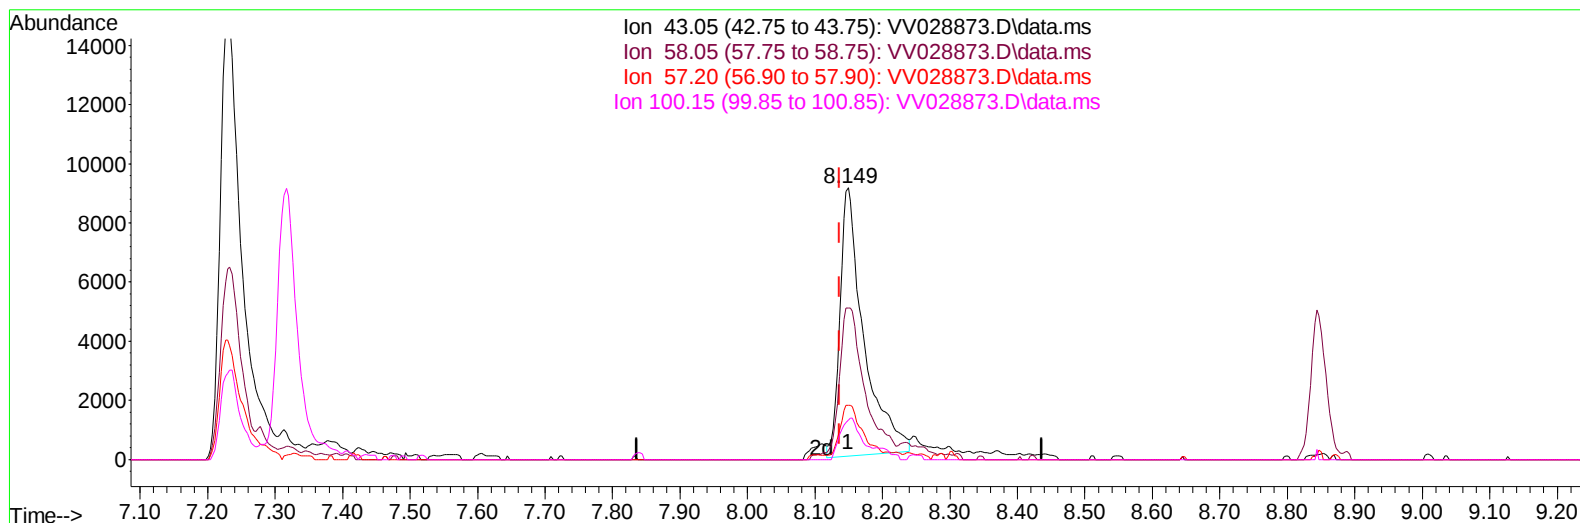

TIC: VV028873.D\data.ms

(48) 2-Hexanone (T)

8.149min (+ 0.013) 3.76 ug/L

response 22250

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	62.80	62.10
57.20	22.30	17.73#
100.15	16.10	13.85




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

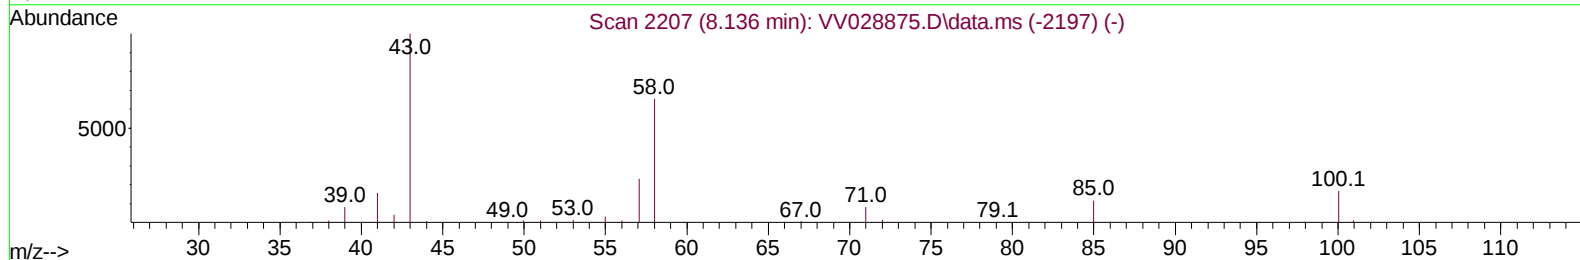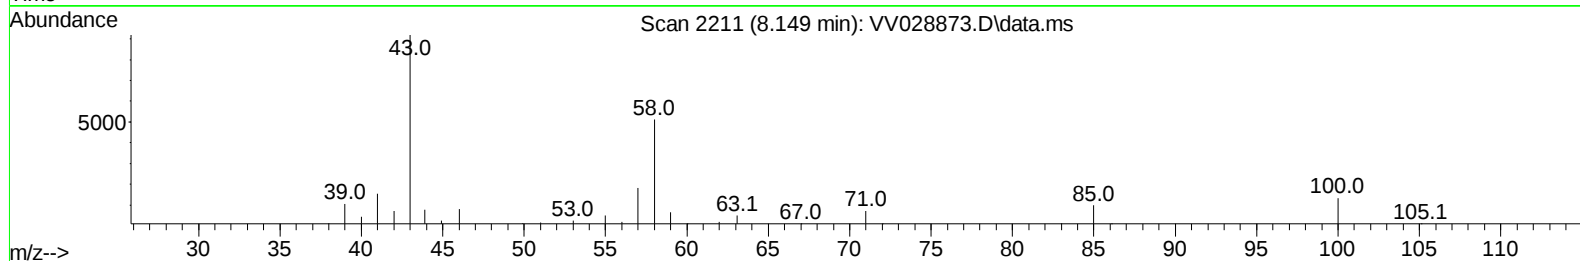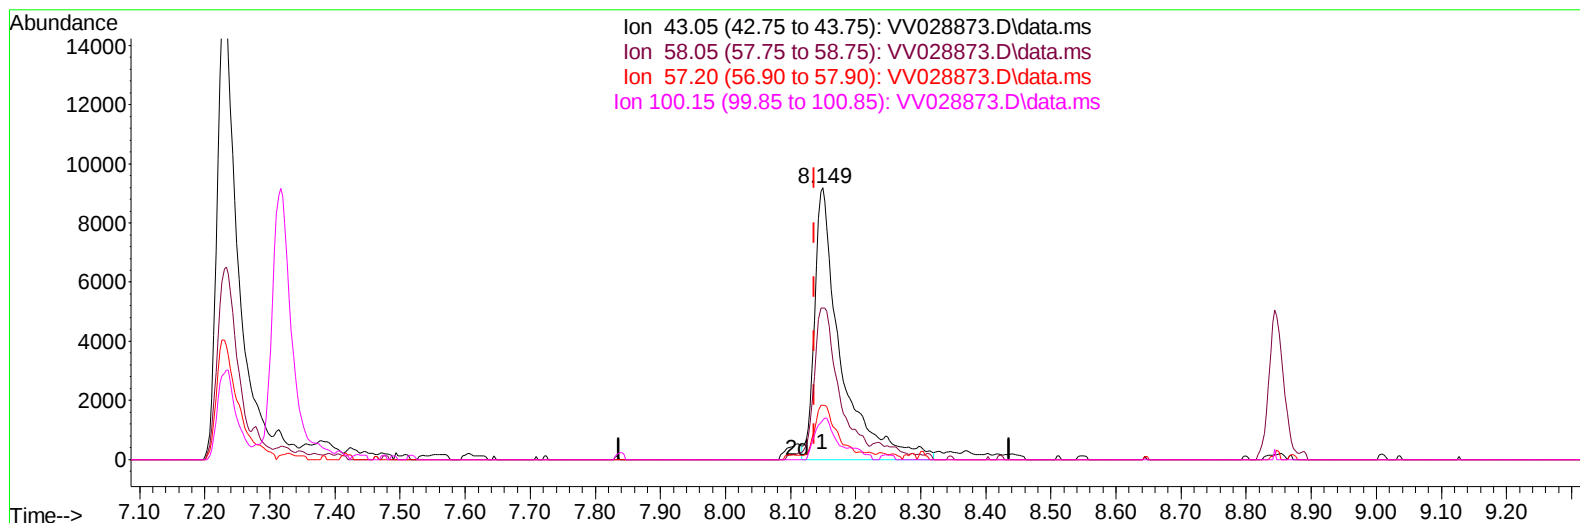

TIC: VV028873.D\data.ms

(48) 2-Hexanone (T)

8.149min (+ 0.013) 4.32 ug/L m

response 25605

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	62.80	53.97
57.20	22.30	15.40#
100.15	16.10	12.04#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	306642	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	280742	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	141365	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	8394	0.449	ug/L	0.00
7) Chloroethane-d5	1.564	69	7115	0.433	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.108	63	14356	0.421	ug/L	0.00
20) 2-Butanone-d5	3.924	46	14839m	4.786	ug/L	0.03
24) Chloroform-d	4.346	84	16036	0.418	ug/L	0.00
26) 1,2-Dichloroethane-d4	5.040	65	7322	0.424	ug/L	0.00
32) Benzene-d6	5.050	84	32382	0.386	ug/L	0.00
36) 1,2-Dichloropropane-d6	6.072	67	9095	0.389	ug/L	0.00
41) Toluene-d8	7.316	98	29049	0.385	ug/L	0.00
43) trans-1,3-Dichloroprop...	7.632	79	2756	0.361	ug/L	0.01
46) 2-Hexanone-d5	8.101	63	11694m	3.629	ug/L	0.02
56) 1,1,2,2-Tetrachloroeth...	10.210	84	6597	0.407	ug/L	0.00
66) 1,2-Dichlorobenzene-d4	11.619	152	10511	0.416	ug/L	0.00
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.127	85	11759	0.460	ug/L	96
3) Chloromethane	1.240	50	9943	0.469	ug/L	98
5) Vinyl chloride	1.310	62	11276	0.466	ug/L	95
6) Bromomethane	1.519	94	6658	0.460	ug/L	89
8) Chloroethane	1.584	64	7494	0.527	ug/L	96
9) Trichlorofluoromethane	1.751	101	15443	0.473	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	2.114	101	8670	0.469	ug/L	97
12) 1,1-Dichloroethene	2.117	96	8585	0.462	ug/L	95
13) Acetone	2.182	43	15545	7.722	ug/L	89
14) Carbon disulfide	2.291	76	31218	0.474	ug/L	99
15) Methyl Acetate	2.439	43	2586	0.529	ug/L	93
16) Methylene chloride	2.503	84	11114	0.463	ug/L	95
17) Methyl tert-butyl Ether	2.764	73	17084	0.429	ug/L #	96
18) trans-1,2-Dichloroethene	2.760	96	9939	0.462	ug/L	93
19) 1,1-Dichloroethane	3.188	63	15776	0.448	ug/L	96
21) 2-Butanone	4.005	43	15918m	5.218	ug/L	
22) cis-1,2-Dichloroethene	3.915	96	9207	0.421	ug/L	94
23) Bromochloromethane	4.249	128	4165	0.450	ug/L	96
25) Chloroform	4.375	83	16087	0.436	ug/L	100
27) 1,2-Dichloroethane	5.140	62	8430	0.444	ug/L	98
29) 1,1,1-Trichloroethane	4.600	97	14341	0.435	ug/L	93
30) Cyclohexane	4.667	56	13710	0.409	ug/L	98
31) Carbon tetrachloride	4.825	117	12848	0.453	ug/L	96
33) Benzene	5.098	78	36593	0.427	ug/L	100
34) Trichloroethene	5.918	95	9204	0.419	ug/L	94
35) Methylcyclohexane	6.124	83	16053	0.416	ug/L	100
37) 1,2-Dichloropropane	6.175	63	8553	0.432	ug/L #	96
38) Bromodichloromethane	6.509	83	10594	0.423	ug/L	98
39) cis-1,3-Dichloropropene	7.034	75	10743	0.389	ug/L	98
40) 4-Methyl-2-pentanone	7.230	43	35525m	4.181	ug/L	
42) Toluene	7.387	91	45394	0.490	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028873.D
 Acq On : 11 Nov 2022 13:30
 Operator : SY/MD
 Sample : VSTD0.577
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5277

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/14/2022
 Supervised By :Mahesh Dadoda 11/15/2022

Quant Time: Nov 11 21:54:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 11 21:54:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) trans-1,3-Dichloropropene	7.657	75	8687	0.405	ug/L	96
45) 1,1,2-Trichloroethane	7.841	97	5576	0.431	ug/L	95
47) Tetrachloroethene	7.972	164	7639	0.434	ug/L	96
48) 2-Hexanone	8.149	43	25605m	4.324	ug/L	
49) Dibromochloromethane	8.243	129	6736	0.430	ug/L	100
50) 1,2-Dibromoethane	8.355	107	5079	0.422	ug/L #	98
51) Chlorobenzene	8.879	112	25511	0.445	ug/L	98
52) Ethylbenzene	9.011	91	42110	0.436	ug/L	98
53) m,p-Xylene	9.136	106	17091	0.445	ug/L	98
54) o-Xylene	9.538	106	15708	0.431	ug/L	97
55) Styrene	9.561	104	24338	0.398	ug/L	96
57) 1,1,2,2-Tetrachloroethane	10.236	83	6772	0.449	ug/L	99
59) Bromoform	9.728	173	3219	0.418	ug/L	95
60) Isopropylbenzene	9.924	105	40553	0.442	ug/L	100
61) 1,2,3-Trichloropropane	10.271	75	4225	0.437	ug/L #	93
62) 1,3,5-Trimethylbenzene	10.535	105	33794	0.435	ug/L	100
63) 1,2,4-Trimethylbenzene	10.908	105	33595	0.431	ug/L	98
64) 1,3-Dichlorobenzene	11.178	146	19317	0.448	ug/L	98
65) 1,4-Dichlorobenzene	11.268	146	20418	0.471	ug/L	96
67) 1,2-Dichlorobenzene	11.638	146	17063	0.440	ug/L	95
68) 1,2-Dibromo-3-chloropr...	12.429	75	762	0.401	ug/L	94
69) 1,3,5-Trichlorobenzene	12.638	180	14157	0.426	ug/L	97
70) 1,2,4-trichlorobenzene	13.255	180	8859	0.352	ug/L	92
71) Naphthalene	13.503	128	11628	0.358	ug/L	99
72) 1,2,3-Trichlorobenzene	13.737	180	7916	0.371	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

