

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028916.D
 Acq On : 12 Nov 2022 08:18
 Operator : SY/MD
 Sample : N5602-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG6

Quant Time: Nov 14 00:25:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 12 03:43:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	309553	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	281425	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	137187	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	81971	4.344	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.800%
7) Chloroethane-d5	1.565	69	77976	4.700	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.000%
11) 1,1-Dichloroethene-d2	2.105	63	115586	3.361	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.200%
20) 2-Butanone-d5	3.892	46	139837	44.265	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.540%
24) Chloroform-d	4.343	84	188466	4.864	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	5.031	65	85299	4.893	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%
32) Benzene-d6	5.044	84	394454	4.696	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	6.066	67	117533	5.011	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.200%
41) Toluene-d8	7.310	98	345486	4.569	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.400%
43) trans-1,3-Dichloroprop...	7.622	79	30777	4.023	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%
46) 2-Hexanone-d5	8.088	63	156369	47.885	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.780%
56) 1,1,2,2-Tetrachloroeth...	10.211	84	80253	4.935	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.600%
66) 1,2-Dichlorobenzene-d4	11.616	152	126637	5.160	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.200%
Target Compounds						
22) cis-1,2-Dichloroethene	3.909	96	3590	0.162	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028916.D
Acq On : 12 Nov 2022 08:18
Operator : SY/MD
Sample : N5602-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Quant Time: Nov 14 00:25:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 12 03:43:58 2022
Response via : Initial Calibration

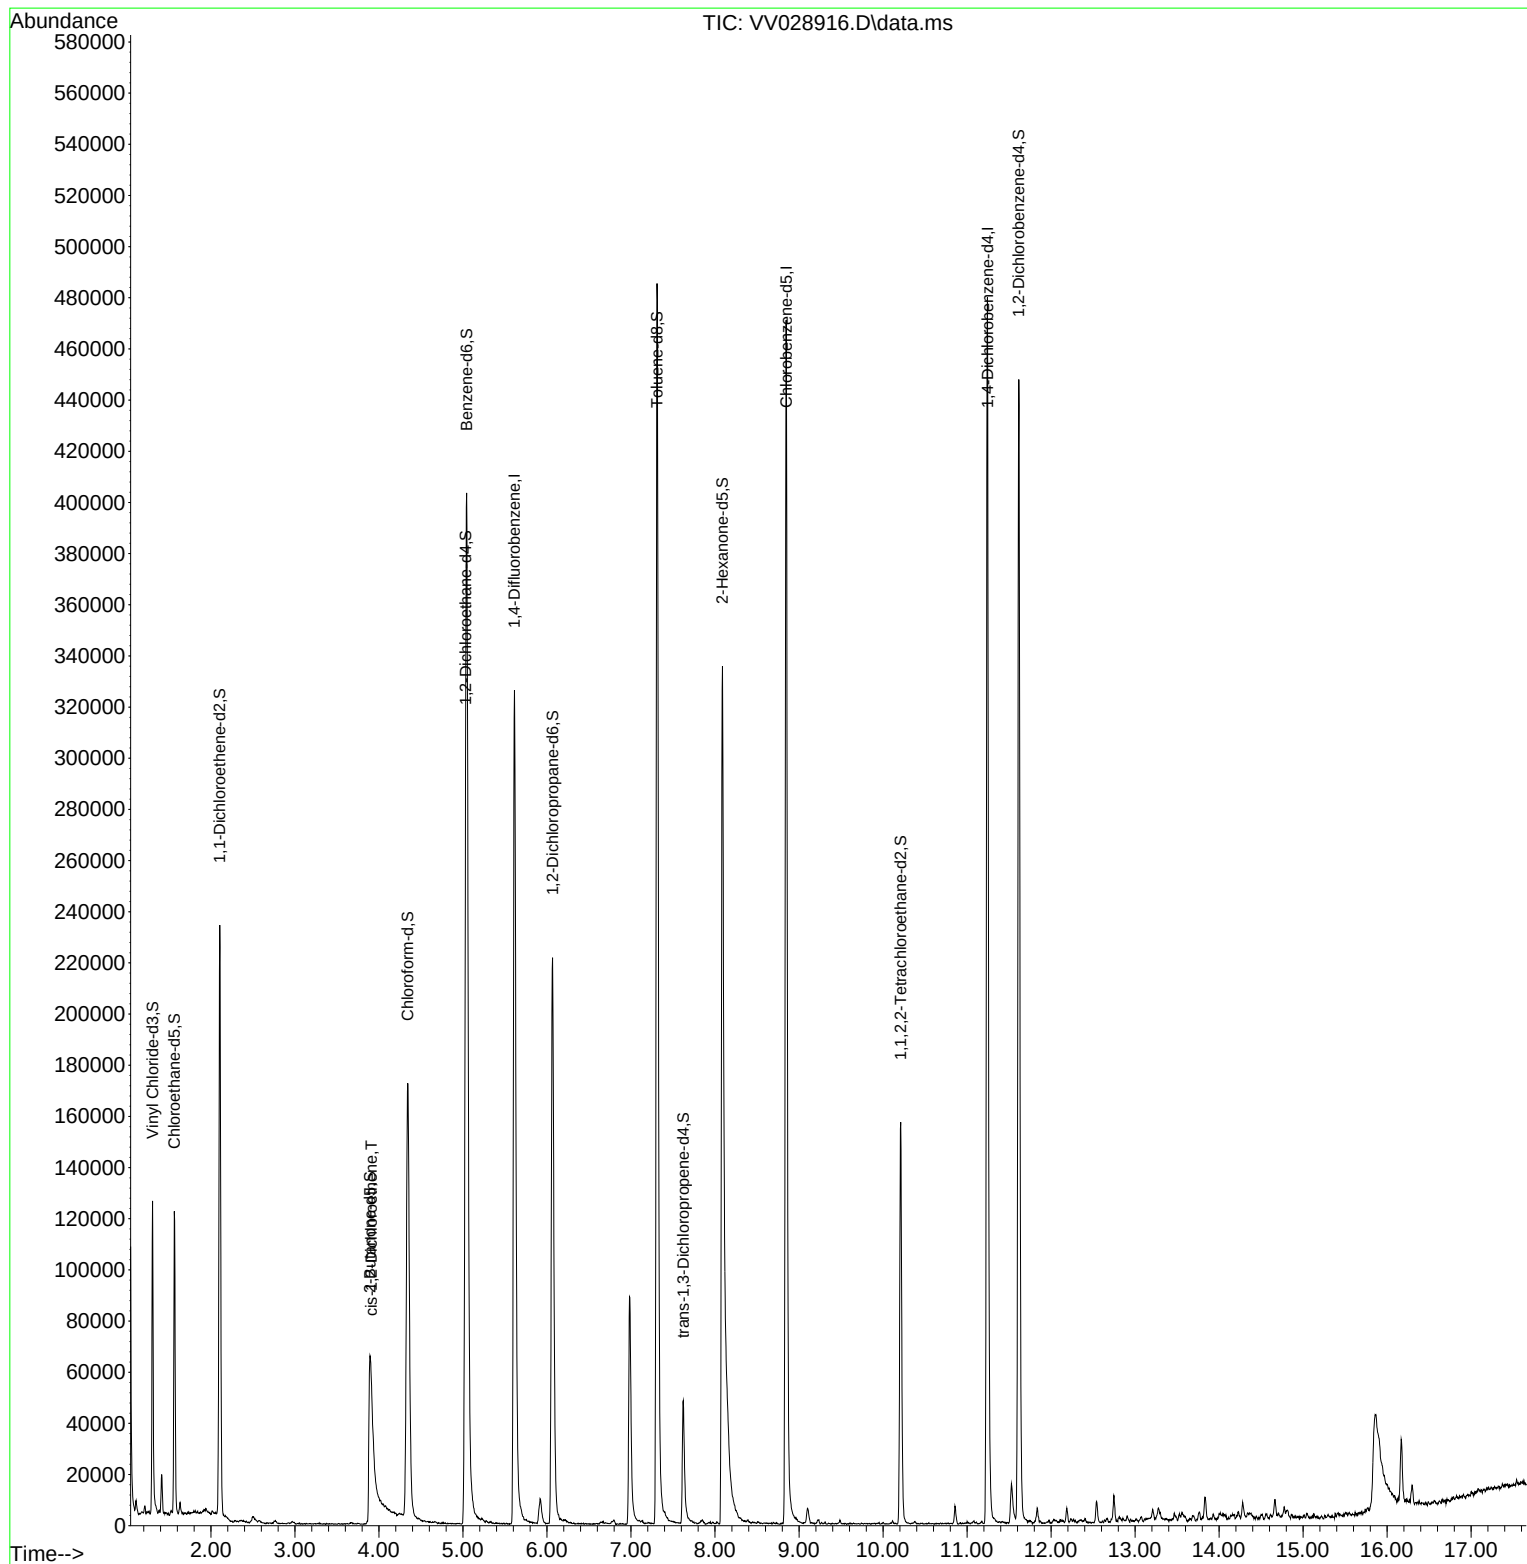

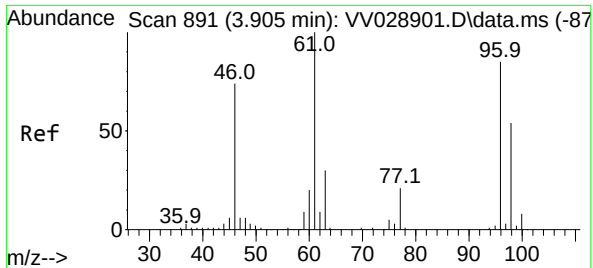

#22
 cis-1,2-Dichloroethene
 Concen: 0.162 ug/L
 RT: 3.909 min Scan# 891
 Delta R.T. 0.003 min
 Lab File: VV028916.D
 Acq: 12 Nov 2022 08:18

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG6

Tgt Ion: 96 Resp: 3590
 Ion Ratio Lower Upper
 96 100
 61 120.2 82.3 152.9
 68 0.0 0.0 0.0

