

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028919.D
 Acq On : 12 Nov 2022 09:32
 Operator : SY/MD
 Sample : N5602-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Quant Time: Nov 14 00:26:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 12 03:43:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.583	114	223303	5.000	ug/L	-0.03
28) Chlorobenzene-d5	8.853	117	270298	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	137694	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.297	65	74514	5.473	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.400%
7) Chloroethane-d5	1.561	69	72408	6.050	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	121.000%
11) 1,1-Dichloroethene-d2	2.098	63	98522	3.971	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.400%
20) 2-Butanone-d5	3.966	46	117191	51.425	ug/L	0.08
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.860%
24) Chloroform-d	4.336	84	153393	5.488	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.800%
26) 1,2-Dichloroethane-d4	5.030	65	71371	5.675	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.600%
32) Benzene-d6	5.034	84	327556	4.060	ug/L	-0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.200%
36) 1,2-Dichloropropane-d6	6.040	67	78857	3.500	ug/L	-0.03
Spiked Amount	5.000	Range	60 - 140	Recovery	=	70.000%
41) Toluene-d8	7.317	98	334475	4.605	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	7.632	79	21839	2.972	ug/L	0.01
Spiked Amount	5.000	Range	55 - 130	Recovery	=	59.400%
46) 2-Hexanone-d5	8.117	63	135703	43.267	ug/L	0.03
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.540%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	75816	4.854	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	11.619	152	126431	5.132	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.600%
Target Compounds					Qvalue	
13) Acetone	2.256	43	9955	6.791	ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028919.D
Acq On : 12 Nov 2022 09:32
Operator : SY/MD
Sample : N5602-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Time: Nov 14 00:26:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 12 03:43:58 2022
Response via : Initial Calibration

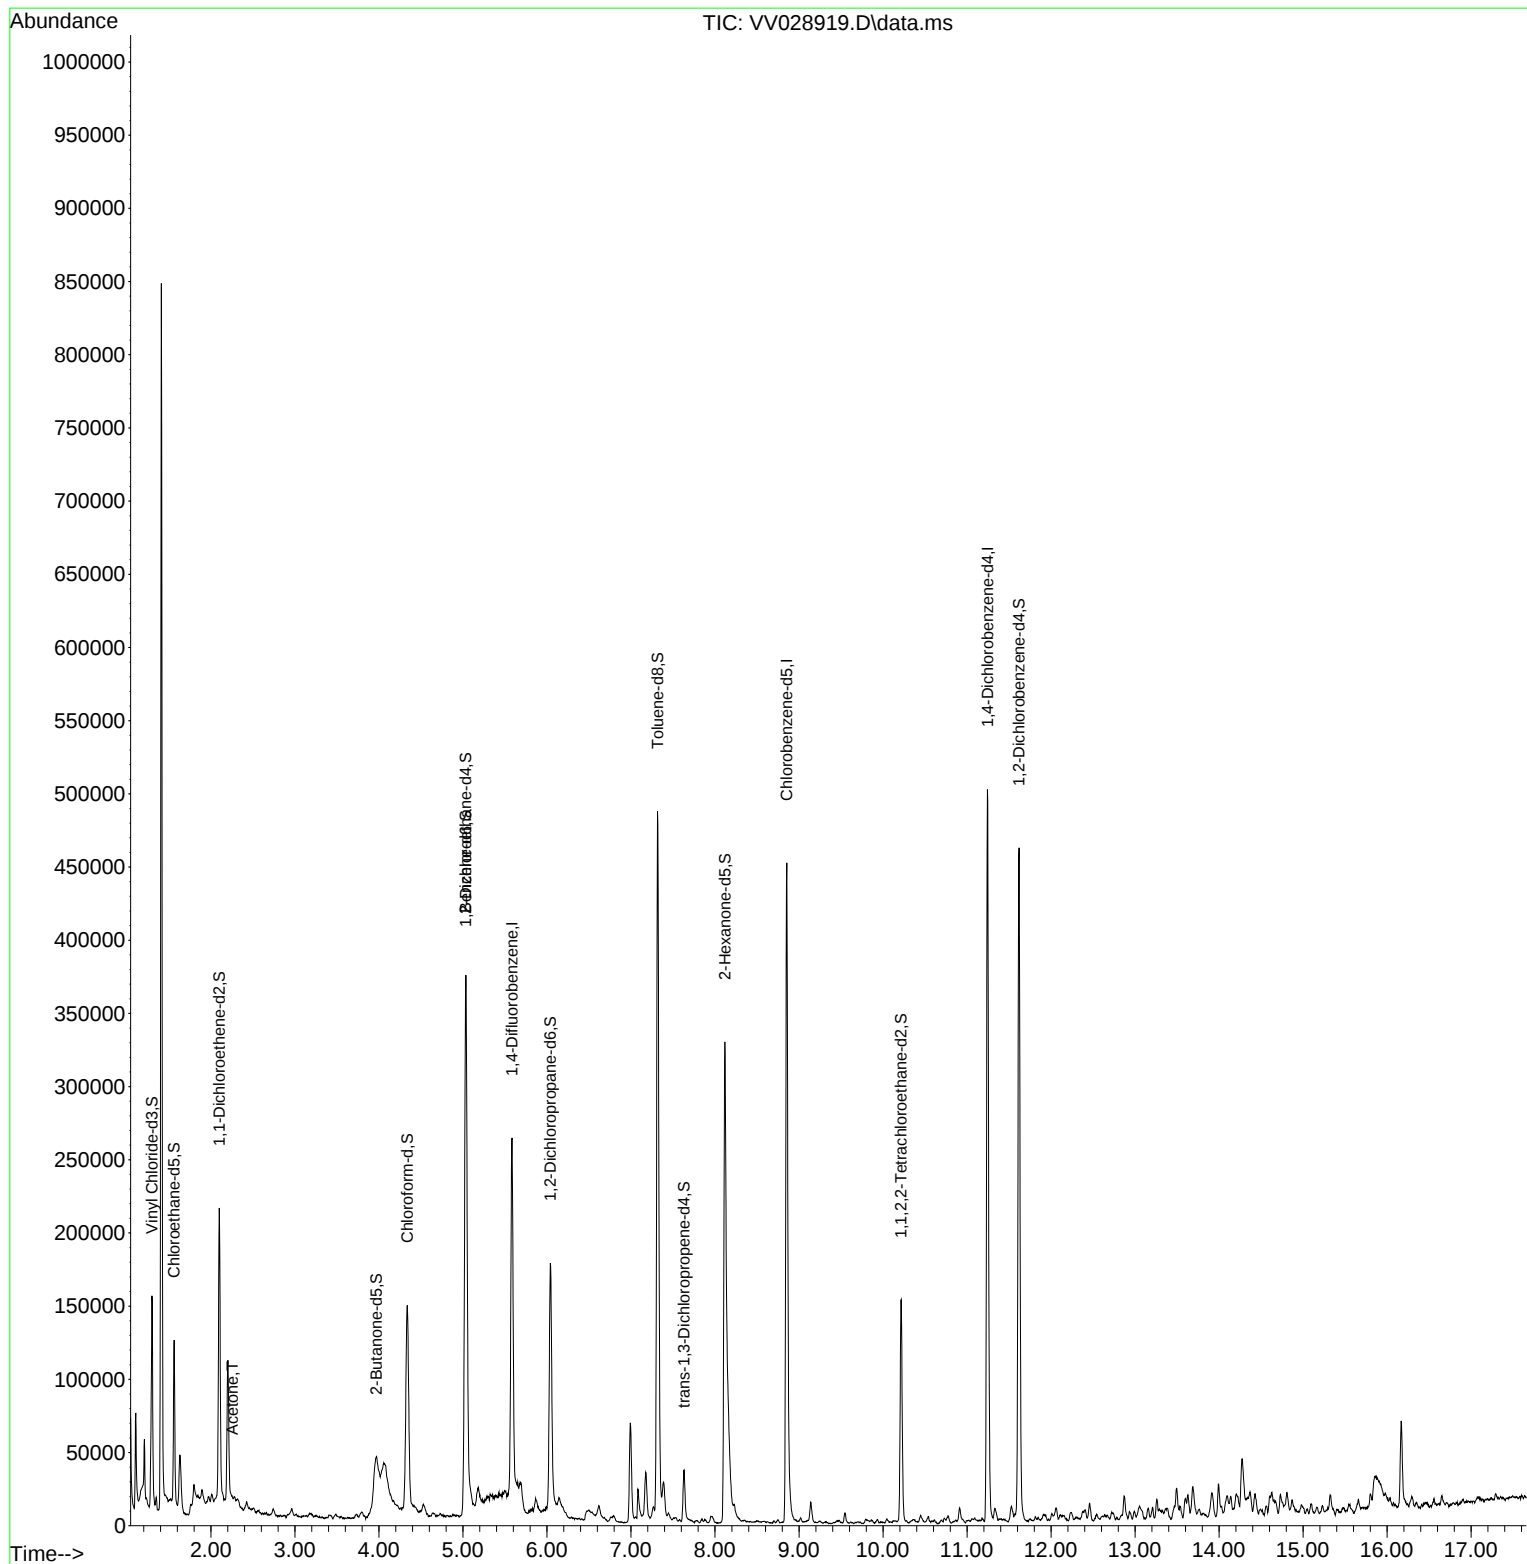

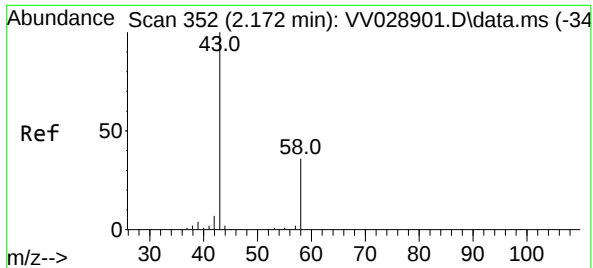

#13
 Acetone
 Concen: 6.791 ug/L
 RT: 2.256 min Scan# 31
 Delta R.T. 0.084 min
 Lab File: VV028919.D
 Acq: 12 Nov 2022 09:32

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Tgt Ion: 43 Resp: 9955
 Ion Ratio Lower Upper
 43 100
 58 14.5 0.0 56.6

