

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028885.D
 Acq On : 11 Nov 2022 19:11
 Operator : SY/MD
 Sample : N5602-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.072	7	10	16	rVB	25896	22680	1.36%	0.239%
2	1.108	16	21	38	rVB2	25523	30278	1.82%	0.319%
3	1.304	74	82	102	rVB	129789	145111	8.73%	1.529%
4	1.413	110	116	124	rVB	14934	16946	1.02%	0.179%
5	1.564	155	163	176	rBV	119622	136158	8.19%	1.434%
6	2.105	320	331	347	rBV2	242156	359506	21.62%	3.787%
7	2.760	523	535	549	rBV2	16003	29873	1.80%	0.315%
8	3.905	875	891	925	rBV2	654575	1662896	100.00%	17.517%
9	4.342	1013	1027	1058	rVB	172499	434809	26.15%	4.580%
10	5.043	1227	1245	1283	rBV2	409043	1034677	62.22%	10.900%
11	5.612	1410	1422	1451	rBV	311722	647593	38.94%	6.822%
12	5.918	1506	1517	1542	rVB8	18642	45017	2.71%	0.474%
13	6.066	1550	1563	1591	rBV	220101	460817	27.71%	4.854%
14	6.985	1837	1849	1866	rBV	94464	180092	10.83%	1.897%
15	7.313	1939	1951	1982	rBV	501689	904325	54.38%	9.526%
16	7.622	2036	2047	2066	rBV	50702	97474	5.86%	1.027%
17	8.088	2182	2192	2252	rBV	313390	823284	49.51%	8.673%
18	8.847	2417	2428	2465	rBV	445326	763183	45.89%	8.040%
19	10.210	2838	2852	2876	rBV	152374	253660	15.25%	2.672%
20	11.242	3161	3173	3201	rBV	454202	727397	43.74%	7.663%
21	11.615	3278	3289	3313	rVV	438910	717086	43.12%	7.554%




Sum of corrected areas: 9492862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028885.D
Acq On : 11 Nov 2022 19:11
Operator : SY/MD
Sample : N5602-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

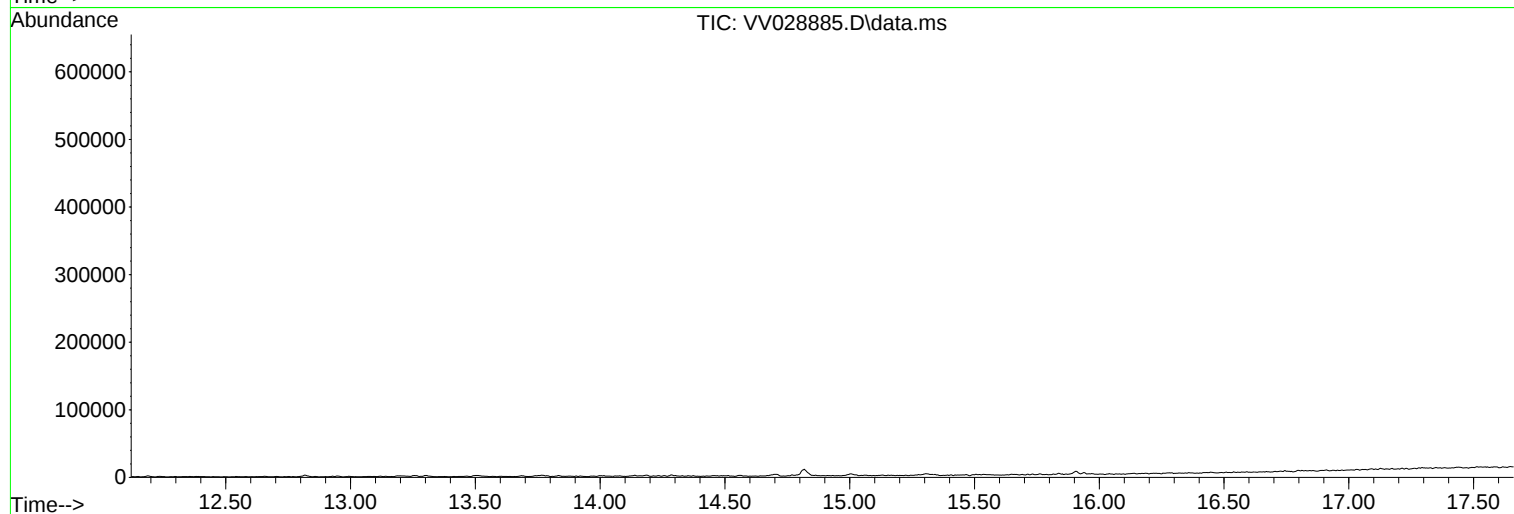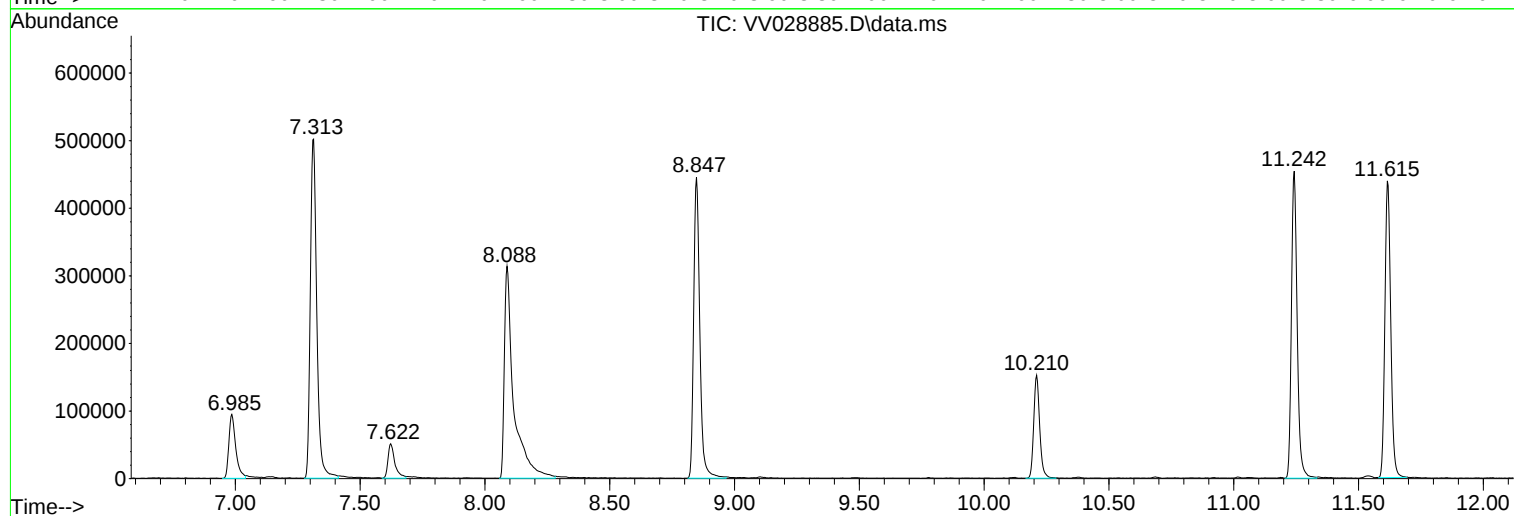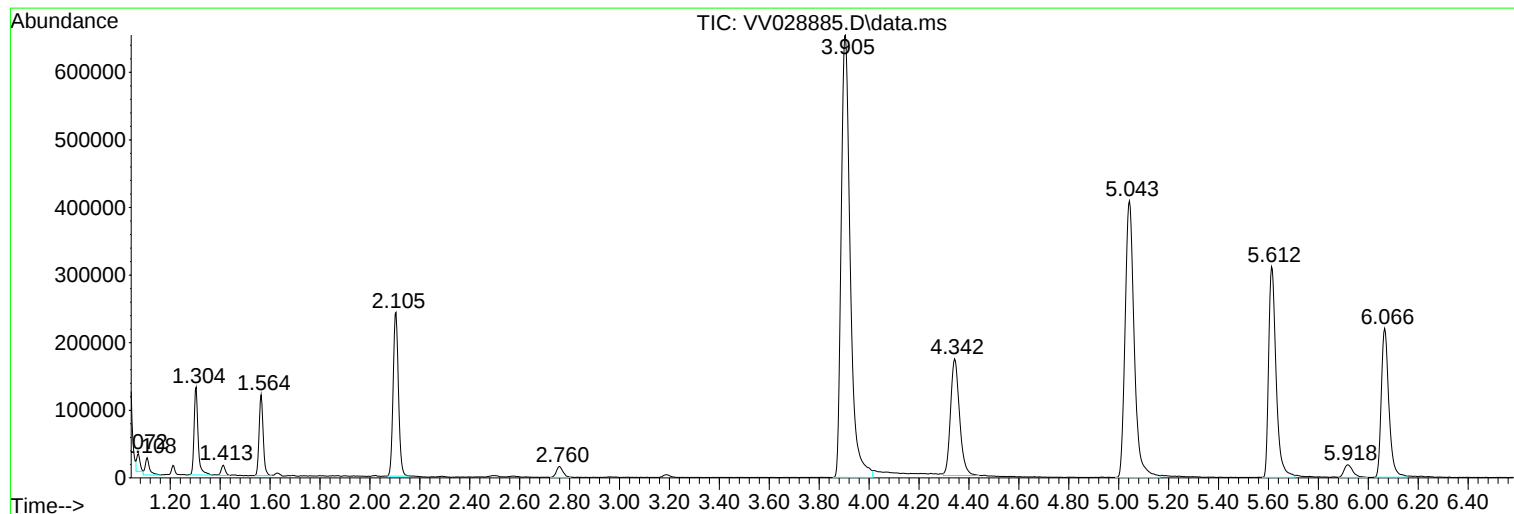

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028885.D
Acq On : 11 Nov 2022 19:11
Operator : SY/MD
Sample : N5602-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028885.D
Acq On : 11 Nov 2022 19:11
Operator : SY/MD
Sample : N5602-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
