

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028895.D
 Acq On : 11 Nov 2022 23:17
 Operator : SY/MD
 Sample : N5592-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AC2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	119610	132908	3.28%	1.002%
2	1.446	112	126	140	rBV3	14466	58572	1.45%	0.441%
3	1.565	156	163	178	rVB	117821	141286	3.49%	1.065%
4	2.108	321	332	348	rVB3	276052	444529	10.98%	3.350%
5	3.886	875	885	922	rBV	99225	329043	8.13%	2.480%
6	4.343	1011	1027	1059	rBV	172240	448590	11.08%	3.381%
7	5.043	1229	1245	1276	rBV2	405784	1019585	25.19%	7.684%
8	5.613	1411	1422	1453	rBV	316766	659304	16.29%	4.969%
9	5.912	1501	1515	1550	rBV	532752	1069179	26.41%	8.057%
10	6.066	1551	1563	1587	rVV2	225409	462284	11.42%	3.484%
11	6.986	1838	1849	1875	rBV	93982	183195	4.53%	1.381%
12	7.310	1939	1950	1977	rBV	490706	889899	21.98%	6.706%
13	7.622	2037	2047	2079	rBV	51437	100096	2.47%	0.754%
14	7.969	2133	2155	2182	rBV	2421808	4048037	100.00%	30.507%
15	8.088	2182	2192	2229	rVV	374101	804030	19.86%	6.059%
16	8.847	2416	2428	2455	rBV	464254	784113	19.37%	5.909%
17	10.210	2840	2852	2870	rBV	157561	254287	6.28%	1.916%
18	11.243	3162	3173	3203	rBV	457943	749178	18.51%	5.646%
19	11.616	3274	3289	3310	rBV	421841	691273	17.08%	5.210%




Sum of corrected areas: 13269388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028895.D
Acq On : 11 Nov 2022 23:17
Operator : SY/MD
Sample : N5592-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

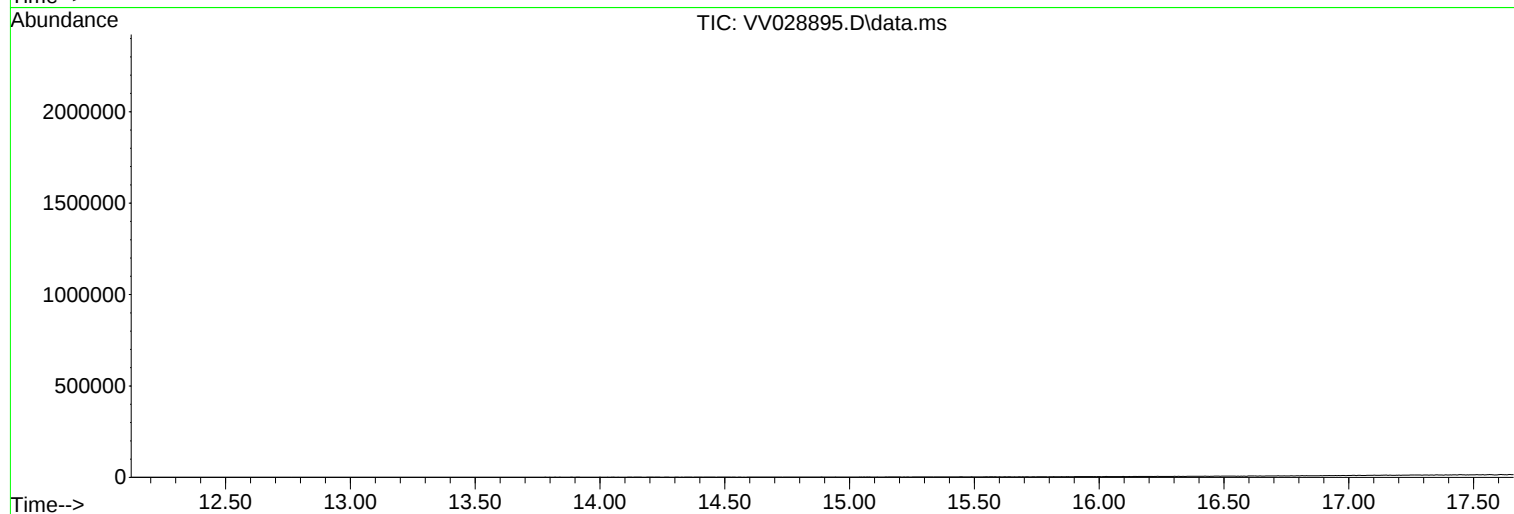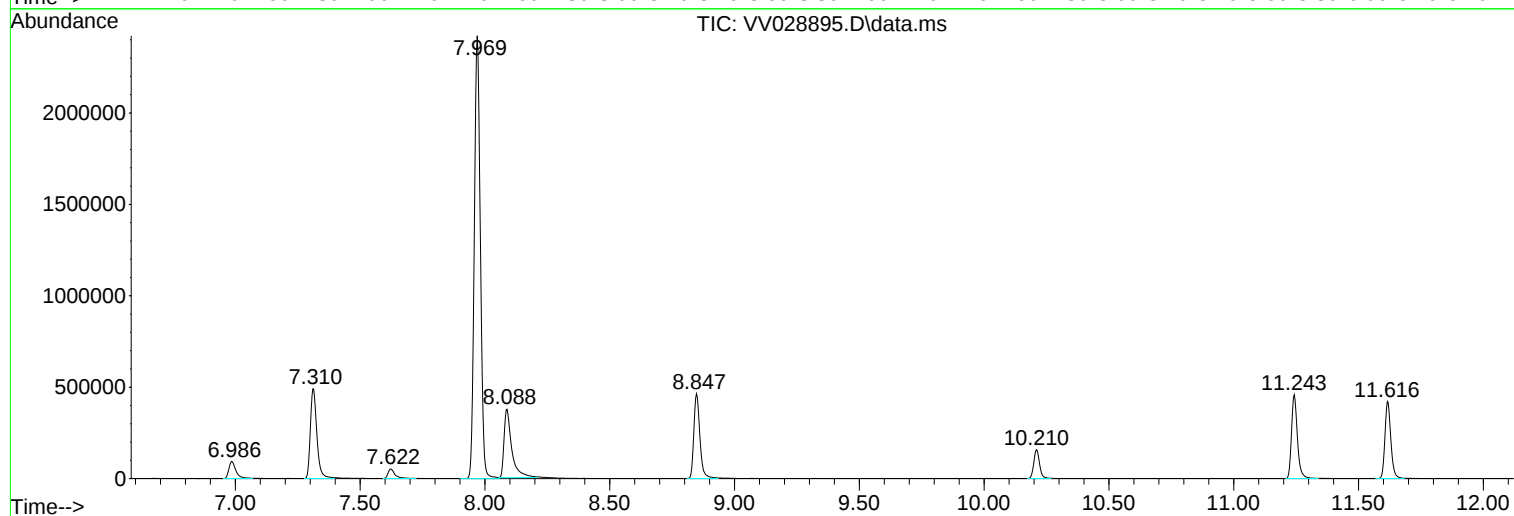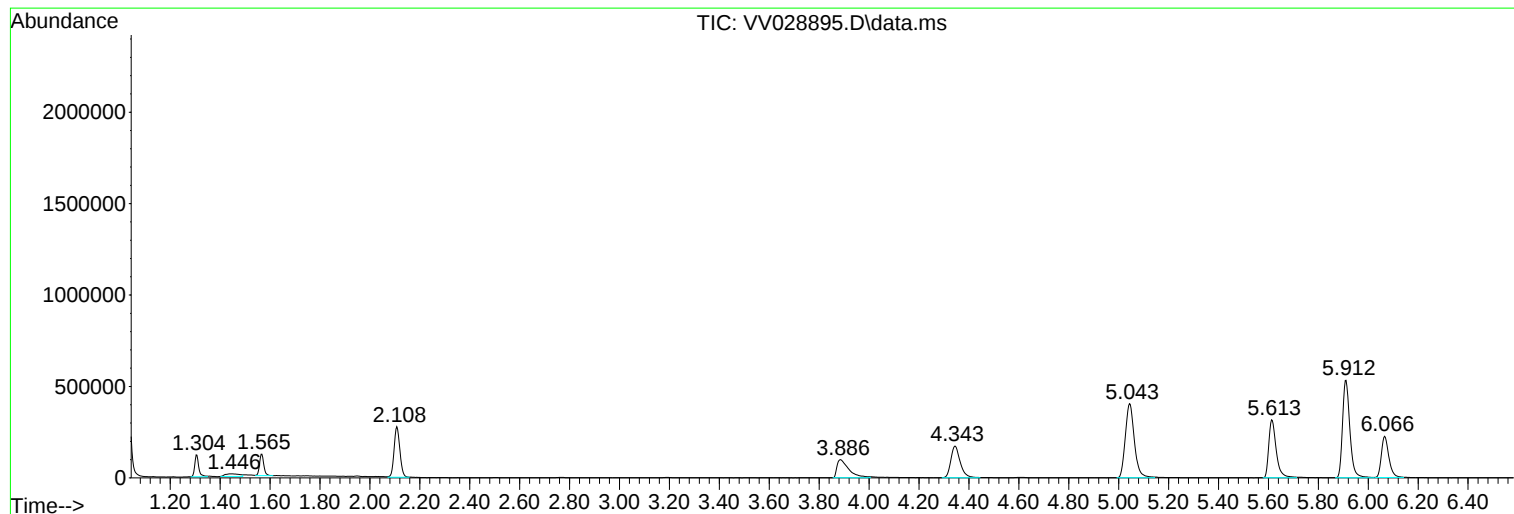

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028895.D
Acq On : 11 Nov 2022 23:17
Operator : SY/MD
Sample : N5592-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028895.D
Acq On : 11 Nov 2022 23:17
Operator : SY/MD
Sample : N5592-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc