

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028898.D
 Acq On : 12 Nov 2022 00:31
 Operator : SY/MD
 Sample : N5592-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AE1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rBV	118017	134057	10.69%	1.413%
2	1.471	121	134	140	rBV	7472	19064	1.52%	0.201%
3	1.568	156	164	176	rVB	117618	136321	10.87%	1.437%
4	1.751	211	221	241	rVB	962832	1253528	100.00%	13.210%
5	2.108	321	332	346	rVB	232331	339650	27.10%	3.579%
6	3.883	875	884	920	rBV	92571	293795	23.44%	3.096%
7	4.346	1011	1028	1059	rBV	173125	461004	36.78%	4.858%
8	5.043	1229	1245	1275	rBV2	402549	1007441	80.37%	10.617%
9	5.613	1408	1422	1458	rBV	319361	672441	53.64%	7.086%
10	5.915	1506	1516	1535	rVB8	4893	13009	1.04%	0.137%
11	6.066	1550	1563	1588	rBV	221187	464414	37.05%	4.894%
12	6.985	1839	1849	1879	rBV	90302	178287	14.22%	1.879%
13	7.310	1939	1950	1991	rBV	482383	889089	70.93%	9.370%
14	7.622	2037	2047	2071	rBV	50198	99141	7.91%	1.045%
15	7.973	2144	2156	2175	rBV	112326	192014	15.32%	2.024%
16	8.088	2182	2192	2239	rBV	363797	827642	66.03%	8.722%
17	8.847	2417	2428	2461	rBV	464949	791469	63.14%	8.341%
18	10.210	2839	2852	2870	rBV	156802	254716	20.32%	2.684%
19	11.243	3160	3173	3197	rBV	455773	748594	59.72%	7.889%
20	11.615	3278	3289	3317	rBV	433335	713383	56.91%	7.518%




Sum of corrected areas: 9489059

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028898.D
Acq On : 12 Nov 2022 00:31
Operator : SY/MD
Sample : N5592-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

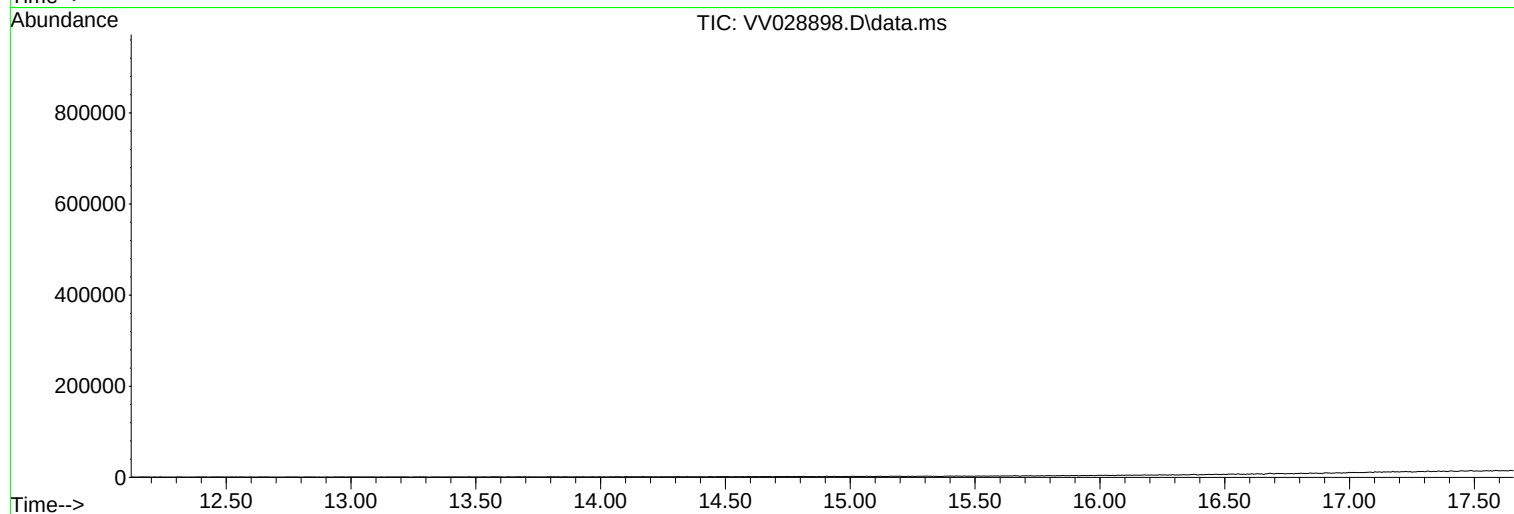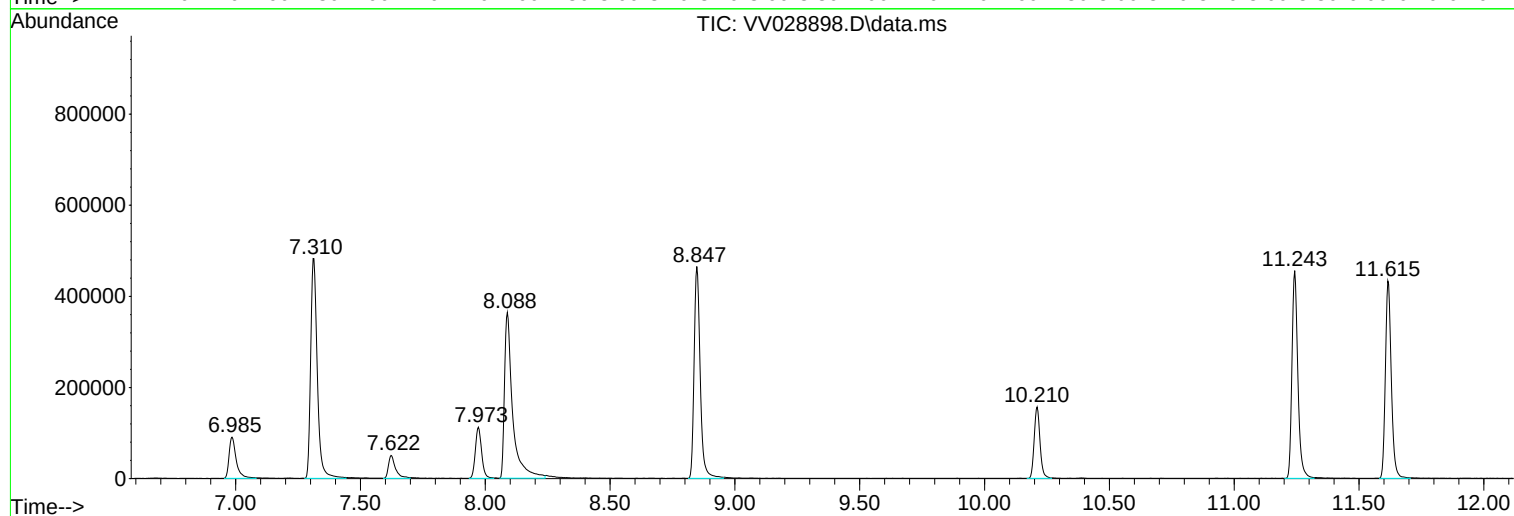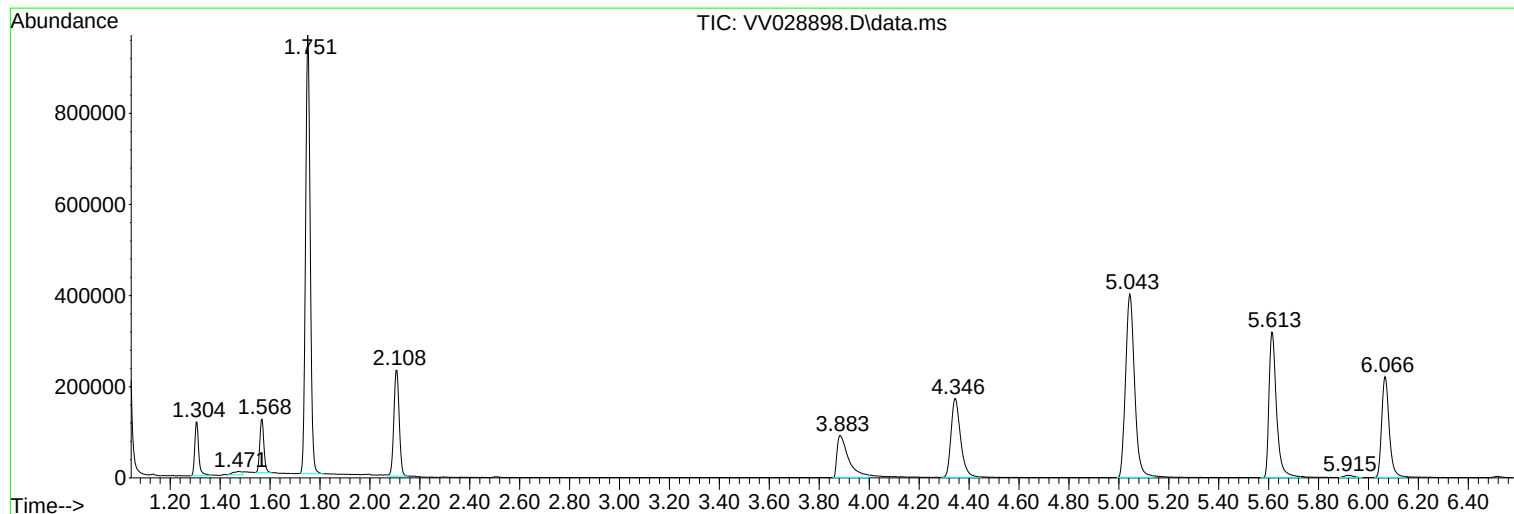

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028898.D
Acq On : 12 Nov 2022 00:31
Operator : SY/MD
Sample : N5592-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028898.D
Acq On : 12 Nov 2022 00:31
Operator : SY/MD
Sample : N5592-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc