

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028903.D
 Acq On : 12 Nov 2022 02:58
 Operator : SY/MD
 Sample : N5590-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBMY6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.211	45	53	57	rBV2	41874	43220	1.53%	0.128%
2	1.240	57	62	75	rVV	92764	110444	3.92%	0.328%
3	1.304	75	82	96	rVV	121765	132257	4.69%	0.393%
4	1.413	109	116	123	rBV	33531	37916	1.35%	0.113%
5	1.519	142	149	157	rBV	88990	106501	3.78%	0.316%
6	1.564	157	163	177	rVB	115325	138056	4.90%	0.410%
7	1.751	211	221	235	rBV	387153	500451	17.76%	1.487%
8	2.111	321	333	344	rBV3	361022	612855	21.74%	1.821%
9	2.179	344	354	378	rVV2	80470	203545	7.22%	0.605%
10	2.291	378	389	409	rVB	260972	390457	13.85%	1.160%
11	2.503	444	455	472	rBV	111257	184280	6.54%	0.547%
12	2.764	520	536	562	rBV	331977	703080	24.95%	2.089%
13	3.185	650	667	693	rBV	311133	663407	23.54%	1.971%
14	3.889	875	886	899	rBV	105840	294816	10.46%	0.876%
15	3.963	899	909	955	rVB	201665	654972	23.24%	1.946%
16	4.342	1011	1027	1060	rBV	174183	450592	15.99%	1.339%
17	4.603	1084	1108	1118	rBV	321967	803560	28.51%	2.387%
18	4.674	1118	1130	1157	rVB	620459	1547857	54.92%	4.599%
19	5.043	1228	1245	1261	rBV2	413972	1025437	36.38%	3.046%
20	5.127	1261	1271	1299	rVB	155446	355837	12.63%	1.057%
21	5.616	1411	1423	1453	rBV	282583	589584	20.92%	1.752%
22	5.912	1503	1515	1544	rBV	304756	610455	21.66%	1.814%
23	6.066	1550	1563	1571	rBV	229791	441993	15.68%	1.313%
24	6.127	1572	1582	1592	rVV	429475	821163	29.14%	2.440%
25	6.985	1836	1849	1869	rBV2	93100	179803	6.38%	0.534%
26	7.313	1939	1951	1962	rBV	496462	878259	31.16%	2.609%
27	7.381	1962	1972	1999	rVB	1035735	1795106	63.69%	5.333%
28	7.622	2037	2047	2062	rBV	53884	96825	3.44%	0.288%
29	7.969	2138	2155	2177	rBV	647975	1084444	38.48%	3.222%
30	8.085	2181	2191	2200	rBV	449757	797823	28.31%	2.370%
31	8.137	2200	2207	2238	rVB	499748	961947	34.13%	2.858%
32	8.346	2261	2272	2295	rVB	292231	494115	17.53%	1.468%
33	8.873	2416	2436	2454	rBV2	1120228	2495532	88.54%	7.414%
34	8.969	2455	2466	2471	rVV	364664	604647	21.45%	1.796%
35	9.005	2471	2477	2505	rVV	899933	1437134	50.99%	4.270%
36	9.133	2506	2517	2562	rVB	1815090	2818446	100.00%	8.373%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028903.D
 Acq On : 12 Nov 2022 02:58
 Operator : SY/MD
 Sample : N5590-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBMY6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

37	9.545	2628	2645	2686	rBV3	926769	2175800	77.20%	6.464%
38	9.725	2690	2701	2719	rVV	86584	147339	5.23%	0.438%
39	9.924	2751	2763	2794	rBV	500500	784947	27.85%	2.332%
40	10.210	2837	2852	2872	rBV	170134	271465	9.63%	0.806%
41	11.243	3162	3173	3176	rBV	489540	684692	24.29%	2.034%
42	11.632	3277	3294	3315	rBV2	1256801	2554370	90.63%	7.589%
43	12.423	3530	3540	3555	rBV2	29832	48788	1.73%	0.145%
44	12.635	3595	3606	3624	rBV	543419	845494	30.00%	2.512%
45	13.734	3935	3948	3966	rBV	693320	1080241	38.33%	3.209%




Sum of corrected areas: 33659952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028903.D
Acq On : 12 Nov 2022 02:58
Operator : SY/MD
Sample : N5590-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBMY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

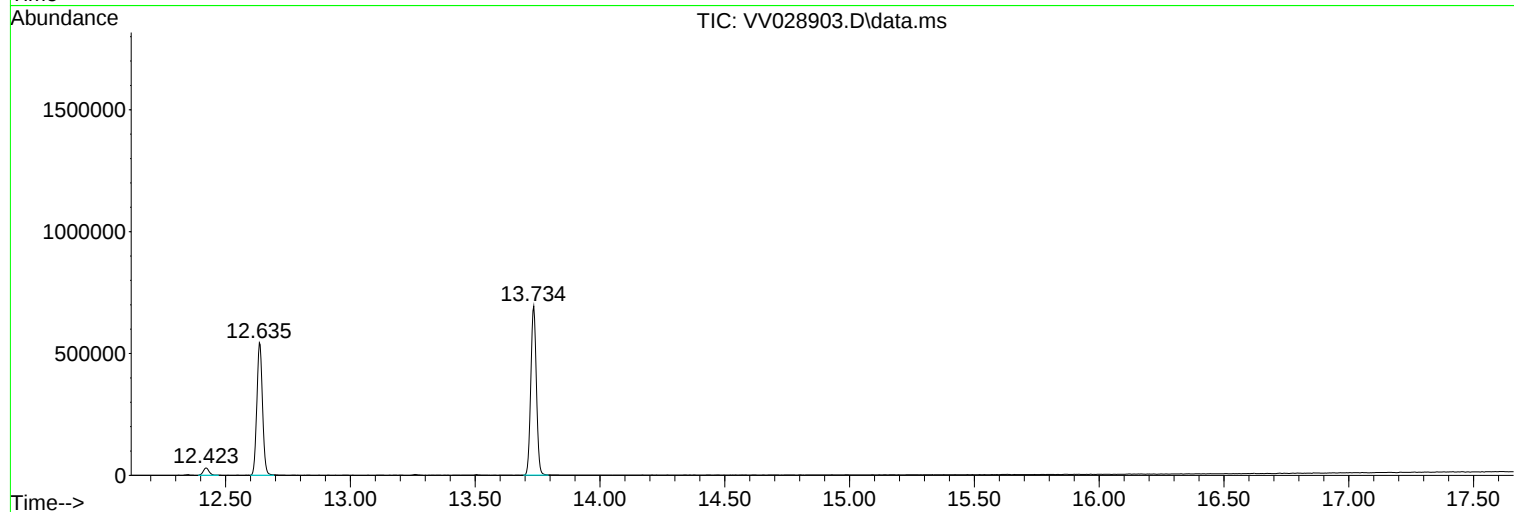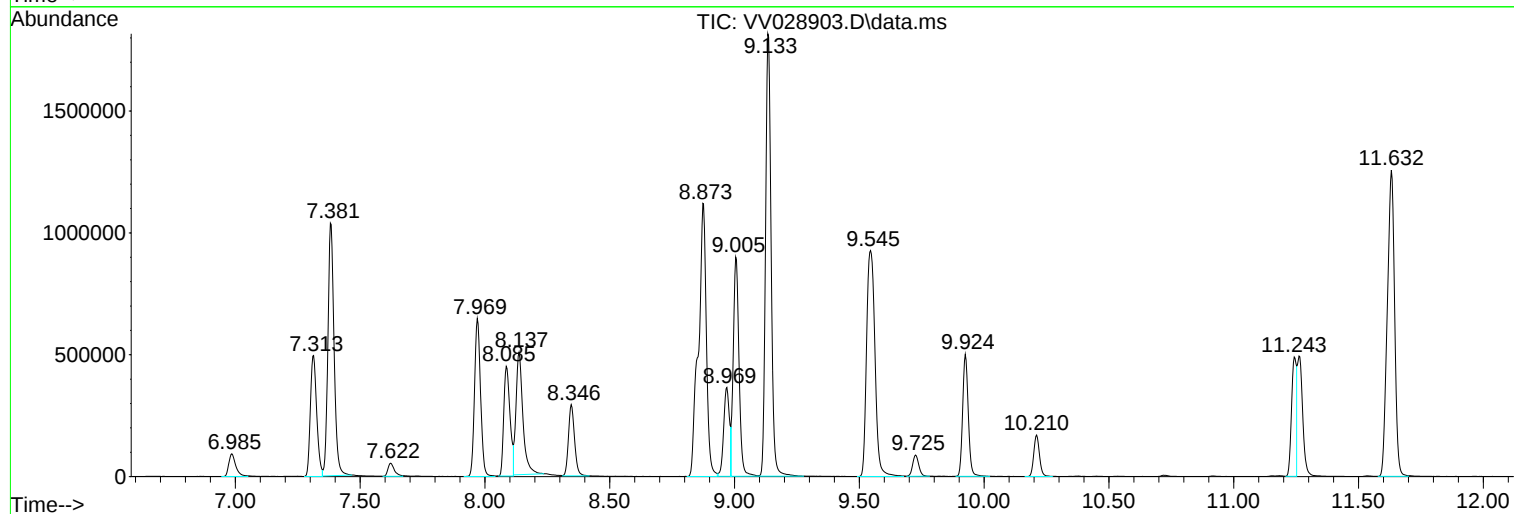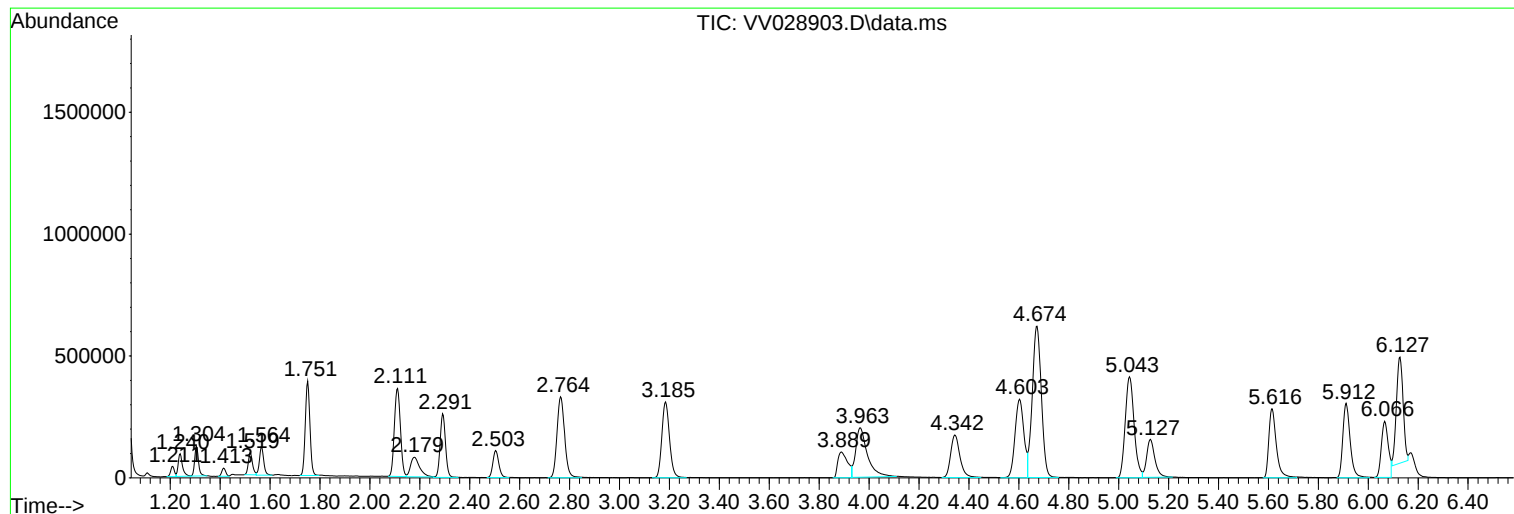

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028903.D
Acq On : 12 Nov 2022 02:58
Operator : SY/MD
Sample : N5590-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBMY6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1,3,5-trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.635	6.17 ug/L	845494	1,4-Dichlorobenzene-d4	11.243

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
3			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
4			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
5			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	97

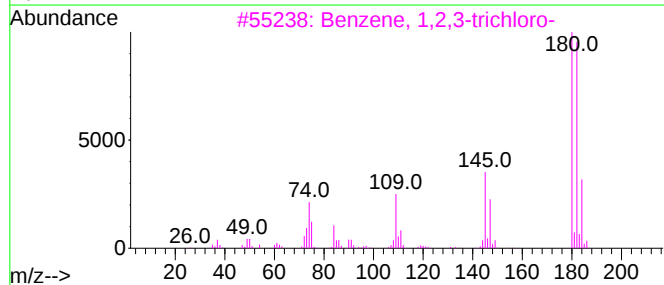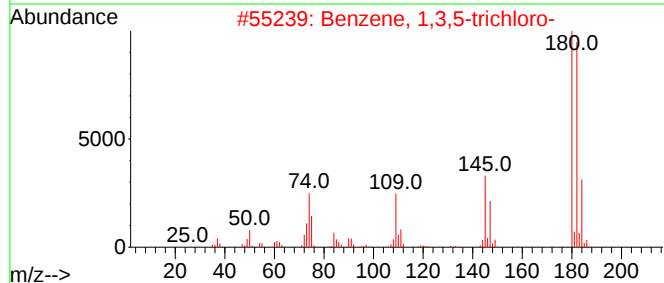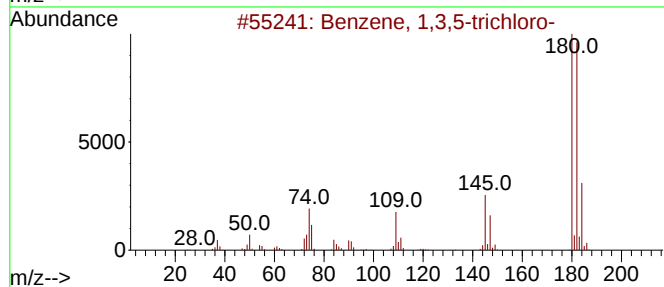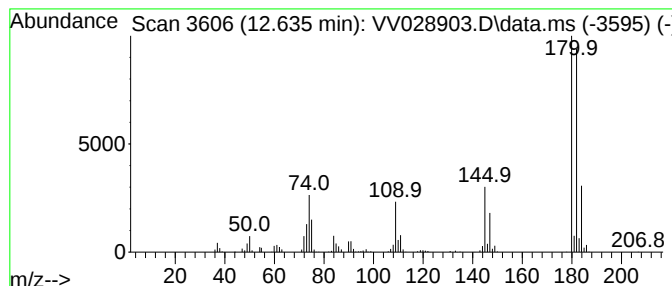

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028903.D
Acq On : 12 Nov 2022 02:58
Operator : SY/MD
Sample : N5590-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBMY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	12.635	6.2	ug/L	845494	3	11.243	684692	5.0