

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028915.D
 Acq On : 12 Nov 2022 07:54
 Operator : SY/MD
 Sample : N5602-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	103	rVB2	145364	165707	16.00%	1.855%
2	1.413	110	116	124	rVB	16385	18530	1.79%	0.207%
3	1.568	155	164	176	rBV	118546	142444	13.75%	1.594%
4	2.105	320	331	347	rVB	232403	348178	33.62%	3.897%
5	2.764	525	536	544	rBV7	5973	10478	1.01%	0.117%
6	3.905	876	891	937	rBV2	306603	925362	89.35%	10.358%
7	4.342	1011	1027	1052	rBV	171301	427862	41.31%	4.789%
8	5.043	1228	1245	1281	rBV2	405630	1035683	100.00%	11.593%
9	5.612	1410	1422	1453	rBV	336288	695889	67.19%	7.789%
10	5.918	1504	1517	1538	rBV4	18361	40169	3.88%	0.450%
11	6.066	1550	1563	1597	rBV	227409	471518	45.53%	5.278%
12	6.985	1837	1849	1876	rBV	88634	173951	16.80%	1.947%
13	7.310	1939	1950	1972	rBV	477297	869157	83.92%	9.729%
14	7.622	2037	2047	2066	rBV	49049	92032	8.89%	1.030%
15	8.088	2181	2192	2231	rBV2	383711	863525	83.38%	9.666%
16	8.847	2416	2428	2454	rBV	481565	806674	77.89%	9.029%
17	10.210	2840	2852	2875	rBV	160497	259605	25.07%	2.906%
18	11.242	3158	3173	3200	rBV	482787	781748	75.48%	8.750%
19	11.615	3277	3289	3311	rBV	440224	717395	69.27%	8.030%
20	16.168	4694	4705	4715	rBV3	32271	57468	5.55%	0.643%
21	16.297	4737	4745	4757	rVB2	20888	30404	2.94%	0.340%




Sum of corrected areas: 8933779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028915.D
Acq On : 12 Nov 2022 07:54
Operator : SY/MD
Sample : N5602-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

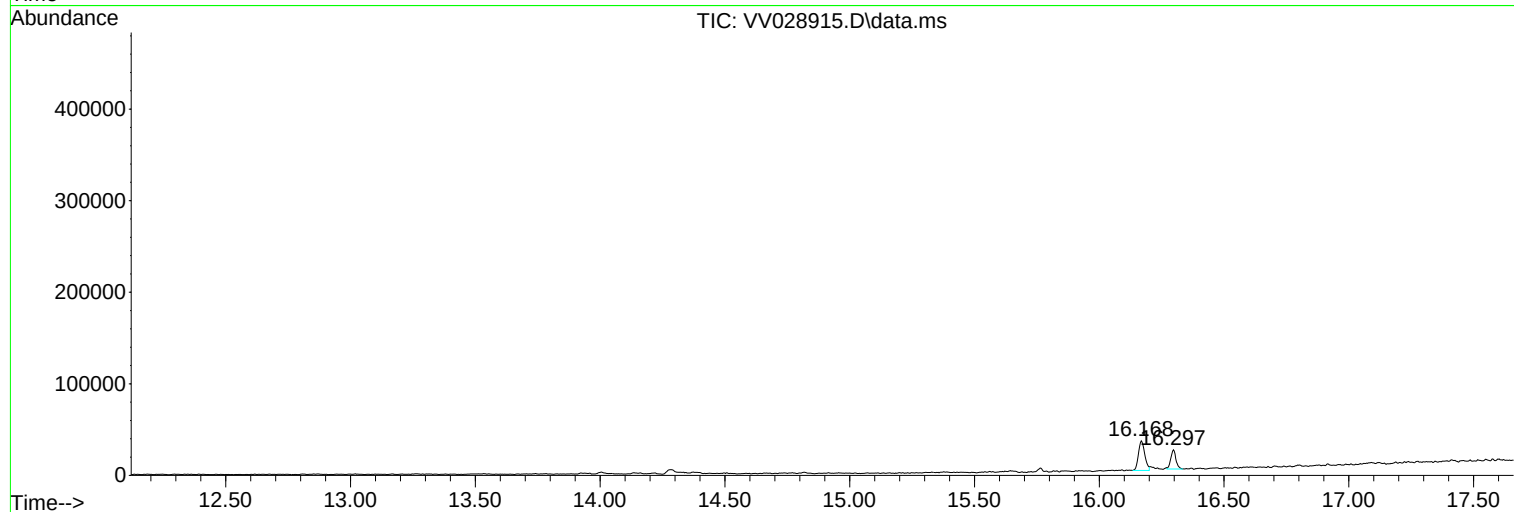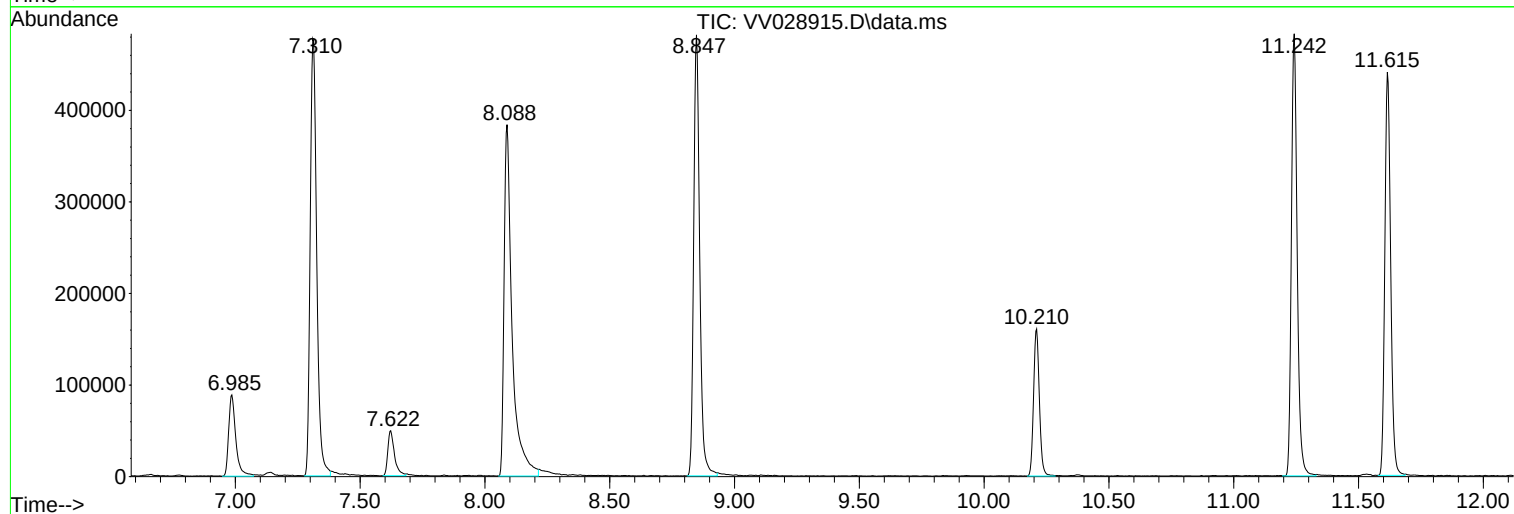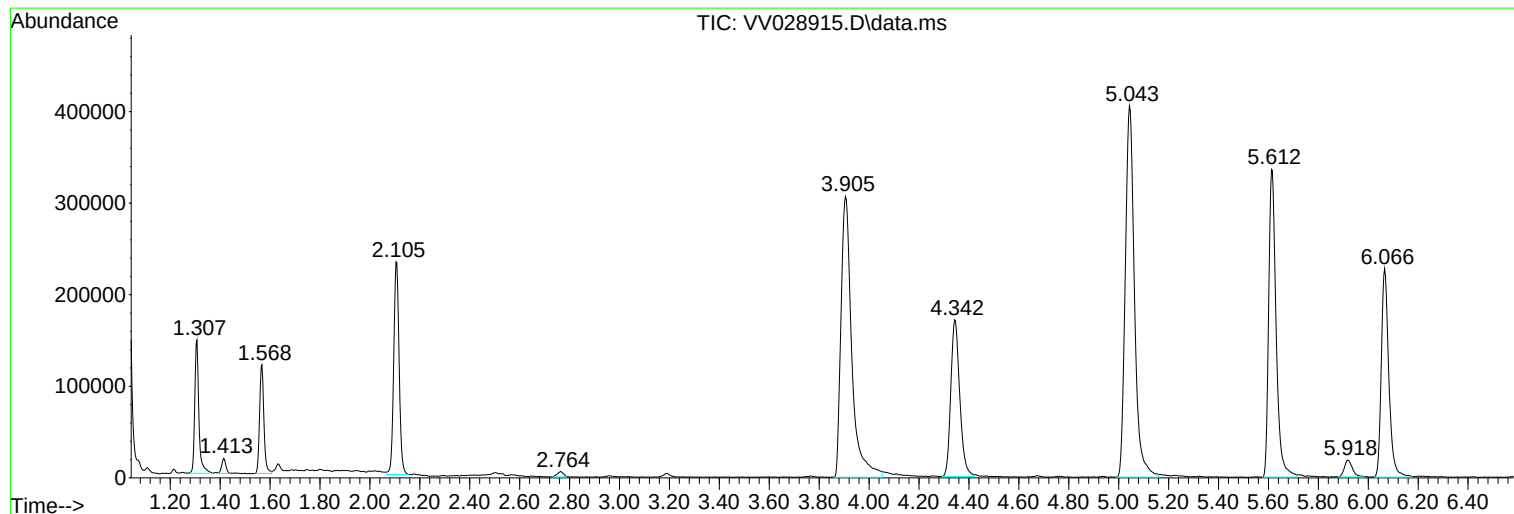

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028915.D
Acq On : 12 Nov 2022 07:54
Operator : SY/MD
Sample : N5602-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028915.D
Acq On : 12 Nov 2022 07:54
Operator : SY/MD
Sample : N5602-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
