

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028916.D
 Acq On : 12 Nov 2022 08:18
 Operator : SY/MD
 Sample : N5602-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	102	rBV	122355	133416	13.12%	1.611%
2	1.413	110	116	124	rVB	15260	17121	1.68%	0.207%
3	1.565	156	163	177	rVB	118273	135520	13.32%	1.637%
4	2.105	320	331	345	rVB	230678	332055	32.64%	4.010%
5	3.892	878	887	923	rBV	64766	246618	24.24%	2.978%
6	4.343	1012	1027	1056	rVB	169358	425498	41.83%	5.138%
7	5.044	1226	1245	1278	rBV2	403129	1017242	100.00%	12.284%
8	5.613	1409	1422	1458	rBV	325886	683149	67.16%	8.250%
9	5.918	1506	1517	1537	rVB8	9849	23068	2.27%	0.279%
10	6.066	1550	1563	1584	rBV	221125	462158	45.43%	5.581%
11	6.982	1837	1848	1880	rBV	88905	176411	17.34%	2.130%
12	7.310	1938	1950	1974	rBV	484856	874234	85.94%	10.557%
13	7.622	2037	2047	2065	rBV	47959	90014	8.85%	1.087%
14	8.088	2181	2192	2241	rBV2	335350	860554	84.60%	10.392%
15	8.847	2416	2428	2459	rBV	470444	793937	78.05%	9.588%
16	9.101	2497	2507	2517	rVB4	5763	10269	1.01%	0.124%
17	10.211	2838	2852	2871	rBV	157129	261940	25.75%	3.163%
18	11.243	3160	3173	3199	rBV	479380	775176	76.20%	9.361%
19	11.529	3252	3262	3277	rBV2	15413	31922	3.14%	0.385%
20	11.616	3277	3289	3315	rVB	446037	736693	72.42%	8.896%
21	12.542	3568	3577	3590	rBV4	8409	13457	1.32%	0.163%
22	12.747	3633	3641	3650	rVB3	10264	14367	1.41%	0.173%
23	13.831	3971	3978	3989	rVB3	8809	14159	1.39%	0.171%
24	14.281	4110	4118	4130	rBV3	6430	10532	1.04%	0.127%
25	14.664	4227	4237	4245	rBV3	6889	10639	1.05%	0.128%
26	15.857	4588	4608	4610	rBV5	37129	77477	7.62%	0.936%
27	16.168	4697	4705	4718	rVB5	24457	41407	4.07%	0.500%
28	16.297	4738	4745	4754	rVB2	7575	11803	1.16%	0.143%




Sum of corrected areas: 8280836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028916.D
Acq On : 12 Nov 2022 08:18
Operator : SY/MD
Sample : N5602-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

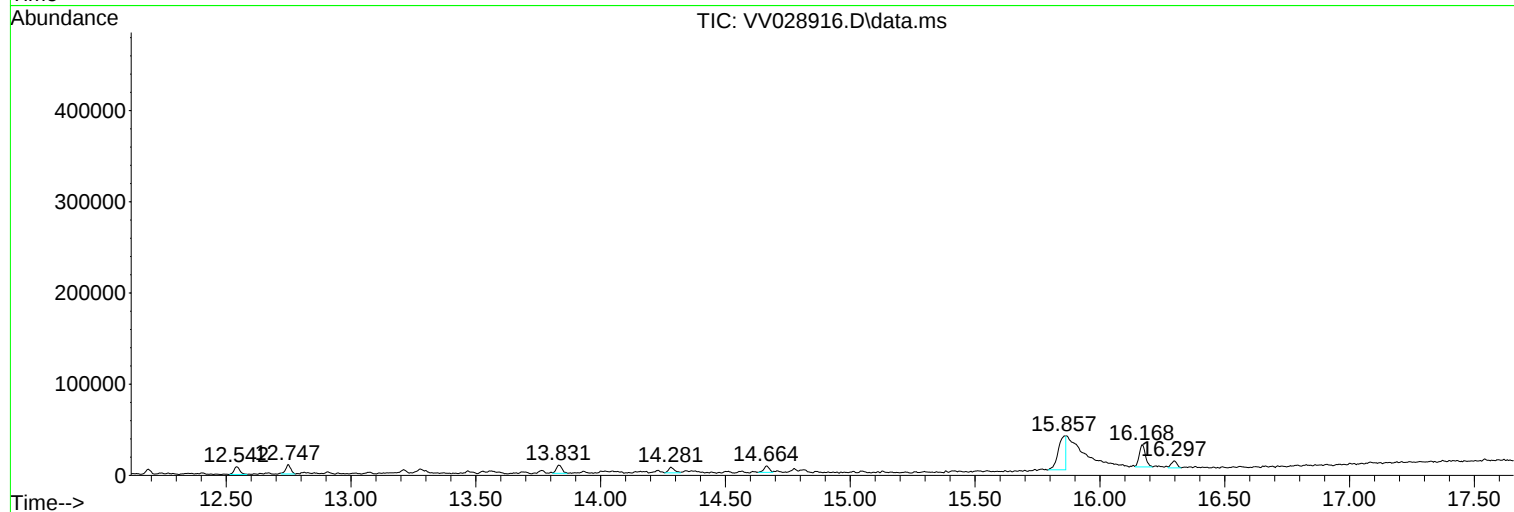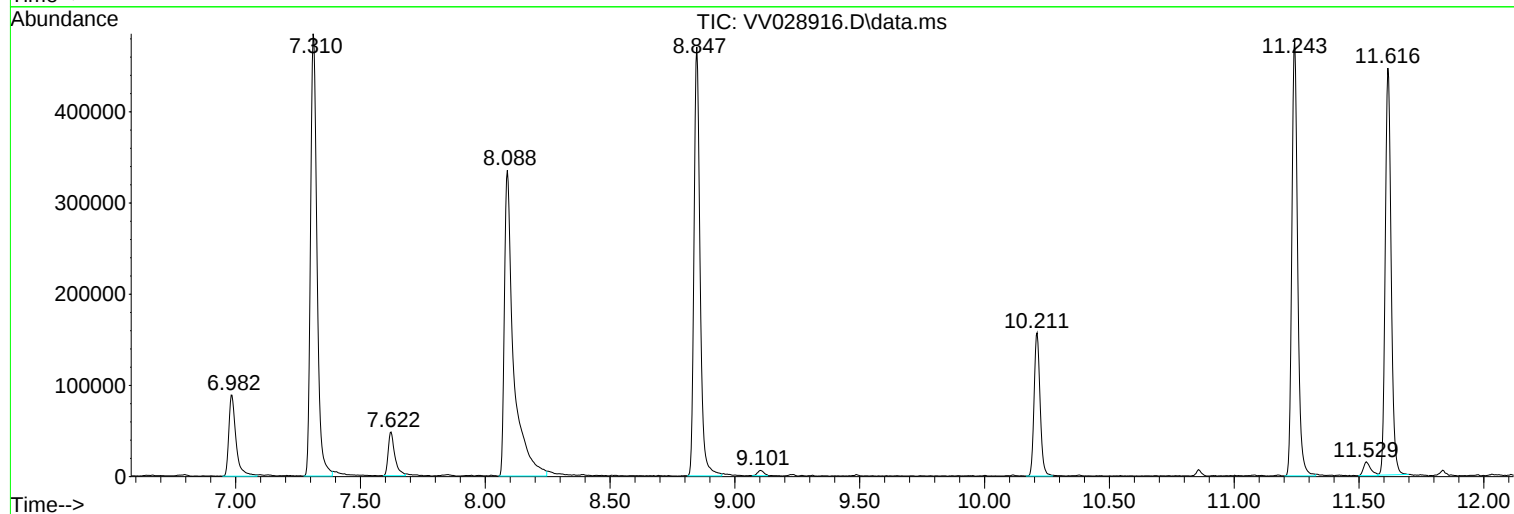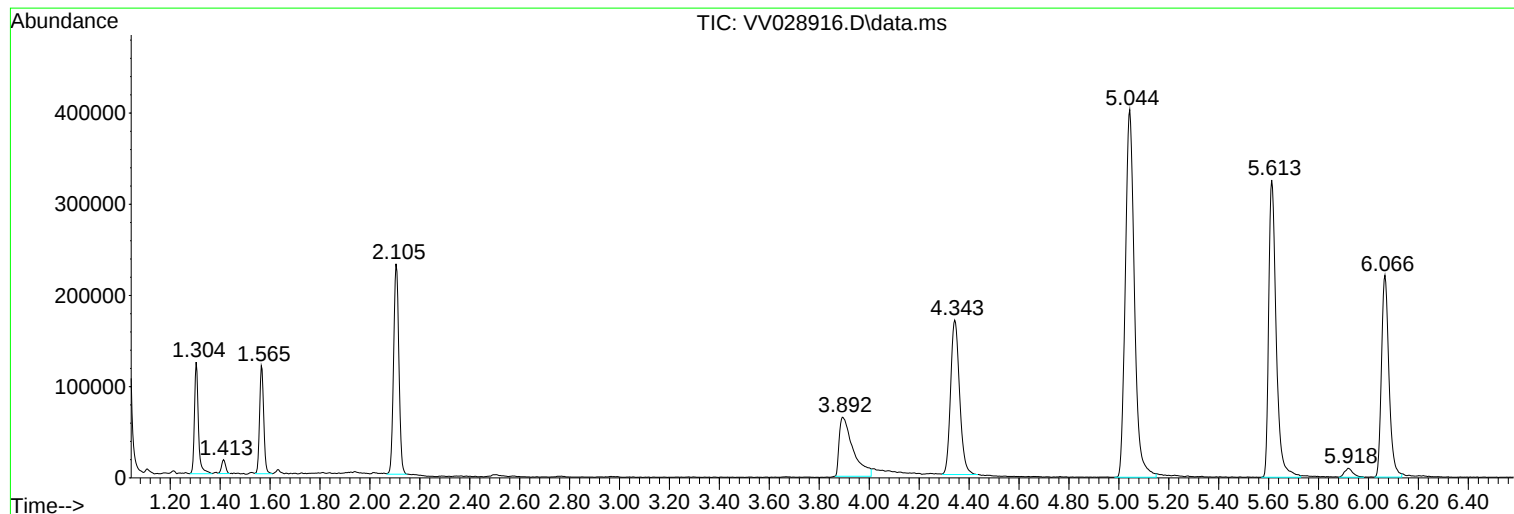

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028916.D
Acq On : 12 Nov 2022 08:18
Operator : SY/MD
Sample : N5602-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
Data File : VV028916.D
Acq On : 12 Nov 2022 08:18
Operator : SY/MD
Sample : N5602-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc