
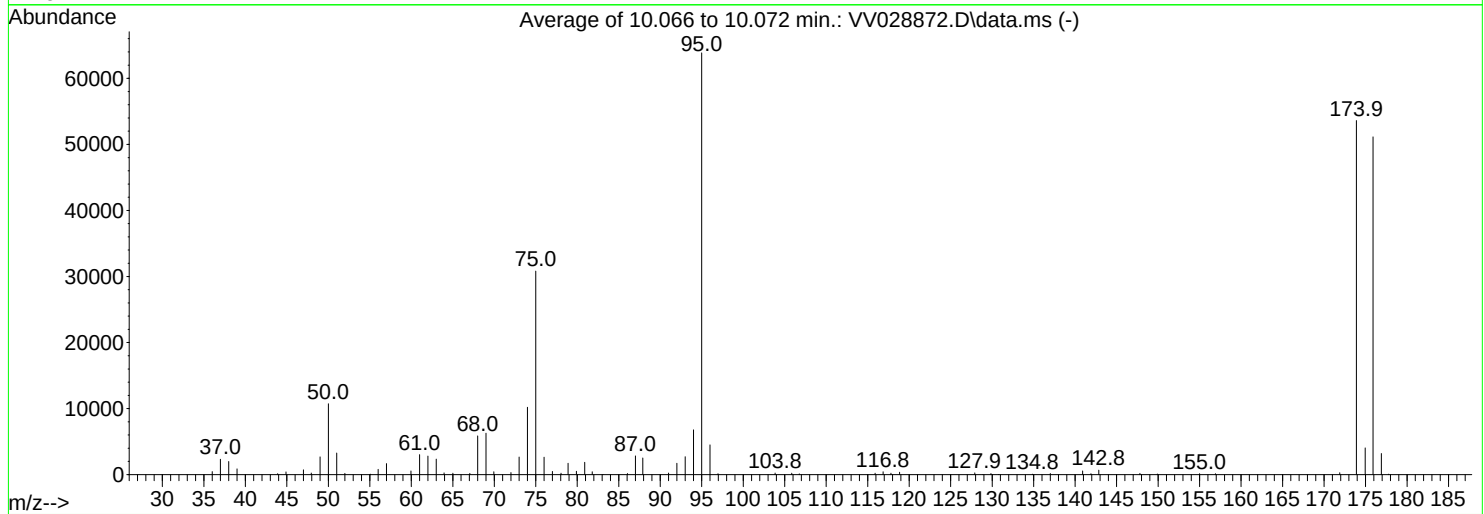


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111122\
 Data File : VV028872.D
 Acq On : 11 Nov 2022 11:53
 Operator : SY/MD
 Sample : BFB394
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB394

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Nov 16 03:16:14 2022

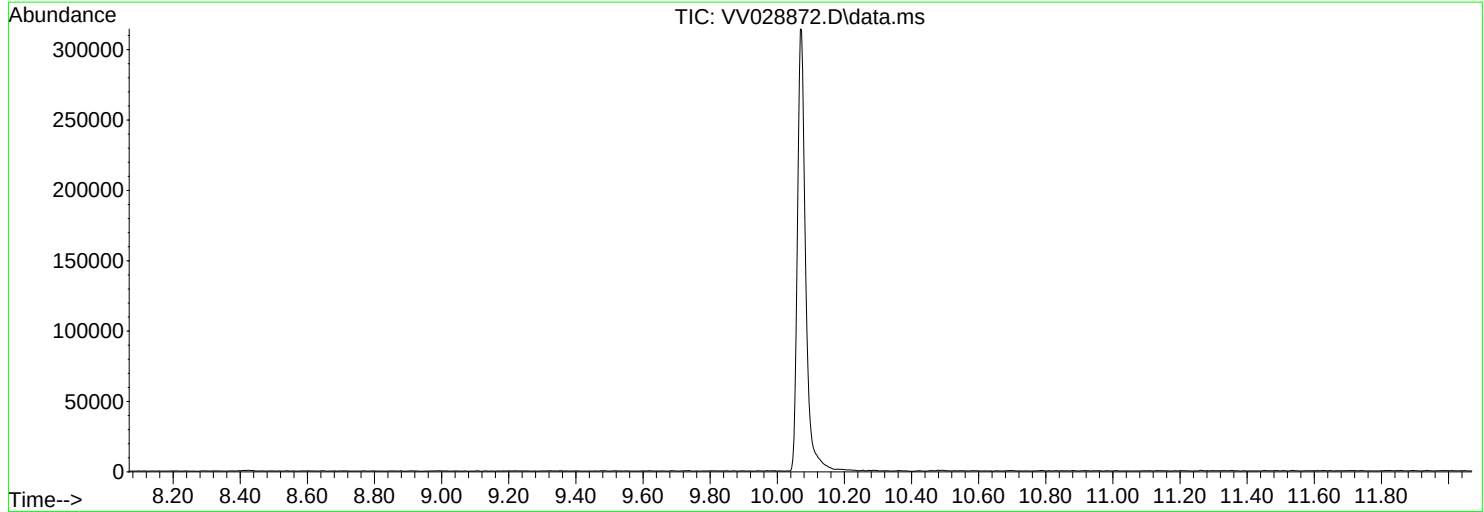

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	10731	PASS
75	95	30	80	48.3	30824	PASS
95	95	100	100	100.0	63859	PASS
96	95	5	9	7.1	4518	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	53613	PASS
175	174	5	9	7.6	4052	PASS
176	174	95	105	95.4	51128	PASS
177	176	5	10	6.2	3192	PASS

m/z	Abundance
39.90	216.0
43.90	483.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
36.00	477.0
37.00	2142.0
38.00	1793.0
39.00	839.0
39.90	227.0
43.90	621.0
44.90	434.0
47.00	844.0
47.90	271.0
49.00	2557.0
50.00	10228.0
51.00	3077.0
52.10	165.0
56.00	789.0
57.00	1593.0
59.90	513.0
61.00	2665.0
62.00	2682.0
63.00	2256.0
63.90	241.0
64.90	218.0
67.00	197.0
68.00	5381.0
69.00	5968.0
69.90	452.0
72.00	301.0
73.00	2494.0
74.00	9329.0
75.00	28640.0
76.00	2455.0
77.00	473.0
78.10	199.0
78.90	1598.0
79.90	432.0
80.90	1722.0
81.80	402.0
86.00	186.0
87.00	2760.0
87.90	2386.0
91.00	292.0
92.00	1760.0
93.00	2772.0
94.00	6259.0
95.00	59880.0
96.00	4193.0
97.00	131.0
103.90	241.0
105.90	205.0
106.70	110.0
115.90	160.0
116.90	359.0
117.80	221.0
118.90	342.0
127.90	220.0
128.90	105.0
129.80	195.0
137.00	143.0
140.90	475.0
141.90	118.0
142.80	579.0
147.80	187.0
149.90	144.0
155.00	136.0
156.90	107.0
171.90	244.0
173.90	48960.0
175.00	3651.0
175.90	46656.0
176.90	3159.0
177.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
36.00	456.0
37.00	2401.0
38.00	2047.0
39.00	899.0
39.80	199.0
44.00	622.0
44.90	449.0
47.00	734.0
47.90	234.0
49.00	2871.0
50.00	11118.0
51.00	3400.0
52.00	192.0
55.10	115.0
56.00	835.0
57.00	1747.0
60.00	579.0
61.00	3152.0
62.00	2950.0
63.00	2518.0
64.00	296.0
65.00	219.0
67.00	213.0
68.00	6092.0
69.00	6531.0
70.00	443.0
72.00	315.0
73.00	2756.0
74.00	10664.0
75.00	31808.0
76.00	2720.0
77.00	508.0
78.10	231.0
78.90	1790.0
79.90	520.0
80.90	1945.0
81.80	456.0
83.10	104.0
86.10	171.0
87.00	2995.0
87.90	2622.0
91.00	254.0
92.00	1726.0
93.00	2772.0
94.00	7021.0
95.00	66200.0
96.00	4782.0
96.90	163.0
103.80	244.0
105.90	224.0
106.80	127.0
115.90	211.0
116.90	458.0
117.80	239.0
118.90	400.0
127.90	266.0
129.80	180.0
130.80	117.0
134.80	107.0
137.00	183.0
140.90	568.0
141.90	158.0
142.90	709.0
147.80	197.0
149.90	127.0
155.00	151.0
156.90	151.0
171.90	305.0
173.90	55448.0
175.00	4163.0
175.90	52752.0
176.90	3262.0
177.80	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
36.00	429.0
37.00	2416.0
38.00	2094.0
39.00	873.0
39.90	164.0
43.90	643.0
44.90	389.0
47.00	636.0
48.00	207.0
49.00	2621.0
50.00	10848.0
51.00	3371.0
51.90	195.0
55.00	147.0
56.00	810.0
57.00	1700.0
60.00	593.0
61.00	3289.0
62.00	2816.0
63.00	2294.0
64.00	295.0
65.10	208.0
67.10	187.0
68.00	6139.0
69.00	6295.0
69.90	436.0
72.00	331.0
73.00	2733.0
74.00	10600.0
75.00	32024.0
76.00	2729.0
77.00	500.0
78.00	217.0
78.90	1771.0
79.90	555.0
80.90	1912.0
81.80	450.0
86.00	155.0
87.00	2727.0
87.90	2580.0
91.00	184.0
92.00	1677.0
93.00	2604.0
94.00	7069.0
95.00	65496.0
96.00	4579.0
96.90	157.0
103.80	259.0
105.80	240.0
106.80	108.0
115.90	262.0
116.80	512.0
117.80	228.0
118.80	375.0
127.90	281.0
129.90	174.0
134.90	103.0
137.00	161.0
140.90	601.0
141.90	172.0
142.90	782.0
147.80	199.0
155.00	140.0
156.90	156.0
171.90	329.0
173.90	56432.0
174.90	4341.0
175.90	53976.0
176.90	3156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394