

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111219\
 Data File : VV013586.D
 Acq On : 12 Nov 2019 13:50
 Operator : SY/MD
 Sample : K5743-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Nov 13 05:28:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 13 04:27:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	382806	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	390062	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	165008	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72494	4.49	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.80%
7) Chloroethane-d5	1.58	69	78684	5.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.80%
11) 1,1-Dichloroethene-d2	2.13	63	94458	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	3.94	46	265781	45.95	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.90%
24) Chloroform-d	4.40	84	235535	5.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.60%
26) 1,2-Dichloroethane-d4	5.08	65	118926	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.60%
32) Benzene-d6	5.09	84	389220	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
36) 1,2-Dichloropropane-d6	6.11	67	137579	5.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.20%
41) Toluene-d8	7.36	98	284489	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.20%
43) trans-1,3-Dichloropropene-	7.66	79	48033	4.69	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.80%
46) 2-Hexanone-d5	8.13	63	238472	58.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.20%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	113562	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	154541	5.67	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.40%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	9079	0.301 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111219\
Data File : VV013586.D
Acq On : 12 Nov 2019 13:50
Operator : SY/MD
Sample : K5743-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Nov 13 05:28:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 13 04:27:44 2019
Response via : Initial Calibration

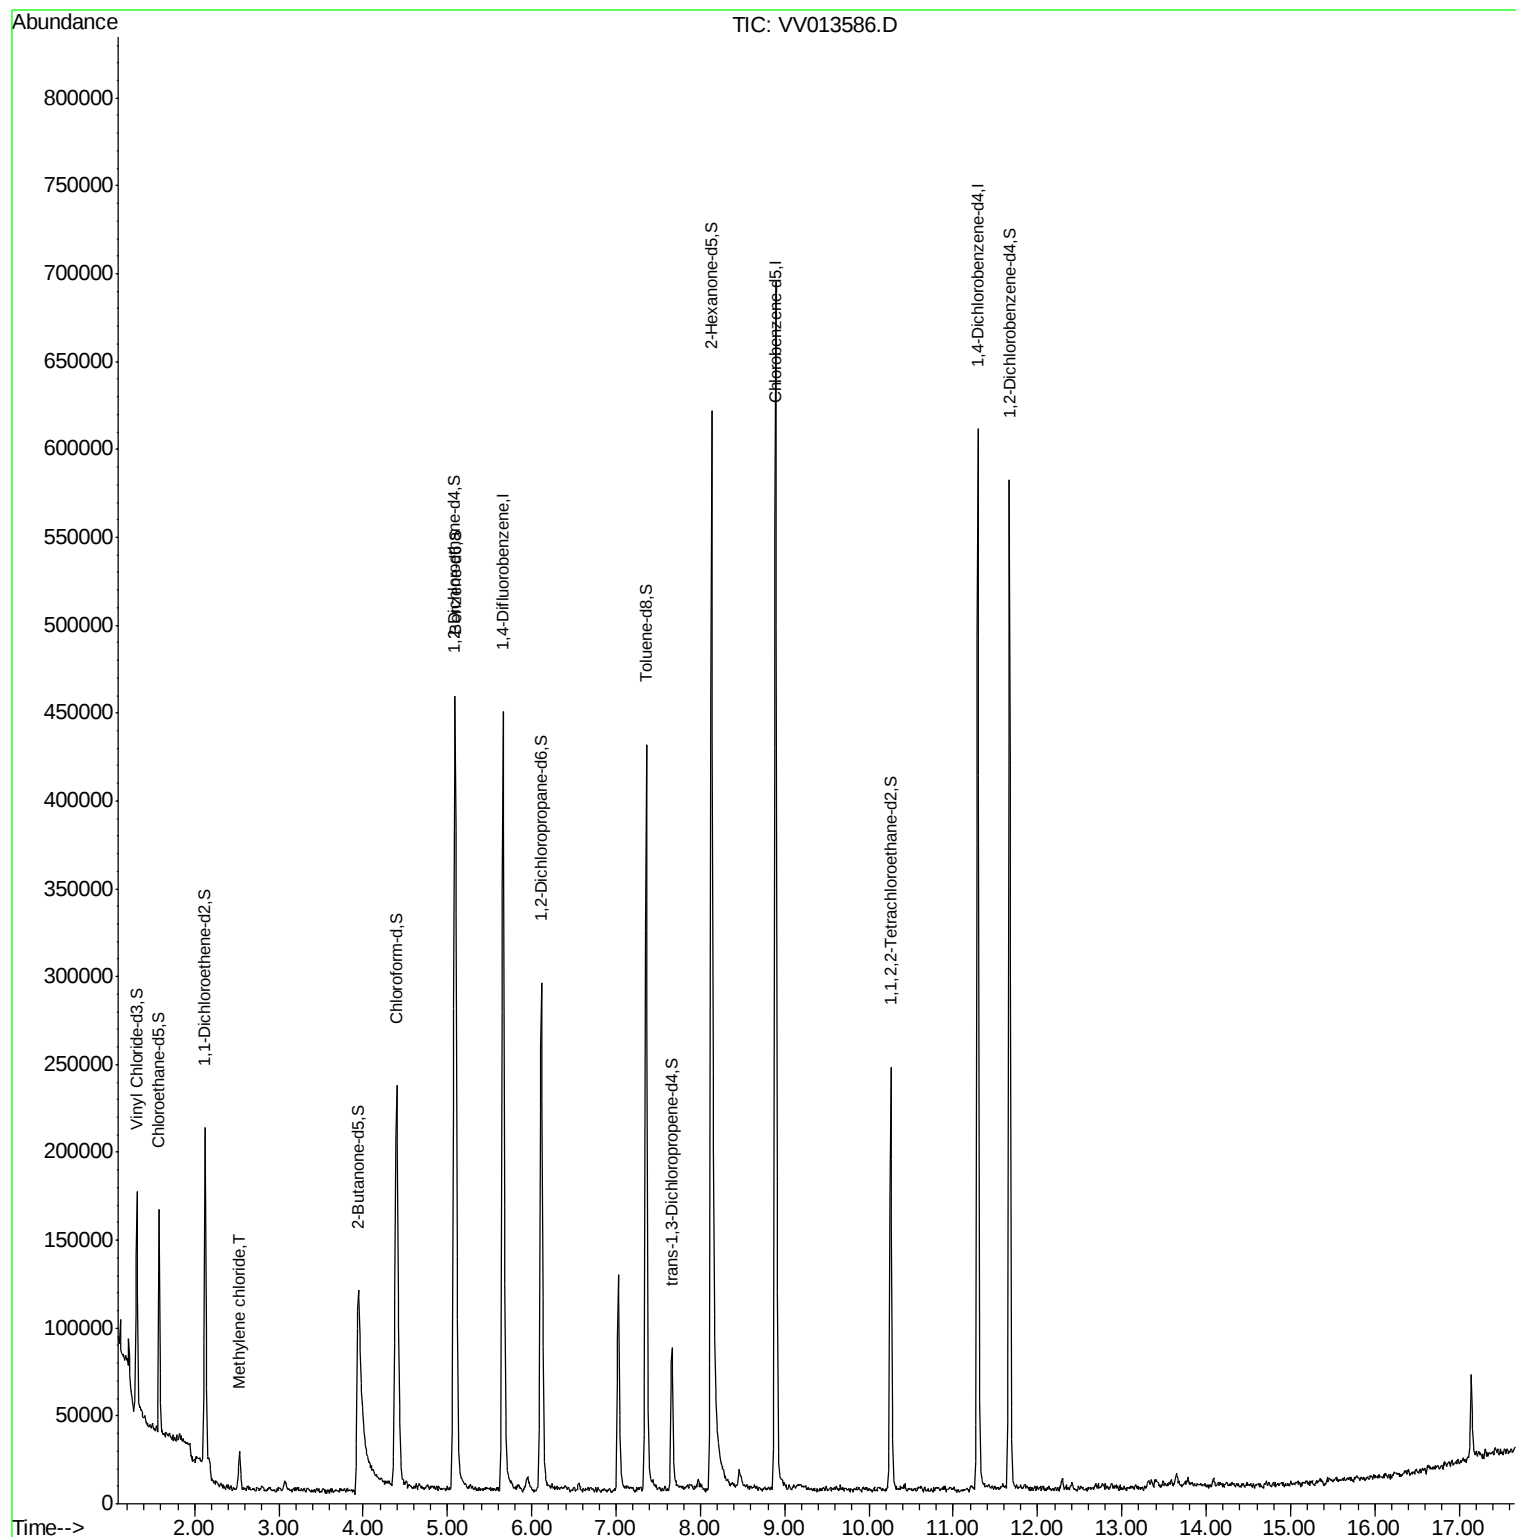

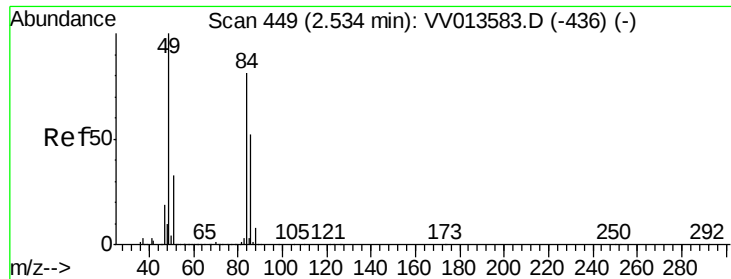

#16
 Methvlene chloride
 Concen: 0.301 ug/L
 RT: 2.53 min Scan# 448
 Delta R.T. -0.00 min
 Lab File: VV013586.D
 Acq: 12 Nov 2019 13:50

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 9079
 Ion Ratio Lower Upper
 84 100
 86 60.1 44.2 82.2
 49 115.0 88.8 164.8

