

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111219\
 Data File : VV013587.D
 Acq On : 12 Nov 2019 14:21
 Operator : SY/MD
 Sample : K5747-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Nov 13 05:31:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 13 04:27:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	376540	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	370419	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	159191	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72136	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.58	69	76654	5.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.80%
11) 1,1-Dichloroethene-d2	2.13	63	96371	3.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.40%
20) 2-Butanone-d5	3.94	46	319195	56.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.20%
24) Chloroform-d	4.40	84	226216	5.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.80%
26) 1,2-Dichloroethane-d4	5.08	65	121047	5.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.40%
32) Benzene-d6	5.09	84	371373	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	6.11	67	136935	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.35	98	267513	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
43) trans-1,3-Dichloropropene-	7.66	79	46056	4.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.60%
46) 2-Hexanone-d5	8.13	63	272535	69.92	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	139.84%#
57) 1,1,2,2-Tetrachloroethane-	10.26	84	121468	6.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	120.40%#
64) 1,2-Dichlorobenzene-d4	11.67	152	150464	5.72	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.40%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	4953	0.167 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111219\
Data File : VV013587.D
Acq On : 12 Nov 2019 14:21
Operator : SY/MD
Sample : K5747-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Nov 13 05:31:50 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 13 04:27:44 2019
Response via : Initial Calibration

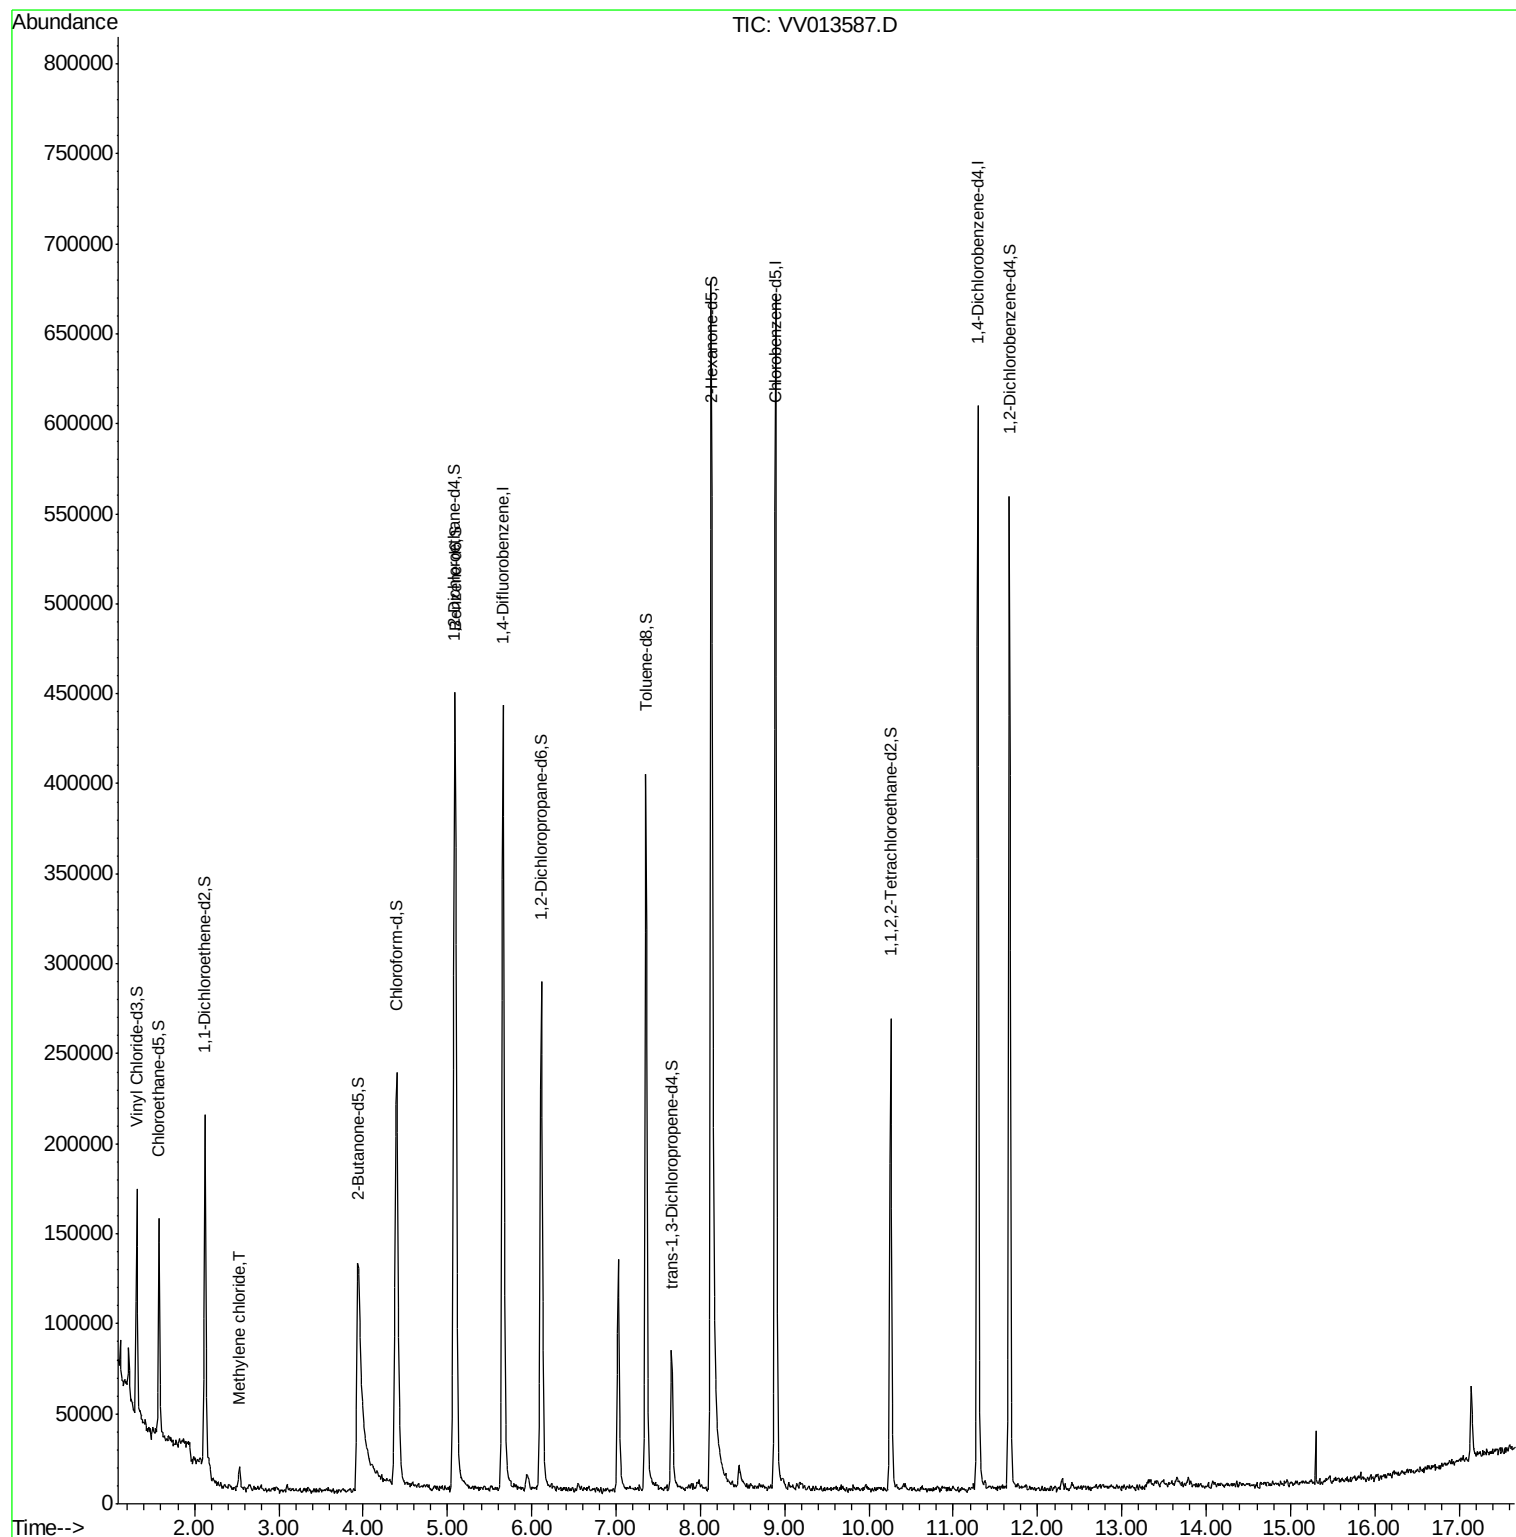

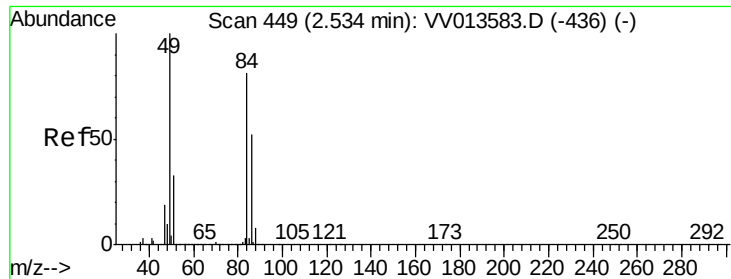

#16
 Methvlene chloride
 Concen: 0.167 ug/L
 RT: 2.53 min Scan# 448
 Delta R.T. -0.00 min
 Lab File: VV013587.D
 Acq: 12 Nov 2019 14:21

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 4953
 Ion Ratio Lower Upper
 84 100
 86 55.5 44.2 82.2
 49 124.6 88.8 164.8

