

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019353.D
 Acq On : 12 Nov 2020 15:35
 Operator : SY/MD
 Sample : VV1112MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	129321	125637	15.98%	2.009%
2	1.576	144	151	164	rBV	107496	118463	15.07%	1.895%
3	2.122	310	321	346	rVB	226019	346018	44.01%	5.534%
4	2.672	490	492	493	rBV	121	45	0.01%	0.001%
5	2.720	504	507	508	rBV2	168	97	0.01%	0.002%
6	2.753	514	517	520	rBV	201	127	0.02%	0.002%
7	2.788	524	528	530	rBV	251	147	0.02%	0.002%
8	2.833	539	542	547	rBV2	219	197	0.03%	0.003%
9	3.000	591	594	595	rBV	133	80	0.01%	0.001%
10	3.068	613	615	617	rBV	167	86	0.01%	0.001%
11	3.126	630	633	637	rVB2	233	141	0.02%	0.002%
12	3.171	644	647	653	rVB2	271	264	0.03%	0.004%
13	3.203	654	657	658	rBV	178	88	0.01%	0.001%
14	3.277	679	680	681	rVB	115	22	0.00%	0.000%
15	3.364	704	707	711	rVB	236	143	0.02%	0.002%
16	3.412	718	722	725	rBV	189	206	0.03%	0.003%
17	3.428	725	727	729	rBV2	137	87	0.01%	0.001%
18	3.627	787	789	790	rBV	130	73	0.01%	0.001%
19	3.695	804	810	812	rBV	221	275	0.03%	0.004%
20	3.746	822	826	829	rVB2	198	204	0.03%	0.003%
21	3.772	830	834	837	rBV2	186	147	0.02%	0.002%
22	3.817	845	848	851	rBV	180	161	0.02%	0.003%
23	3.846	855	857	858	rBV	125	56	0.01%	0.001%
24	3.904	866	875	903	rBV	51142	141572	18.01%	2.264%
25	4.376	1001	1022	1050	rBV	135700	334968	42.60%	5.357%
26	4.572	1079	1083	1085	rBV2	303	253	0.03%	0.004%
27	4.627	1098	1100	1101	rBV2	218	91	0.01%	0.001%
28	4.637	1101	1103	1105	rVB2	264	74	0.01%	0.001%
29	4.653	1105	1108	1110	rBV	181	155	0.02%	0.002%
30	4.701	1121	1123	1126	rBV	170	138	0.02%	0.002%
31	4.762	1140	1142	1144	rVB	252	120	0.02%	0.002%
32	4.778	1145	1147	1149	rBV	247	149	0.02%	0.002%
33	4.987	1211	1212	1213	rBV	98	22	0.00%	0.000%
34	4.997	1213	1215	1217	rBV	129	51	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019353.D
 Acq On : 12 Nov 2020 15:35
 Operator : SY/MD
 Sample : VV1112MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

35	5.071	1221	1238	1263	rBV2	305897	786236	100.00%	12.575%
36	5.286	1303	1305	1309	rBV	299	187	0.02%	0.003%
37	5.389	1332	1337	1343	rVB	205	256	0.03%	0.004%
38	5.415	1343	1345	1347	rVV	169	93	0.01%	0.001%
39	5.444	1351	1354	1357	rVB	308	181	0.02%	0.003%
40	5.476	1362	1364	1366	rVB	171	48	0.01%	0.001%
41	5.495	1367	1370	1372	rBV	147	91	0.01%	0.001%
42	5.576	1393	1395	1399	rVB	171	85	0.01%	0.001%
43	5.595	1399	1401	1403	rBV	172	79	0.01%	0.001%
44	5.640	1403	1415	1438	rBV	243576	482046	61.31%	7.710%
45	5.929	1495	1505	1521	rBV3	16554	32676	4.16%	0.523%
46	6.023	1533	1534	1536	rVB	217	60	0.01%	0.001%
47	6.042	1536	1540	1542	rBV	210	187	0.02%	0.003%
48	6.093	1542	1556	1575	rBV	171190	341308	43.41%	5.459%
49	6.193	1585	1587	1588	rBV	224	74	0.01%	0.001%
50	6.232	1595	1599	1602	rBV4	360	341	0.04%	0.005%
51	6.489	1677	1679	1687	rVB2	191	258	0.03%	0.004%
52	6.560	1697	1701	1703	rVB2	181	125	0.02%	0.002%
53	6.653	1728	1730	1731	rBV2	224	92	0.01%	0.001%
54	6.823	1780	1783	1785	rBV	227	115	0.01%	0.002%
55	6.868	1792	1797	1802	rBV	288	328	0.04%	0.005%
56	6.949	1817	1822	1828	rBV2	230	338	0.04%	0.005%
57	7.006	1828	1840	1861	rBV	102582	183992	23.40%	2.943%
58	7.283	1924	1926	1928	rBV	145	77	0.01%	0.001%
59	7.338	1931	1943	1973	rVV	372248	646033	82.17%	10.333%
60	7.550	2006	2009	2014	rVB3	364	269	0.03%	0.004%
61	7.643	2025	2038	2063	rBV	75868	134513	17.11%	2.151%
62	7.762	2073	2075	2078	rBV2	251	122	0.02%	0.002%
63	7.923	2122	2125	2130	rVB	280	185	0.02%	0.003%
64	7.949	2130	2133	2135	rBV	185	134	0.02%	0.002%
65	8.106	2172	2182	2216	rBV2	165616	312500	39.75%	4.998%
66	8.357	2254	2260	2261	rBV2	189	202	0.03%	0.003%
67	8.550	2317	2320	2322	rBV2	226	184	0.02%	0.003%
68	8.785	2391	2393	2395	rBV	117	32	0.00%	0.001%
69	8.871	2409	2420	2446	rBV	373168	604250	76.85%	9.664%
70	9.048	2471	2475	2478	rVB2	439	371	0.05%	0.006%
71	9.080	2481	2485	2486	rBV	212	149	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019353.D
 Acq On : 12 Nov 2020 15:35
 Operator : SY/MD
 Sample : VV1112MBL01
 Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

72	9.485	2609	2611	2612	rBV	162	47	0.01%	0.001%
73	9.518	2619	2621	2624	rBV	233	180	0.02%	0.003%
74	9.656	2662	2664	2665	rBV	111	24	0.00%	0.000%
75	9.669	2666	2668	2669	rBV	168	51	0.01%	0.001%
76	10.235	2833	2844	2861	rBV	222437	341912	43.49%	5.469%
77	10.572	2943	2949	2953	rBV3	419	379	0.05%	0.006%
78	11.186	3138	3140	3142	rBV2	176	100	0.01%	0.002%
79	11.209	3144	3147	3149	rBV	400	291	0.04%	0.005%
80	11.270	3155	3166	3191	rBV	424725	644597	81.99%	10.310%
81	11.646	3270	3283	3301	rBV	422591	665508	84.64%	10.644%
82	12.498	3545	3548	3551	rBV	225	174	0.02%	0.003%
83	13.247	3778	3781	3783	rBV2	396	270	0.03%	0.004%
84	13.289	3791	3794	3796	rBV2	443	280	0.04%	0.004%


Sum of corrected areas: 6252387

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111220\
Data File : VV019353.D
Acq On : 12 Nov 2020 15:35
Operator : SY/MD
Sample : VV1112MBL01
Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK81

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

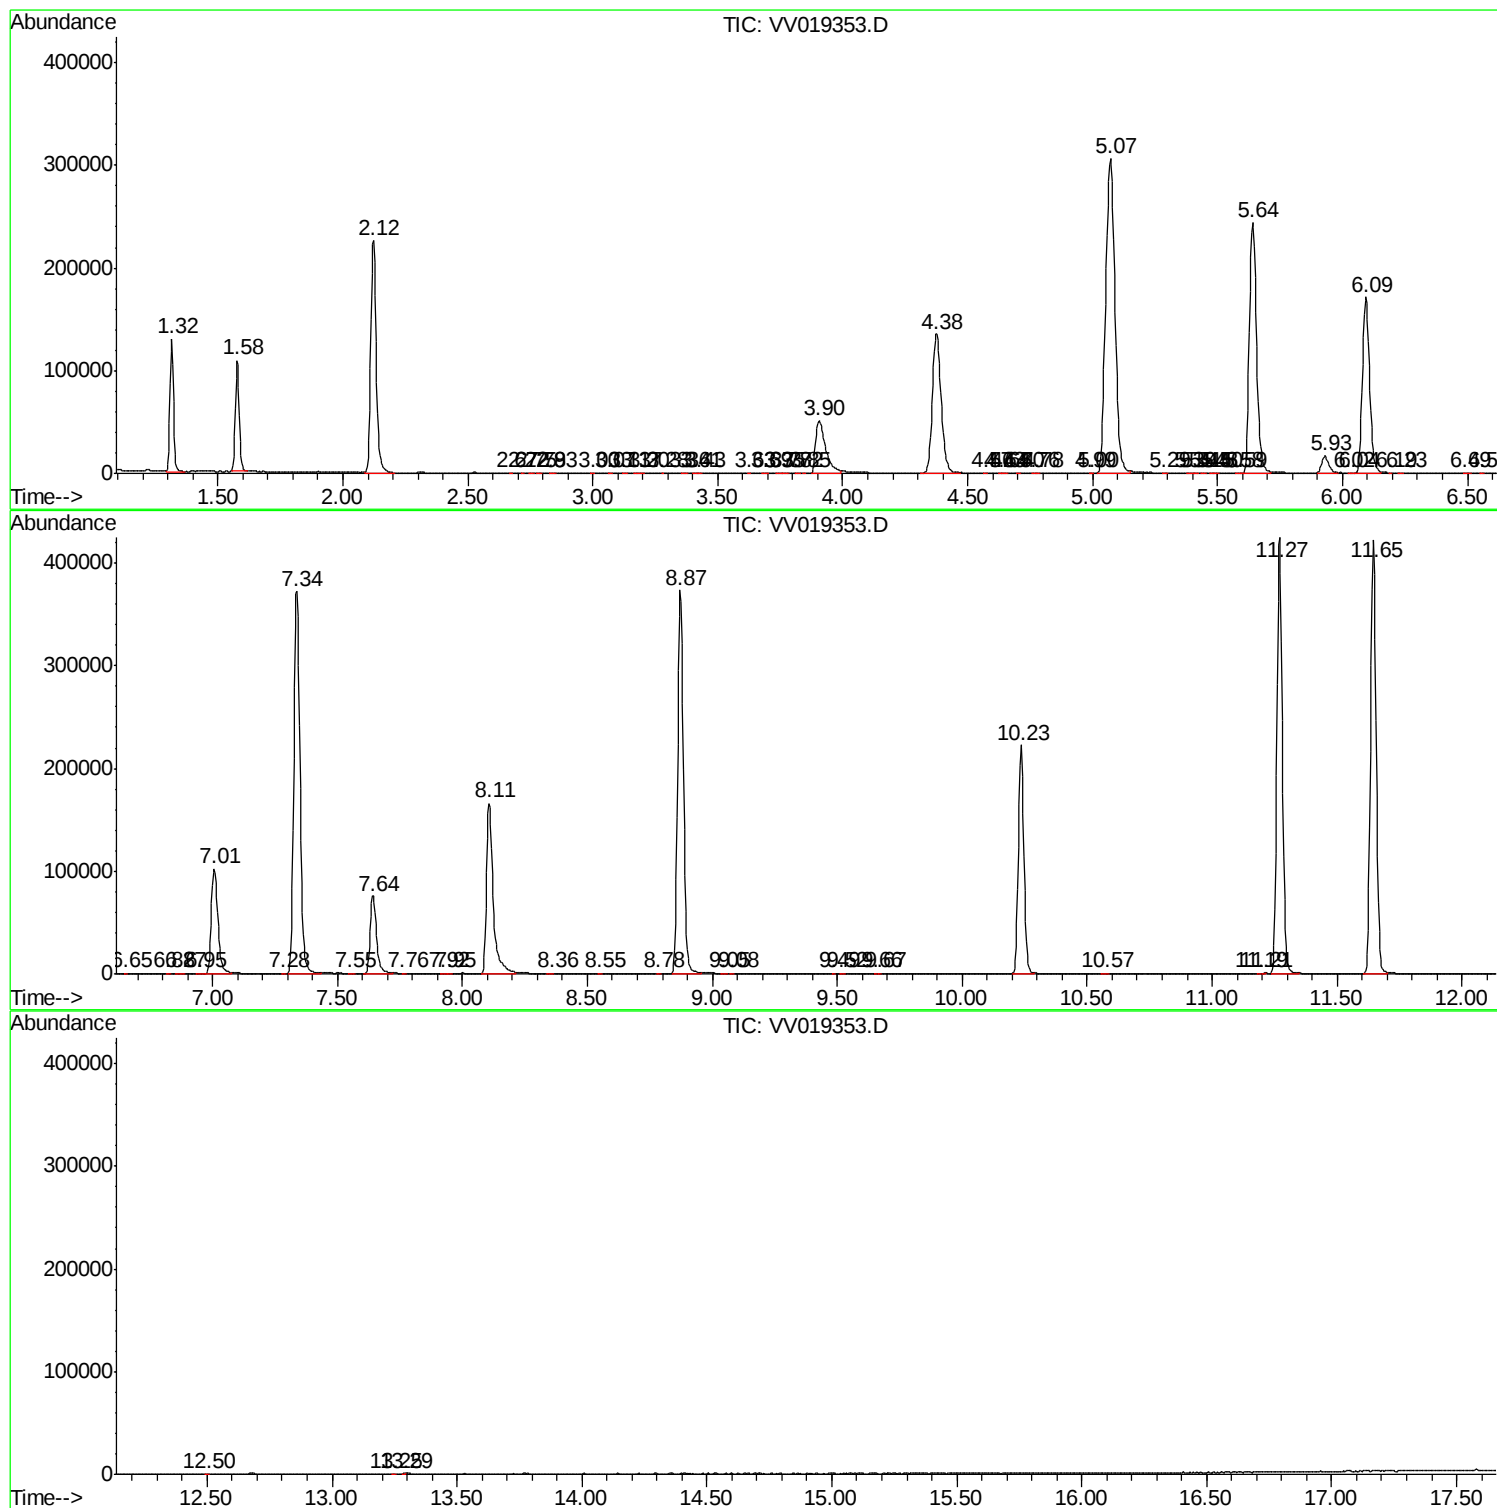

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111220\
Data File : VV019353.D
Acq On : 12 Nov 2020 15:35
Operator : SY/MD
Sample : VV1112MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK81

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV111220\
Data File : VV019353.D
Acq On : 12 Nov 2020 15:35
Operator : SY/MD
Sample : VV1112MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK81

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
