

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019355.D
 Acq On : 12 Nov 2020 16:34
 Operator : SY/MD
 Sample : L4693-09ME 10X
 Misc : 6.12g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4D9ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	82	rVB	120969	124307	8.06%	1.575%
2	1.573	144	150	163	rVB	115891	125452	8.13%	1.590%
3	2.119	309	320	346	rVB	228101	348559	22.60%	4.417%
4	2.347	390	391	392	rBV	134	34	0.00%	0.000%
5	2.431	413	417	421	rVB2	248	195	0.01%	0.002%
6	2.524	439	446	452	rBV3	891	1229	0.08%	0.016%
7	2.630	472	479	495	rVB2	1017	2156	0.14%	0.027%
8	2.875	553	555	557	rVB	160	61	0.00%	0.001%
9	2.968	582	584	587	rBV2	179	120	0.01%	0.002%
10	2.994	590	592	593	rVV2	110	44	0.00%	0.001%
11	3.048	603	609	612	rBV2	339	404	0.03%	0.005%
12	3.154	640	642	646	rBV	168	95	0.01%	0.001%
13	3.380	709	712	717	rBV	196	243	0.02%	0.003%
14	3.431	725	728	730	rBV2	166	100	0.01%	0.001%
15	3.470	738	740	741	rBV	126	69	0.00%	0.001%
16	3.524	754	757	758	rBV	139	61	0.00%	0.001%
17	3.553	765	766	767	rVB	116	22	0.00%	0.000%
18	3.572	769	772	773	rBV	177	108	0.01%	0.001%
19	3.621	784	787	789	rVB	130	71	0.00%	0.001%
20	3.637	789	792	794	rVB2	153	87	0.01%	0.001%
21	3.653	794	797	801	rBB	152	99	0.01%	0.001%
22	3.756	827	829	831	rBV	171	99	0.01%	0.001%
23	3.830	848	852	855	rVB2	185	144	0.01%	0.002%
24	3.846	855	857	860	rBV2	124	87	0.01%	0.001%
25	3.904	865	875	923	rBV	52765	156510	10.15%	1.983%
26	4.373	1004	1021	1045	rBV	136144	337286	21.87%	4.274%
27	4.508	1060	1063	1066	rBV2	157	123	0.01%	0.002%
28	4.563	1078	1080	1081	rBV2	116	46	0.00%	0.001%
29	4.585	1085	1087	1090	rVB	174	54	0.00%	0.001%
30	4.617	1094	1097	1101	rVB	207	129	0.01%	0.002%
31	4.672	1112	1114	1116	rBV2	146	104	0.01%	0.001%
32	4.833	1161	1164	1166	rBV	187	161	0.01%	0.002%
33	4.939	1194	1197	1199	rBV	197	95	0.01%	0.001%
34	4.952	1199	1201	1205	rBV	210	154	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019355.D
 Acq On : 12 Nov 2020 16:34
 Operator : SY/MD
 Sample : L4693-09ME 10X
 Misc : 6.12g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4D9ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

35	4.997	1211	1215	1217	rBV	153	157	0.01%	0.002%
36	5.068	1217	1237	1260	rBV3	317166	807351	52.35%	10.231%
37	5.341	1318	1322	1323	rBV2	299	187	0.01%	0.002%
38	5.579	1394	1396	1403	rVB2	261	216	0.01%	0.003%
39	5.640	1403	1415	1437	rBV	246896	491843	31.89%	6.233%
40	5.929	1494	1505	1526	rVB4	18736	41996	2.72%	0.532%
41	6.093	1543	1556	1579	rBV2	171227	347495	22.53%	4.403%
42	6.215	1591	1594	1597	rBV2	223	187	0.01%	0.002%
43	6.309	1621	1623	1628	rVB	252	141	0.01%	0.002%
44	6.341	1629	1633	1635	rBV2	214	176	0.01%	0.002%
45	6.395	1648	1650	1652	rVB	119	47	0.00%	0.001%
46	6.412	1653	1655	1658	rBV	126	53	0.00%	0.001%
47	6.431	1659	1661	1663	rBV	151	77	0.00%	0.001%
48	6.746	1757	1759	1760	rBV	130	49	0.00%	0.001%
49	6.785	1769	1771	1773	rBV2	195	137	0.01%	0.002%
50	6.868	1795	1797	1798	rBV	141	38	0.00%	0.000%
51	6.923	1809	1814	1819	rBV2	190	178	0.01%	0.002%
52	6.952	1819	1823	1824	rBV	139	100	0.01%	0.001%
53	7.006	1829	1840	1860	rBV	105220	188703	12.24%	2.391%
54	7.167	1887	1890	1895	rBV3	456	350	0.02%	0.004%
55	7.196	1895	1899	1903	rVB2	443	370	0.02%	0.005%
56	7.334	1930	1942	1962	rBV	383363	663511	43.02%	8.408%
57	7.595	2021	2023	2025	rVB	205	114	0.01%	0.001%
58	7.640	2028	2037	2063	rVV	79442	136774	8.87%	1.733%
59	7.778	2077	2080	2085	rBV3	318	380	0.02%	0.005%
60	7.923	2123	2125	2128	rBV2	154	84	0.01%	0.001%
61	7.993	2134	2147	2171	rBV	926218	1542320	100.00%	19.544%
62	8.106	2173	2182	2216	rVB	167992	318391	20.64%	4.035%
63	8.370	2262	2264	2267	rVB2	197	90	0.01%	0.001%
64	8.592	2329	2333	2335	rBV2	215	187	0.01%	0.002%
65	8.675	2356	2359	2363	rBV2	185	160	0.01%	0.002%
66	8.727	2373	2375	2376	rBV	110	23	0.00%	0.000%
67	8.807	2397	2400	2403	rBV2	191	168	0.01%	0.002%
68	8.871	2409	2420	2449	rBV	382263	613274	39.76%	7.771%
69	9.048	2467	2475	2484	rBV4	426	743	0.05%	0.009%
70	9.116	2492	2496	2500	rBV	235	246	0.02%	0.003%
71	9.264	2539	2542	2544	rBV	140	68	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019355.D
 Acq On : 12 Nov 2020 16:34
 Operator : SY/MD
 Sample : L4693-09ME 10X
 Misc : 6.12g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4D9ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

72	9.280	2544	2547	2550	rVB2	194	152	0.01%	0.002%
73	9.611	2648	2650	2652	rBB	199	81	0.01%	0.001%
74	9.704	2676	2679	2684	rBV2	283	284	0.02%	0.004%
75	9.842	2719	2722	2724	rBV2	215	174	0.01%	0.002%
76	10.235	2833	2844	2862	rBV	218907	339652	22.02%	4.304%
77	10.354	2879	2881	2882	rBV	146	79	0.01%	0.001%
78	10.408	2896	2898	2901	rBV	172	77	0.00%	0.001%
79	10.543	2938	2940	2941	rBV	161	90	0.01%	0.001%
80	10.964	3068	3071	3072	rBV	174	90	0.01%	0.001%
81	11.045	3094	3096	3101	rBV2	214	153	0.01%	0.002%
82	11.080	3104	3107	3111	rBV	234	142	0.01%	0.002%
83	11.206	3142	3146	3148	rBV2	418	346	0.02%	0.004%
84	11.270	3155	3166	3189	rBV	416129	633078	41.05%	8.022%
85	11.402	3205	3207	3211	rBV2	306	203	0.01%	0.003%
86	11.646	3270	3283	3304	rBV	422616	660250	42.81%	8.367%
87	11.916	3363	3367	3368	rBV	184	127	0.01%	0.002%
88	11.945	3373	3376	3378	rBV2	269	189	0.01%	0.002%
89	13.234	3774	3777	3779	rBV2	240	139	0.01%	0.002%
90	13.537	3869	3871	3875	rBV	421	338	0.02%	0.004%
91	14.109	4048	4049	4054	rBV2	459	280	0.02%	0.004%
92	14.273	4097	4100	4102	rBV2	354	243	0.02%	0.003%
93	14.691	4227	4230	4234	rBV3	365	373	0.02%	0.005%


Sum of corrected areas: 7891432

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111220\
Data File : VV019355.D
Acq On : 12 Nov 2020 16:34
Operator : SY/MD
Sample : L4693-09ME 10X
Misc : 6.12g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4D9ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

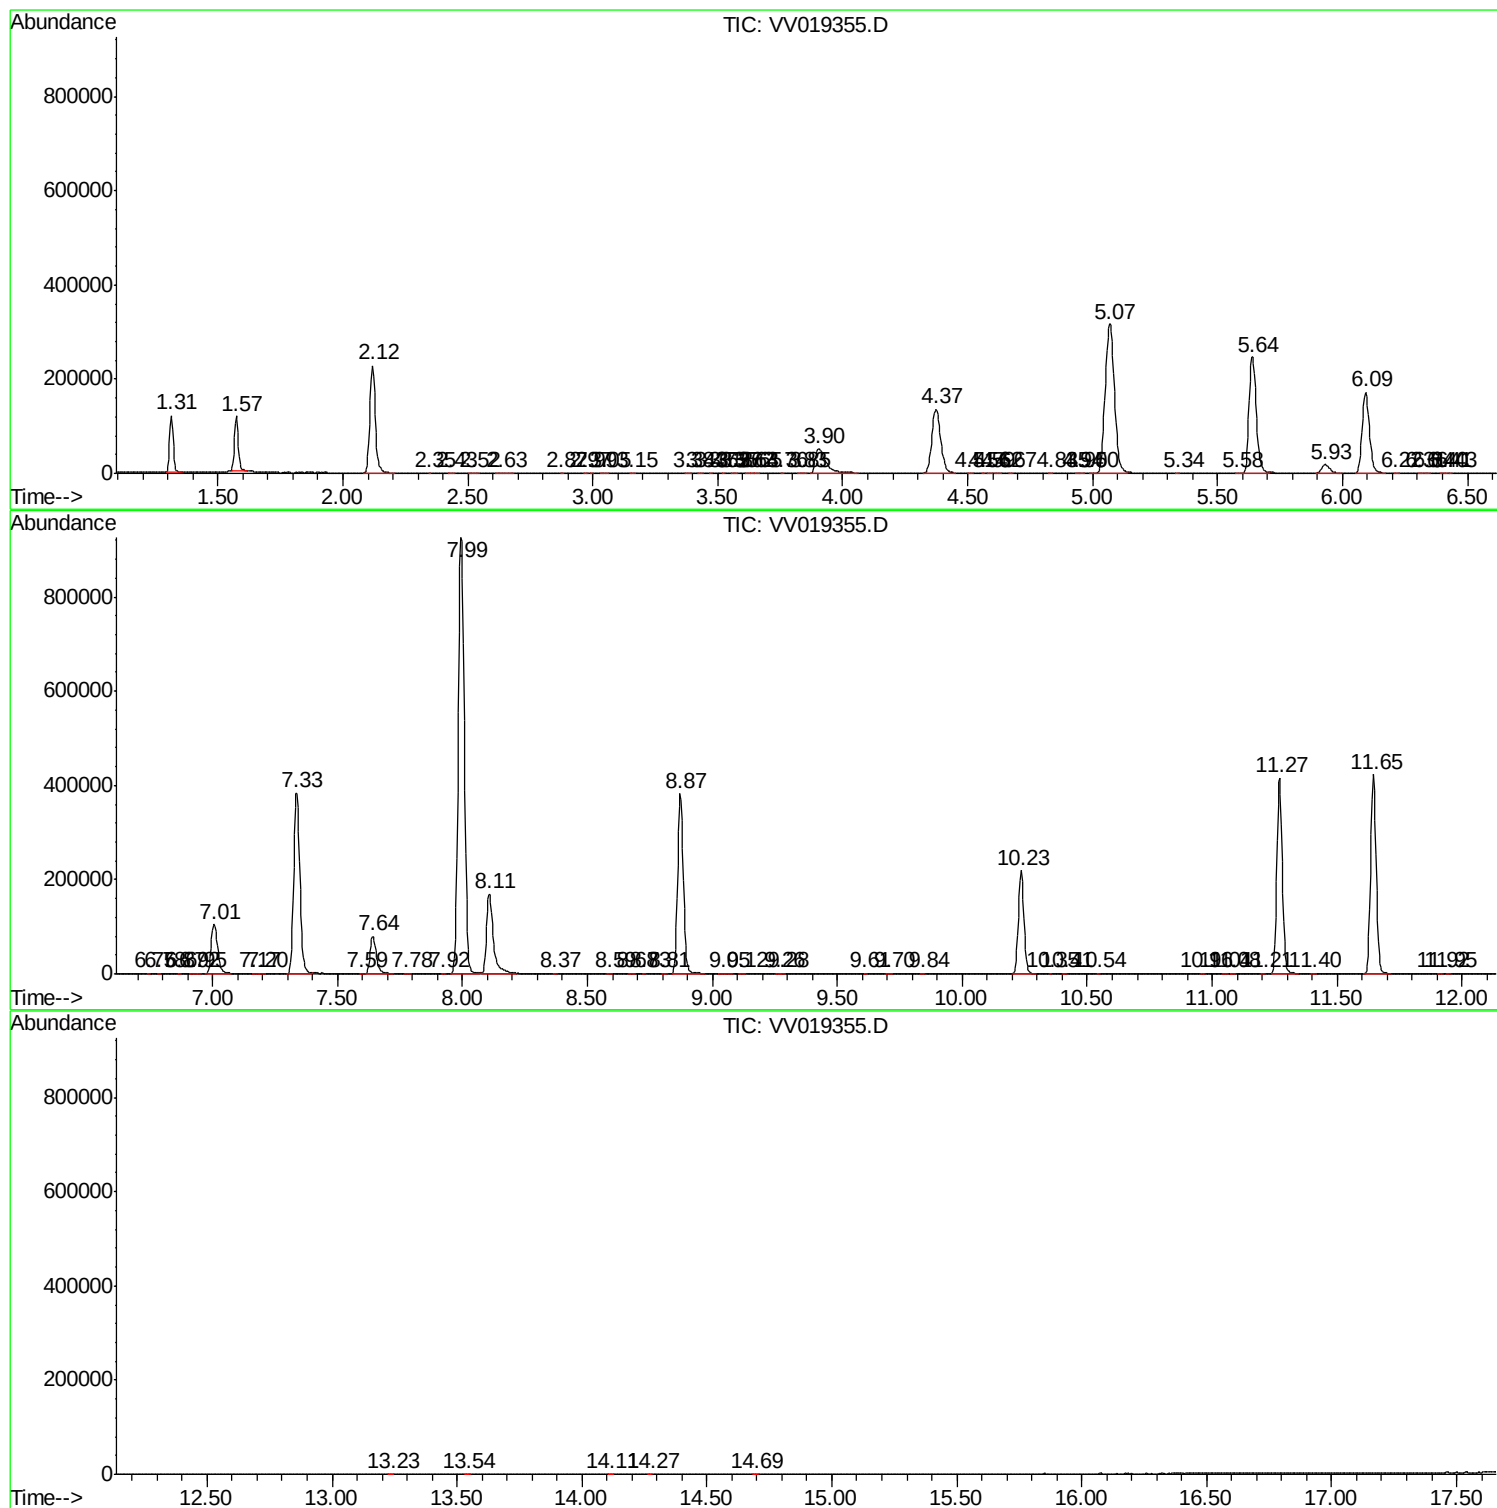

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111220\
Data File : VV019355.D
Acq On : 12 Nov 2020 16:34
Operator : SY/MD
Sample : L4693-09ME 10X
Misc : 6.12g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4D9ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV111220\
Data File : VV019355.D
Acq On : 12 Nov 2020 16:34
Operator : SY/MD
Sample : L4693-09ME 10X
Misc : 6.12g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4D9ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc