

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019358.D
 Acq On : 12 Nov 2020 17:46
 Operator : SY/MD
 Sample : VIBLK98
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK98

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	128394	127353	15.51%	1.974%
2	1.576	144	151	166	rBV	110392	122246	14.89%	1.895%
3	2.119	310	320	346	rVB	230178	354464	43.18%	5.494%
4	2.306	374	378	387	rBV2	689	850	0.10%	0.013%
5	2.528	440	447	451	rBV2	691	921	0.11%	0.014%
6	2.634	477	480	482	rBV2	220	154	0.02%	0.002%
7	2.663	486	489	494	rVB	272	242	0.03%	0.004%
8	2.682	494	495	496	rBV	95	23	0.00%	0.000%
9	2.743	512	514	517	rVB	135	60	0.01%	0.001%
10	2.859	547	550	554	rVB	201	164	0.02%	0.003%
11	2.894	559	561	564	rVB	121	29	0.00%	0.000%
12	2.910	564	566	567	rBV	135	52	0.01%	0.001%
13	2.923	568	570	573	rBV	214	124	0.02%	0.002%
14	2.958	579	581	584	rBV	104	82	0.01%	0.001%
15	2.997	592	593	595	rBV	118	28	0.00%	0.000%
16	3.036	604	605	606	rBV	100	22	0.00%	0.000%
17	3.116	626	630	638	rVB2	342	492	0.06%	0.008%
18	3.158	641	643	647	rVB	290	192	0.02%	0.003%
19	3.184	648	651	652	rBV	150	102	0.01%	0.002%
20	3.206	656	658	659	rVB	114	46	0.01%	0.001%
21	3.322	693	694	695	rBV	128	33	0.00%	0.001%
22	3.357	702	705	707	rBV	147	86	0.01%	0.001%
23	3.383	708	713	715	rVV2	238	210	0.03%	0.003%
24	3.399	716	718	721	rVV	192	98	0.01%	0.002%
25	3.431	725	728	731	rBV	177	89	0.01%	0.001%
26	3.473	738	741	742	rBV	138	85	0.01%	0.001%
27	3.534	757	760	762	rVB2	161	92	0.01%	0.001%
28	3.560	766	768	771	rBV	140	94	0.01%	0.001%
29	3.637	790	792	793	rBV	131	40	0.00%	0.001%
30	3.676	801	804	808	rBV2	155	111	0.01%	0.002%
31	3.704	810	813	814	rBV2	147	63	0.01%	0.001%
32	3.737	820	823	827	rBV2	230	234	0.03%	0.004%
33	3.775	833	835	836	rBV	124	29	0.00%	0.000%
34	3.788	836	839	841	rVV2	144	83	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019358.D
 Acq On : 12 Nov 2020 17:46
 Operator : SY/MD
 Sample : VIBLK98
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK98

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

35	3.856	857	860	862	rBV	182	148	0.02%	0.002%
36	3.868	862	864	866	rVB	154	62	0.01%	0.001%
37	3.907	866	876	909	rBV	50847	149192	18.17%	2.313%
38	4.190	961	964	967	rBV2	396	313	0.04%	0.005%
39	4.376	1004	1022	1049	rBV	139884	345322	42.06%	5.353%
40	4.563	1078	1080	1082	rVB	290	136	0.02%	0.002%
41	4.630	1098	1101	1104	rBV	171	101	0.01%	0.002%
42	4.656	1106	1109	1111	rBV	117	73	0.01%	0.001%
43	4.711	1124	1126	1127	rBV	240	97	0.01%	0.002%
44	4.740	1132	1135	1139	rBV2	325	325	0.04%	0.005%
45	4.762	1139	1142	1145	rVV2	205	144	0.02%	0.002%
46	4.782	1146	1148	1151	rVV	204	131	0.02%	0.002%
47	4.814	1156	1158	1159	rVB	110	45	0.01%	0.001%
48	5.071	1220	1238	1269	rBV2	318654	820963	100.00%	12.725%
49	5.277	1300	1302	1305	rBV	331	257	0.03%	0.004%
50	5.319	1313	1315	1316	rBV	118	24	0.00%	0.000%
51	5.418	1341	1346	1348	rBV2	359	379	0.05%	0.006%
52	5.450	1353	1356	1357	rBV	138	77	0.01%	0.001%
53	5.505	1369	1373	1376	rBV2	182	200	0.02%	0.003%
54	5.524	1376	1379	1382	rVB	179	105	0.01%	0.002%
55	5.640	1403	1415	1440	rBV	245450	486833	59.30%	7.546%
56	5.929	1494	1505	1524	rBV3	17690	35589	4.34%	0.552%
57	6.093	1543	1556	1577	rBV	179299	360554	43.92%	5.589%
58	6.209	1590	1592	1594	rBV	268	88	0.01%	0.001%
59	6.309	1620	1623	1624	rBV2	168	96	0.01%	0.001%
60	6.396	1646	1650	1652	rBV2	194	170	0.02%	0.003%
61	6.540	1689	1695	1696	rBV	152	152	0.02%	0.002%
62	6.624	1717	1721	1724	rVB	217	163	0.02%	0.003%
63	6.669	1733	1735	1738	rVB	175	79	0.01%	0.001%
64	6.708	1745	1747	1748	rBV	139	39	0.00%	0.001%
65	6.778	1766	1769	1773	rBV2	178	176	0.02%	0.003%
66	6.865	1793	1796	1798	rBV	180	124	0.02%	0.002%
67	7.007	1827	1840	1867	rBV	106570	191671	23.35%	2.971%
68	7.283	1922	1926	1930	rBV2	228	207	0.03%	0.003%
69	7.338	1930	1943	1976	rVV	386387	676060	82.35%	10.479%
70	7.598	2022	2024	2027	rBV2	307	203	0.02%	0.003%
71	7.640	2028	2037	2059	rVV	79463	136114	16.58%	2.110%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019358.D
 Acq On : 12 Nov 2020 17:46
 Operator : SY/MD
 Sample : VIBLK98
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK98

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

72	7.881	2108	2112	2115	rBV2	220	216	0.03%	0.003%
73	7.952	2129	2134	2135	rBV2	143	134	0.02%	0.002%
74	8.003	2139	2150	2159	rVB5	4701	7666	0.93%	0.119%
75	8.106	2172	2182	2215	rBV2	177187	333699	40.65%	5.172%
76	8.376	2264	2266	2271	rBV	348	317	0.04%	0.005%
77	8.592	2332	2333	2334	rBV	131	33	0.00%	0.001%
78	8.685	2359	2362	2365	rBV2	204	163	0.02%	0.003%
79	8.871	2409	2420	2444	rBV	379865	612352	74.59%	9.492%
80	9.222	2527	2529	2530	rBV	176	57	0.01%	0.001%
81	9.572	2634	2638	2641	rBV2	225	207	0.03%	0.003%
82	9.624	2652	2654	2657	rBV	179	75	0.01%	0.001%
83	9.887	2733	2736	2741	rBV	261	284	0.03%	0.004%
84	10.013	2773	2775	2779	rBV	173	64	0.01%	0.001%
85	10.196	2829	2832	2833	rBV	209	99	0.01%	0.002%
86	10.235	2833	2844	2864	rVV	227137	356039	43.37%	5.519%
87	10.357	2880	2882	2883	rBV	173	74	0.01%	0.001%
88	10.412	2896	2899	2903	rBV2	254	191	0.02%	0.003%
89	10.457	2911	2913	2915	rBV	230	122	0.01%	0.002%
90	10.881	3042	3045	3047	rBV2	215	131	0.02%	0.002%
91	11.019	3085	3088	3089	rBV	179	109	0.01%	0.002%
92	11.222	3149	3151	3155	rBV	146	56	0.01%	0.001%
93	11.270	3155	3166	3193	rBV	418021	640231	77.99%	9.924%
94	11.566	3254	3258	3261	rBV	271	214	0.03%	0.003%
95	11.646	3270	3283	3302	rBV	431077	682619	83.15%	10.581%
96	11.897	3358	3361	3363	rBV	224	105	0.01%	0.002%
97	12.411	3518	3521	3526	rBV2	241	228	0.03%	0.004%
98	12.688	3602	3607	3611	rBV	326	268	0.03%	0.004%
99	13.601	3889	3891	3893	rVB	336	150	0.02%	0.002%
100	13.833	3960	3963	3965	rBV	271	170	0.02%	0.003%


Sum of corrected areas: 6451478

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111220\
Data File : VV019358.D
Acq On : 12 Nov 2020 17:46
Operator : SY/MD
Sample : VIBLK98
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK98

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

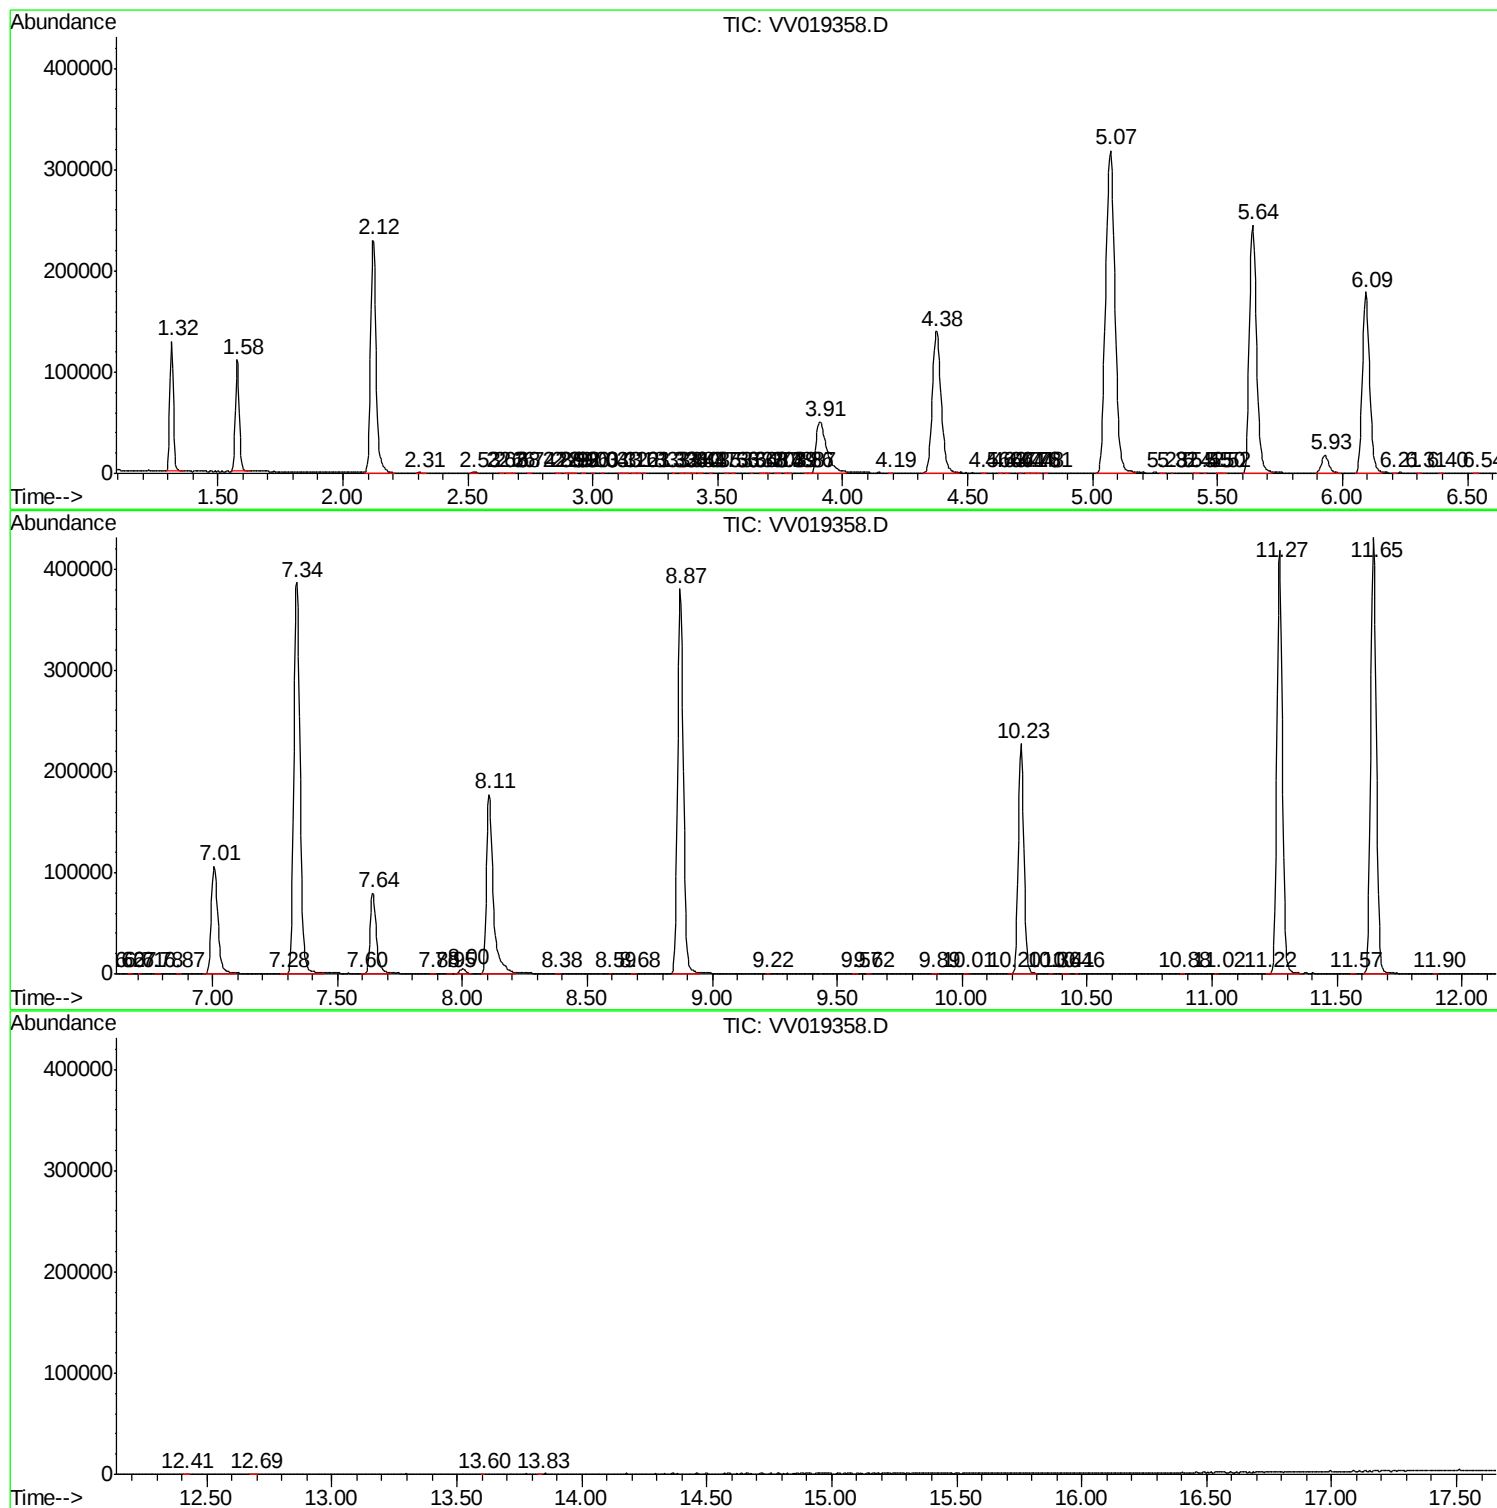

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111220\
Data File : VV019358.D
Acq On : 12 Nov 2020 17:46
Operator : SY/MD
Sample : VIBLK98
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK98

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111220\
Data File : VV019358.D
Acq On : 12 Nov 2020 17:46
Operator : SY/MD
Sample : VIBLK98
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK98

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc