

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019363.D
 Acq On : 12 Nov 2020 19:45
 Operator : SY/MD
 Sample : VIBLK99
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	129239	129291	15.84%	2.026%
2	1.579	144	152	163	rBV	109028	123489	15.13%	1.935%
3	2.122	311	321	347	rVB	227502	346793	42.49%	5.434%
4	2.248	356	360	364	rVB2	240	223	0.03%	0.003%
5	2.302	373	377	380	rBV2	441	408	0.05%	0.006%
6	2.524	440	446	453	rVB4	895	1122	0.14%	0.018%
7	2.573	455	461	463	rBV2	216	251	0.03%	0.004%
8	2.659	485	488	490	rBV	140	99	0.01%	0.002%
9	2.685	494	496	503	rVB	239	163	0.02%	0.003%
10	2.820	536	538	541	rBV	166	131	0.02%	0.002%
11	2.945	574	577	579	rBV2	280	224	0.03%	0.004%
12	3.023	599	601	602	rVB	125	30	0.00%	0.000%
13	3.100	623	625	627	rBV	251	161	0.02%	0.003%
14	3.119	629	631	634	rVB2	292	186	0.02%	0.003%
15	3.145	635	639	640	rBV	233	122	0.01%	0.002%
16	3.161	642	644	648	rVB	194	72	0.01%	0.001%
17	3.180	648	650	651	rBV	164	48	0.01%	0.001%
18	3.235	665	667	670	rVB	242	137	0.02%	0.002%
19	3.254	671	673	675	rBV2	254	166	0.02%	0.003%
20	3.405	716	720	722	rBV	201	183	0.02%	0.003%
21	3.425	725	726	727	rVB	99	23	0.00%	0.000%
22	3.572	769	772	773	rBV	229	118	0.01%	0.002%
23	3.717	815	817	818	rBV	131	32	0.00%	0.001%
24	3.756	826	829	832	rVB	280	198	0.02%	0.003%
25	3.778	833	836	839	rBV2	285	224	0.03%	0.004%
26	3.794	839	841	844	rVV	192	133	0.02%	0.002%
27	3.839	852	855	858	rBV2	187	130	0.02%	0.002%
28	3.910	866	877	911	rBV	50418	149517	18.32%	2.343%
29	4.264	985	987	988	rBV	261	125	0.02%	0.002%
30	4.376	1006	1022	1056	rVB	139255	343432	42.08%	5.381%
31	4.560	1076	1079	1081	rVB2	325	139	0.02%	0.002%
32	4.646	1103	1106	1108	rBV2	132	88	0.01%	0.001%
33	4.691	1118	1120	1122	rBV	150	103	0.01%	0.002%
34	4.736	1130	1134	1138	rBV	236	224	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019363.D
 Acq On : 12 Nov 2020 19:45
 Operator : SY/MD
 Sample : VIBLK99
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

35	4.794	1149	1152	1156	rBV2	157	134	0.02%	0.002%
36	4.826	1159	1162	1165	rVB2	207	141	0.02%	0.002%
37	4.913	1185	1189	1194	rVB	232	234	0.03%	0.004%
38	4.939	1194	1197	1200	rVB2	350	235	0.03%	0.004%
39	4.961	1201	1204	1205	rBV2	229	133	0.02%	0.002%
40	4.984	1208	1211	1212	rBV	186	123	0.02%	0.002%
41	5.071	1220	1238	1266	rBV2	319056	816140	100.00%	12.787%
42	5.318	1312	1315	1317	rVB2	259	163	0.02%	0.003%
43	5.334	1317	1320	1321	rBV	142	76	0.01%	0.001%
44	5.396	1337	1339	1341	rBV	286	176	0.02%	0.003%
45	5.421	1341	1347	1349	rVV2	263	328	0.04%	0.005%
46	5.434	1349	1351	1355	rVV2	390	224	0.03%	0.004%
47	5.460	1355	1359	1363	rVV2	234	229	0.03%	0.004%
48	5.534	1379	1382	1385	rBV	206	179	0.02%	0.003%
49	5.588	1397	1399	1403	rBV2	211	153	0.02%	0.002%
50	5.640	1403	1415	1445	rBV	244015	487547	59.74%	7.639%
51	5.926	1494	1504	1522	rBV2	17766	36972	4.53%	0.579%
52	6.026	1533	1535	1538	rVB	339	164	0.02%	0.003%
53	6.093	1543	1556	1589	rVV	179680	357930	43.86%	5.608%
54	6.309	1620	1623	1625	rBV2	163	118	0.01%	0.002%
55	6.399	1649	1651	1654	rVB	176	72	0.01%	0.001%
56	6.418	1654	1657	1659	rBV2	337	226	0.03%	0.004%
57	6.576	1702	1706	1709	rVB	219	169	0.02%	0.003%
58	6.723	1748	1752	1756	rVB	198	183	0.02%	0.003%
59	6.862	1793	1795	1796	rBV	209	52	0.01%	0.001%
60	7.006	1830	1840	1858	rBV	104673	183256	22.45%	2.871%
61	7.222	1903	1907	1911	rBV2	264	235	0.03%	0.004%
62	7.286	1925	1927	1931	rBV2	279	182	0.02%	0.003%
63	7.338	1931	1943	1968	rBV	386699	661498	81.05%	10.364%
64	7.566	2012	2014	2016	rBV	240	132	0.02%	0.002%
65	7.598	2022	2024	2026	rBV	186	73	0.01%	0.001%
66	7.640	2027	2037	2064	rBV	77921	135682	16.62%	2.126%
67	7.858	2103	2105	2107	rBV	142	83	0.01%	0.001%
68	7.903	2117	2119	2121	rBV	162	69	0.01%	0.001%
69	7.974	2138	2141	2144	rBV	182	165	0.02%	0.003%
70	8.106	2173	2182	2222	rBV2	169497	332237	40.71%	5.206%
71	8.376	2264	2266	2268	rBV	325	188	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019363.D
 Acq On : 12 Nov 2020 19:45
 Operator : SY/MD
 Sample : VIBLK99
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

72	8.611	2336	2339	2340	rBV2	189	111	0.01%	0.002%
73	8.733	2373	2377	2385	rVB2	234	344	0.04%	0.005%
74	8.768	2385	2388	2394	rVV2	186	154	0.02%	0.002%
75	8.794	2394	2396	2398	rVB	167	66	0.01%	0.001%
76	8.871	2408	2420	2443	rBV	375930	614730	75.32%	9.632%
77	9.048	2470	2475	2478	rBV2	296	343	0.04%	0.005%
78	9.222	2526	2529	2532	rBV2	168	161	0.02%	0.003%
79	9.289	2547	2550	2552	rBV	212	139	0.02%	0.002%
80	9.399	2580	2584	2587	rBV	206	120	0.01%	0.002%
81	9.543	2626	2629	2632	rBV	206	102	0.01%	0.002%
82	9.572	2637	2638	2640	rBV	143	58	0.01%	0.001%
83	9.640	2655	2659	2663	rBV2	313	285	0.03%	0.004%
84	9.842	2718	2722	2724	rBV2	263	181	0.02%	0.003%
85	9.897	2738	2739	2742	rBV	127	42	0.01%	0.001%
86	9.929	2746	2749	2753	rBV2	233	195	0.02%	0.003%
87	10.010	2769	2774	2777	rBV2	271	291	0.04%	0.005%
88	10.177	2823	2826	2831	rBV	166	100	0.01%	0.002%
89	10.238	2833	2845	2865	rBV	229927	360939	44.23%	5.655%
90	10.611	2958	2961	2964	rBV2	204	170	0.02%	0.003%
91	11.270	3155	3166	3191	rBV	405677	624635	76.54%	9.787%
92	11.508	3238	3240	3244	rBV2	197	127	0.02%	0.002%
93	11.646	3271	3283	3300	rBV	424255	664885	81.47%	10.417%
94	12.125	3430	3432	3435	rBV	186	121	0.01%	0.002%
95	12.392	3512	3515	3518	rBV	249	148	0.02%	0.002%
96	12.678	3602	3604	3608	rBV2	256	135	0.02%	0.002%
97	13.759	3938	3940	3941	rBV2	308	134	0.02%	0.002%


Sum of corrected areas: 6382402

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111220\
Data File : VV019363.D
Acq On : 12 Nov 2020 19:45
Operator : SY/MD
Sample : VIBLK99
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK99

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

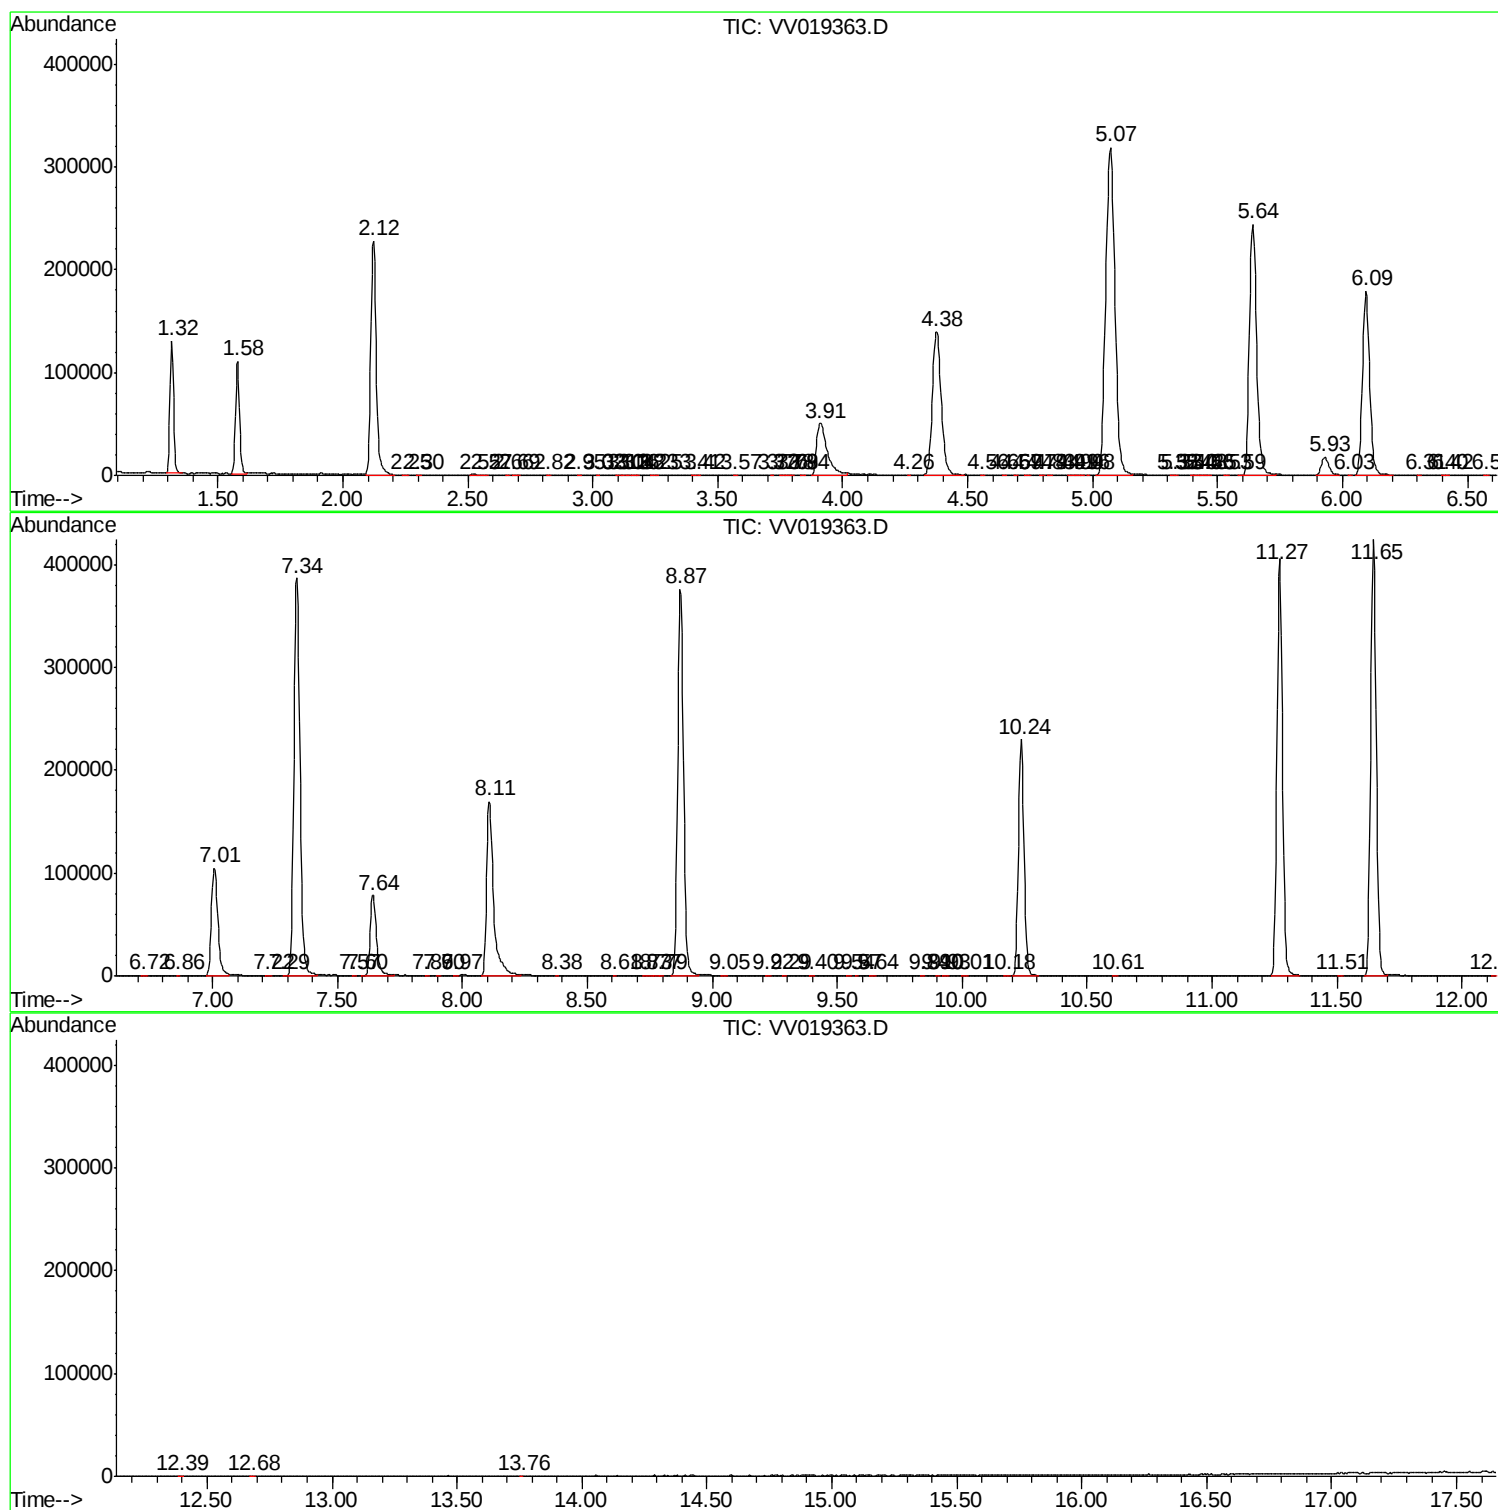

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111220\
Data File : VV019363.D
Acq On : 12 Nov 2020 19:45
Operator : SY/MD
Sample : VIBLK99
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK99

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111220\
Data File : VV019363.D
Acq On : 12 Nov 2020 19:45
Operator : SY/MD
Sample : VIBLK99
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK99

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc