

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019364.D
 Acq On : 12 Nov 2020 20:09
 Operator : SY/MD
 Sample : L4711-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	87	rVB	130179	126855	16.00%	1.984%
2	1.579	144	152	169	rBV	107792	122331	15.42%	1.914%
3	2.122	310	321	355	rVB	227944	347849	43.86%	5.441%
4	2.264	362	365	367	rBV2	182	121	0.02%	0.002%
5	2.296	373	375	376	rBV	187	81	0.01%	0.001%
6	2.434	415	418	419	rBV	156	91	0.01%	0.001%
7	2.489	431	435	439	rBV2	175	187	0.02%	0.003%
8	2.524	439	446	455	rVB3	3481	5319	0.67%	0.083%
9	2.598	465	469	474	rVB2	307	333	0.04%	0.005%
10	2.627	475	478	479	rBV	297	171	0.02%	0.003%
11	2.682	494	495	498	rBV	126	48	0.01%	0.001%
12	2.708	501	503	506	rBV	187	106	0.01%	0.002%
13	2.888	558	559	560	rBV	90	19	0.00%	0.000%
14	2.942	574	576	578	rBV	146	47	0.01%	0.001%
15	3.090	619	622	624	rBV	167	76	0.01%	0.001%
16	3.148	635	640	642	rBV	283	303	0.04%	0.005%
17	3.212	658	660	662	rBV2	200	127	0.02%	0.002%
18	3.286	681	683	686	rBV	117	75	0.01%	0.001%
19	3.338	695	699	703	rVB2	184	156	0.02%	0.002%
20	3.383	710	713	718	rBV2	258	201	0.03%	0.003%
21	3.492	745	747	753	rVB2	167	135	0.02%	0.002%
22	3.550	762	765	768	rVB	269	193	0.02%	0.003%
23	3.573	768	772	777	rBV	210	303	0.04%	0.005%
24	3.682	802	806	808	rBV	168	142	0.02%	0.002%
25	3.736	819	823	824	rBV	291	212	0.03%	0.003%
26	3.769	830	833	836	rBV2	138	114	0.01%	0.002%
27	3.833	850	853	855	rBV	264	172	0.02%	0.003%
28	3.913	867	878	911	rBV	46523	135496	17.08%	2.119%
29	4.376	1006	1022	1049	rBV2	148599	437618	55.18%	6.845%
30	4.534	1066	1071	1074	rVB2	541	430	0.05%	0.007%
31	4.553	1075	1077	1079	rBV	212	100	0.01%	0.002%
32	4.601	1089	1092	1093	rBV	193	131	0.02%	0.002%
33	4.640	1101	1104	1107	rBV	125	83	0.01%	0.001%
34	4.672	1111	1114	1116	rBV	155	70	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019364.D
 Acq On : 12 Nov 2020 20:09
 Operator : SY/MD
 Sample : L4711-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

35	4.688	1117	1119	1121	rVB	132	37	0.00%	0.001%
36	4.711	1124	1126	1129	rVB2	173	95	0.01%	0.001%
37	4.756	1138	1140	1142	rBV	218	144	0.02%	0.002%
38	4.823	1158	1161	1164	rBV	177	130	0.02%	0.002%
39	4.984	1209	1211	1215	rBV	182	92	0.01%	0.001%
40	5.071	1221	1238	1267	rBV3	313066	793087	100.00%	12.406%
41	5.363	1326	1329	1330	rBV	279	163	0.02%	0.003%
42	5.376	1331	1333	1334	rBV	134	49	0.01%	0.001%
43	5.415	1343	1345	1347	rBV	165	56	0.01%	0.001%
44	5.428	1347	1349	1351	rBV	256	135	0.02%	0.002%
45	5.556	1386	1389	1391	rBV	274	183	0.02%	0.003%
46	5.640	1399	1415	1445	rBV	249530	498021	62.80%	7.790%
47	5.929	1494	1505	1523	rBV3	18868	38269	4.83%	0.599%
48	6.093	1543	1556	1581	rBV	171556	349205	44.03%	5.462%
49	6.283	1608	1615	1620	rBV3	306	482	0.06%	0.008%
50	6.312	1620	1624	1627	rVB	276	240	0.03%	0.004%
51	6.331	1628	1630	1636	rBV	173	96	0.01%	0.002%
52	6.379	1639	1645	1647	rVB2	233	249	0.03%	0.004%
53	6.450	1664	1667	1669	rBV2	176	98	0.01%	0.002%
54	6.460	1669	1670	1671	rBV2	101	27	0.00%	0.000%
55	6.476	1671	1675	1678	rVB2	282	241	0.03%	0.004%
56	6.492	1678	1680	1684	rBV	209	153	0.02%	0.002%
57	6.515	1684	1687	1689	rBV2	214	133	0.02%	0.002%
58	6.588	1707	1710	1714	rBV	261	218	0.03%	0.003%
59	6.640	1724	1726	1728	rBV	134	43	0.01%	0.001%
60	6.730	1750	1754	1756	rBV	222	175	0.02%	0.003%
61	6.788	1768	1772	1775	rBV	243	175	0.02%	0.003%
62	6.820	1779	1782	1789	rBV2	166	209	0.03%	0.003%
63	7.006	1828	1840	1865	rBV	99246	181699	22.91%	2.842%
64	7.212	1897	1904	1905	rBV2	421	502	0.06%	0.008%
65	7.338	1931	1943	1976	rBV	377597	657577	82.91%	10.286%
66	7.640	2023	2037	2063	rBV2	75866	131910	16.63%	2.063%
67	7.846	2098	2101	2103	rBV	284	170	0.02%	0.003%
68	7.907	2118	2120	2123	rVB	137	59	0.01%	0.001%
69	7.929	2123	2127	2128	rBV2	233	168	0.02%	0.003%
70	8.039	2158	2161	2163	rBV	176	80	0.01%	0.001%
71	8.106	2173	2182	2218	rBV2	156100	307935	38.83%	4.817%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111220\
 Data File : VV019364.D
 Acq On : 12 Nov 2020 20:09
 Operator : SY/MD
 Sample : L4711-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

72	8.395	2269	2272	2274	rBV	179	128	0.02%	0.002%
73	8.540	2314	2317	2320	rBV2	170	110	0.01%	0.002%
74	8.707	2366	2369	2373	rVB2	246	197	0.02%	0.003%
75	8.740	2376	2379	2380	rBV	148	93	0.01%	0.001%
76	8.785	2390	2393	2394	rBV	140	67	0.01%	0.001%
77	8.871	2408	2420	2445	rBV	391121	632315	79.73%	9.891%
78	9.151	2504	2507	2512	rBV2	333	216	0.03%	0.003%
79	9.177	2512	2515	2517	rBV	178	119	0.02%	0.002%
80	9.325	2559	2561	2563	rBV	138	39	0.00%	0.001%
81	9.473	2604	2607	2611	rBV2	193	169	0.02%	0.003%
82	9.643	2657	2660	2663	rBV	218	182	0.02%	0.003%
83	10.010	2771	2774	2778	rVB	416	318	0.04%	0.005%
84	10.032	2778	2781	2783	rBV	178	153	0.02%	0.002%
85	10.100	2800	2802	2805	rVB	180	68	0.01%	0.001%
86	10.238	2832	2845	2863	rBV	213899	330554	41.68%	5.171%
87	10.473	2915	2918	2920	rBV	180	106	0.01%	0.002%
88	10.598	2953	2957	2959	rBV	184	142	0.02%	0.002%
89	10.772	3009	3011	3014	rBV	128	36	0.00%	0.001%
90	11.135	3121	3124	3125	rBV	209	99	0.01%	0.002%
91	11.270	3155	3166	3190	rBV	415157	637212	80.35%	9.968%
92	11.646	3271	3283	3302	rBV	411589	647194	81.60%	10.124%
93	11.791	3326	3328	3332	rBV2	270	189	0.02%	0.003%
94	11.858	3347	3349	3353	rBV2	304	200	0.03%	0.003%
95	11.897	3357	3361	3364	rBV2	220	179	0.02%	0.003%
96	12.273	3474	3478	3480	rBV3	309	223	0.03%	0.003%
97	13.186	3758	3762	3765	rBV2	254	255	0.03%	0.004%
98	14.103	4044	4047	4050	rBV2	353	289	0.04%	0.005%


Sum of corrected areas: 6392852

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111220\
Data File : VV019364.D
Acq On : 12 Nov 2020 20:09
Operator : SY/MD
Sample : L4711-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

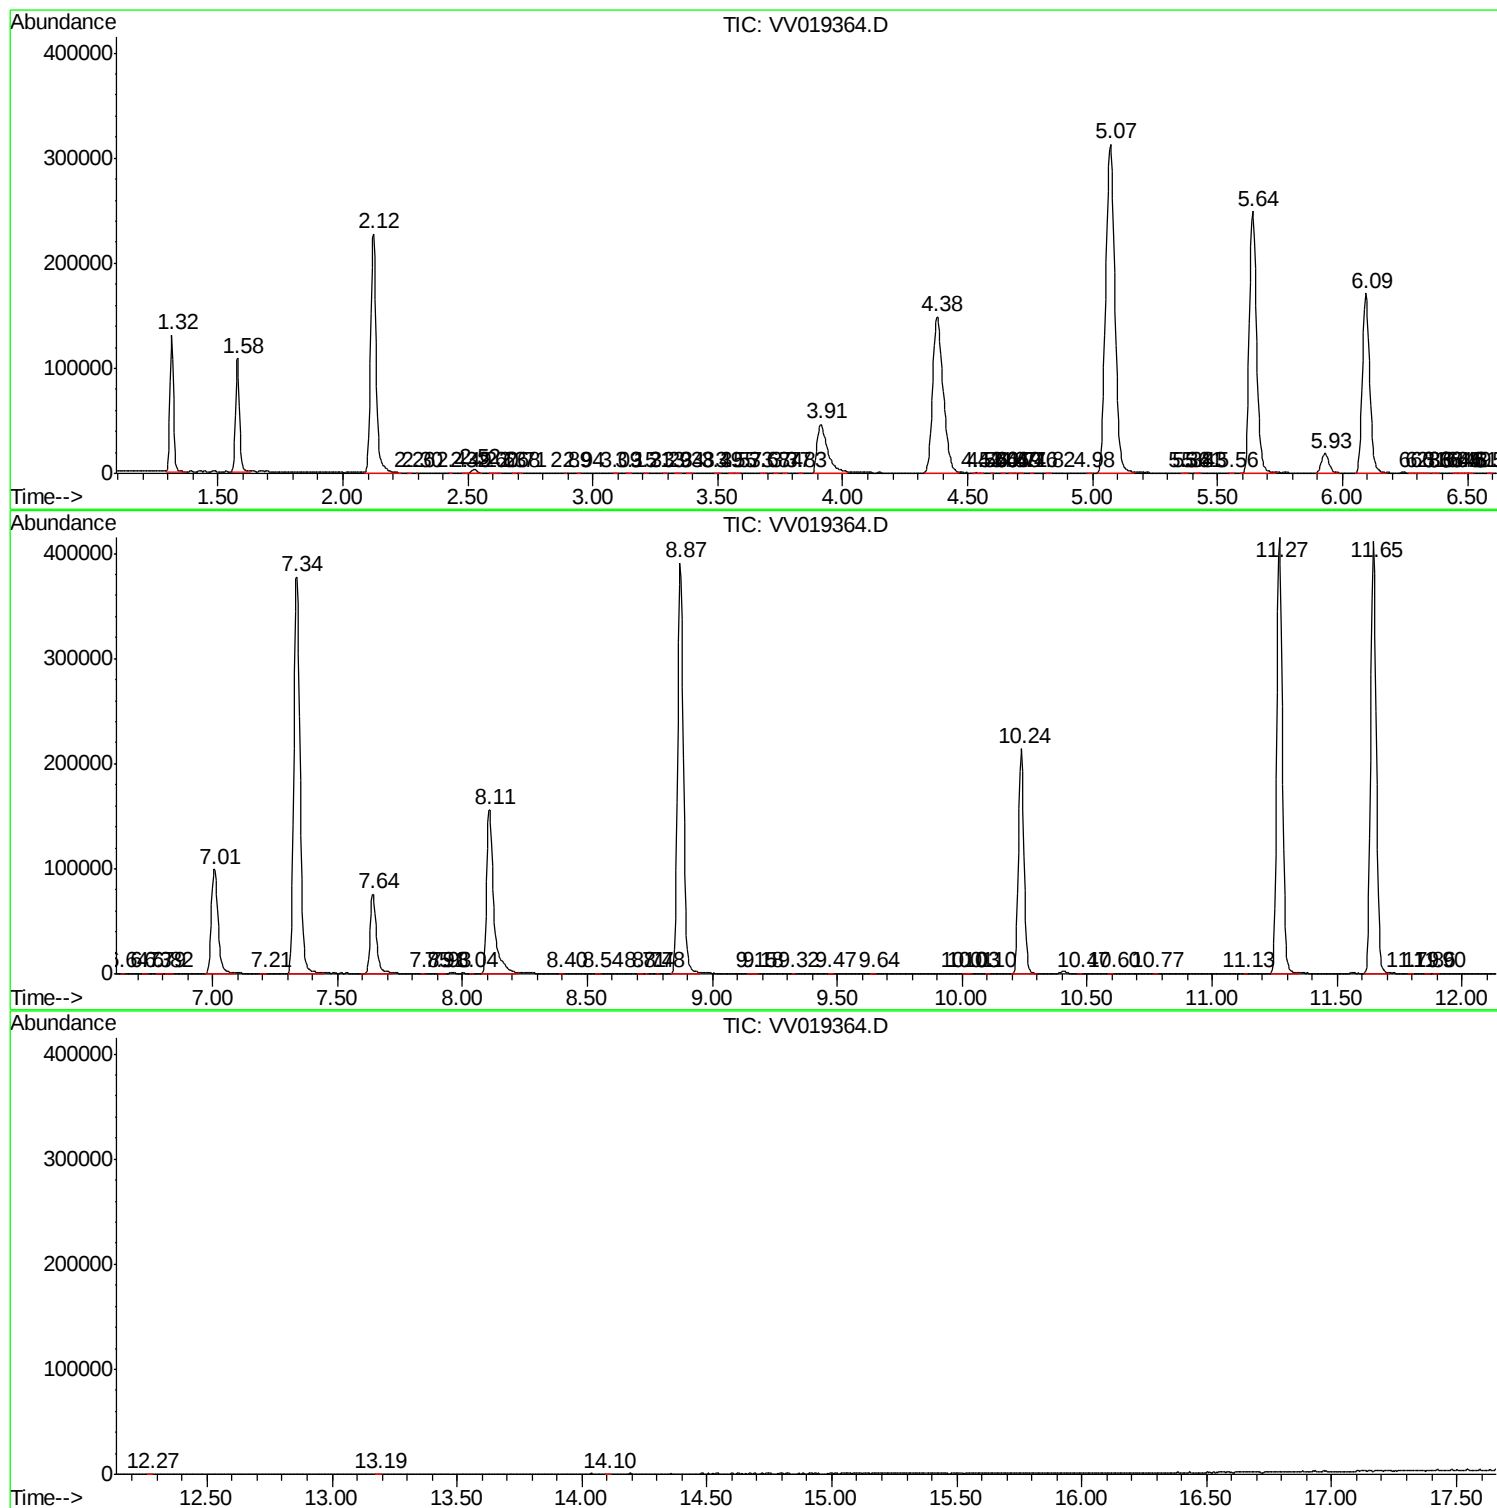

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111220\
Data File : VV019364.D
Acq On : 12 Nov 2020 20:09
Operator : SY/MD
Sample : L4711-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111220\
Data File : VV019364.D
Acq On : 12 Nov 2020 20:09
Operator : SY/MD
Sample : L4711-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc