


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV111220\
 Data File : VV019344.D
 Acq On : 12 Nov 2020 09:55
 Operator : SY/MD
 Sample : BFB93
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB93

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 13 01:06:25 2020

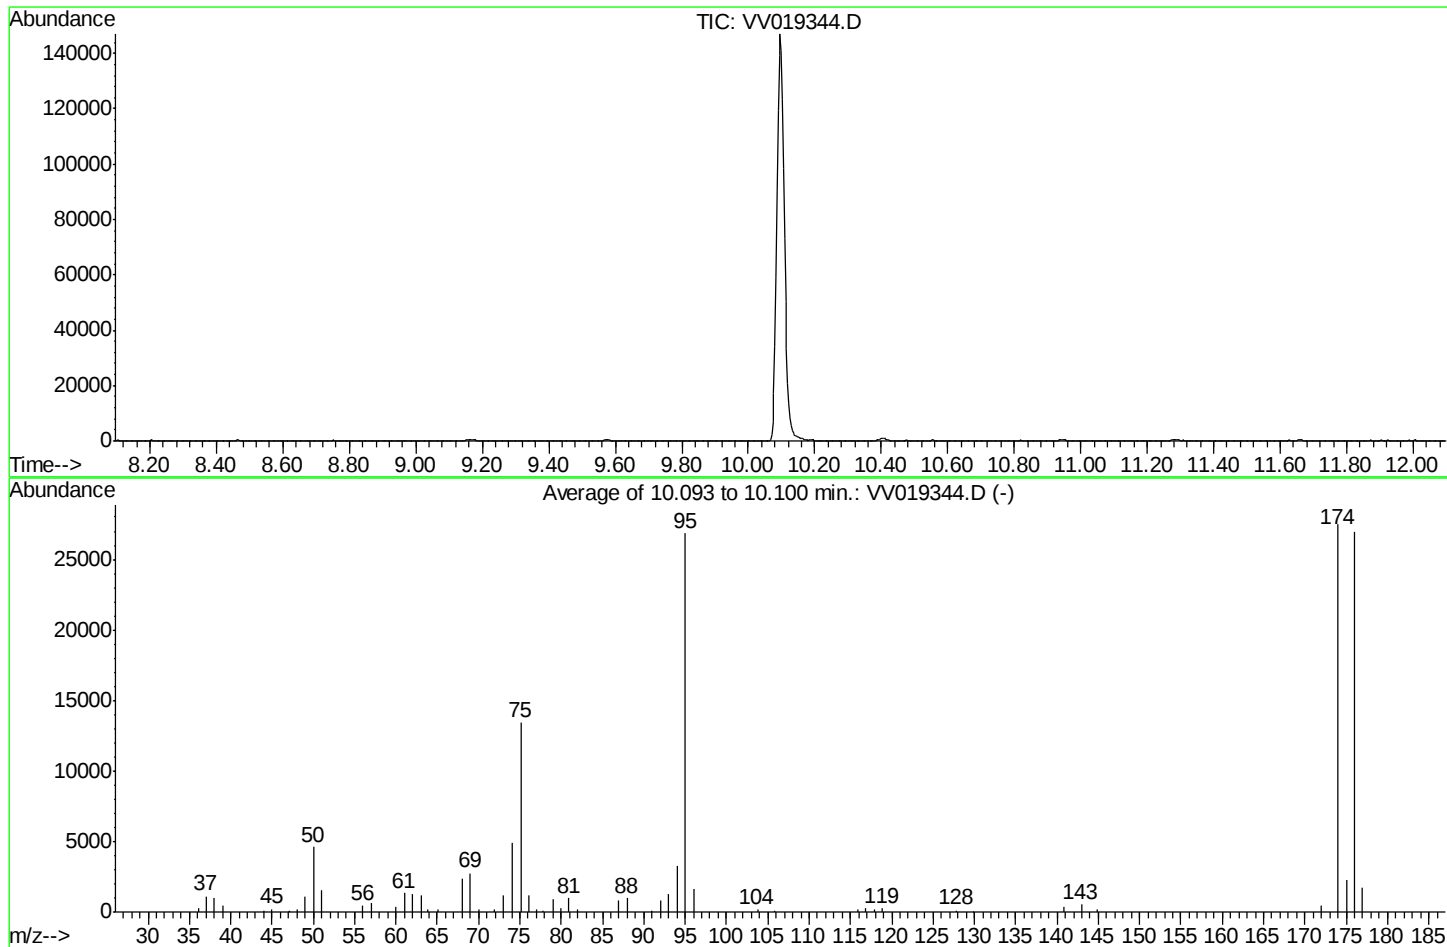

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4627	PASS
75	95	30	80	50.0	13428	PASS
95	95	100	100	100.0	26834	PASS
96	95	5	9	6.0	1600	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	102.4	27485	PASS
175	174	5	9	8.4	2309	PASS
176	174	95	101	97.9	26914	PASS
177	176	5	9	6.5	1739	PASS

m/z	Abundance
36.00	253.0
37.00	1161.0
38.00	1034.0
39.10	438.0
44.00	269.0
45.00	197.0
46.90	144.0
48.00	198.0
49.00	1132.0
50.00	4756.0
51.00	1554.0
56.00	446.0
57.10	619.0
59.90	297.0
61.00	1333.0
62.00	1264.0
63.00	1174.0
63.80	153.0
65.10	185.0
68.00	2297.0
69.00	2714.0
70.00	187.0
72.00	116.0
73.00	1130.0
74.00	4814.0
75.10	13291.0
76.10	1212.0
76.90	163.0
79.00	910.0
79.90	250.0
80.90	1088.0
81.90	205.0
86.90	928.0
88.00	952.0
90.90	111.0
92.10	791.0
93.00	1330.0
94.00	3164.0
95.00	26712.0
96.00	1540.0
103.80	163.0
105.80	143.0
115.90	130.0
116.80	240.0
117.80	146.0
118.80	226.0
127.80	123.0
140.80	381.0
143.00	501.0
144.90	184.0
171.90	456.0
174.00	26208.0
175.00	2251.0
176.00	26112.0
177.00	1634.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.10	248.0
37.00	1155.0
38.00	1089.0
39.10	519.0
43.90	288.0
44.90	193.0
47.10	165.0
48.00	196.0
49.00	1123.0
50.00	4782.0
51.00	1597.0
56.00	441.0
57.10	642.0
59.90	347.0
61.00	1363.0
62.00	1243.0
63.00	1203.0
63.90	146.0
65.10	199.0
68.00	2459.0
69.00	2889.0
70.00	233.0
72.00	151.0
73.10	1203.0
74.00	5137.0
75.10	13766.0
76.10	1251.0
77.00	148.0
77.80	117.0
78.90	971.0
79.90	247.0
80.90	1025.0
82.00	236.0
86.90	861.0
88.00	1032.0
91.00	110.0
92.00	838.0
93.00	1361.0
94.00	3403.0
95.00	27608.0
96.00	1654.0
103.80	193.0
105.90	132.0
115.90	151.0
116.80	274.0
117.80	187.0
118.90	297.0
127.90	113.0
129.90	108.0
140.90	415.0
142.90	540.0
144.90	200.0
171.90	516.0
174.00	28328.0
175.00	2387.0
176.00	27776.0
177.00	1768.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.10	235.0
37.00	1065.0
38.00	1016.0
39.10	508.0
43.90	280.0
44.90	179.0
47.00	195.0
48.00	189.0
49.00	972.0
50.00	4343.0
51.00	1443.0
55.90	372.0
57.00	611.0
59.90	336.0
61.00	1277.0
62.10	1186.0
63.00	1109.0
63.90	136.0
65.10	214.0
68.00	2385.0
69.00	2629.0
70.00	248.0
71.90	177.0
73.00	1243.0
74.00	4816.0
75.10	13227.0
76.10	1171.0
77.00	117.0
77.90	118.0
78.90	958.0
79.90	244.0
80.90	881.0
82.00	235.0
87.00	775.0
88.00	930.0
91.00	106.0
92.00	836.0
93.00	1206.0
94.00	3325.0
95.00	26184.0
96.00	1607.0
103.80	172.0
105.90	120.0
115.90	160.0
116.80	266.0
117.90	169.0
118.90	281.0
127.90	106.0
140.90	381.0
142.90	520.0
144.90	167.0
171.90	530.0
174.00	27920.0
175.00	2291.0
176.00	26856.0
177.00	1815.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
44.00	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93