

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023426.D
 Acq On : 12 Nov 2021 07:47
 Operator : SY/MD
 Sample : M4580-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 GB8H8

Quant Time: Nov 13 00:09:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 12 04:43:24 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/15/2021
 Supervised By : Mahesh Dadoda 11/15/2021

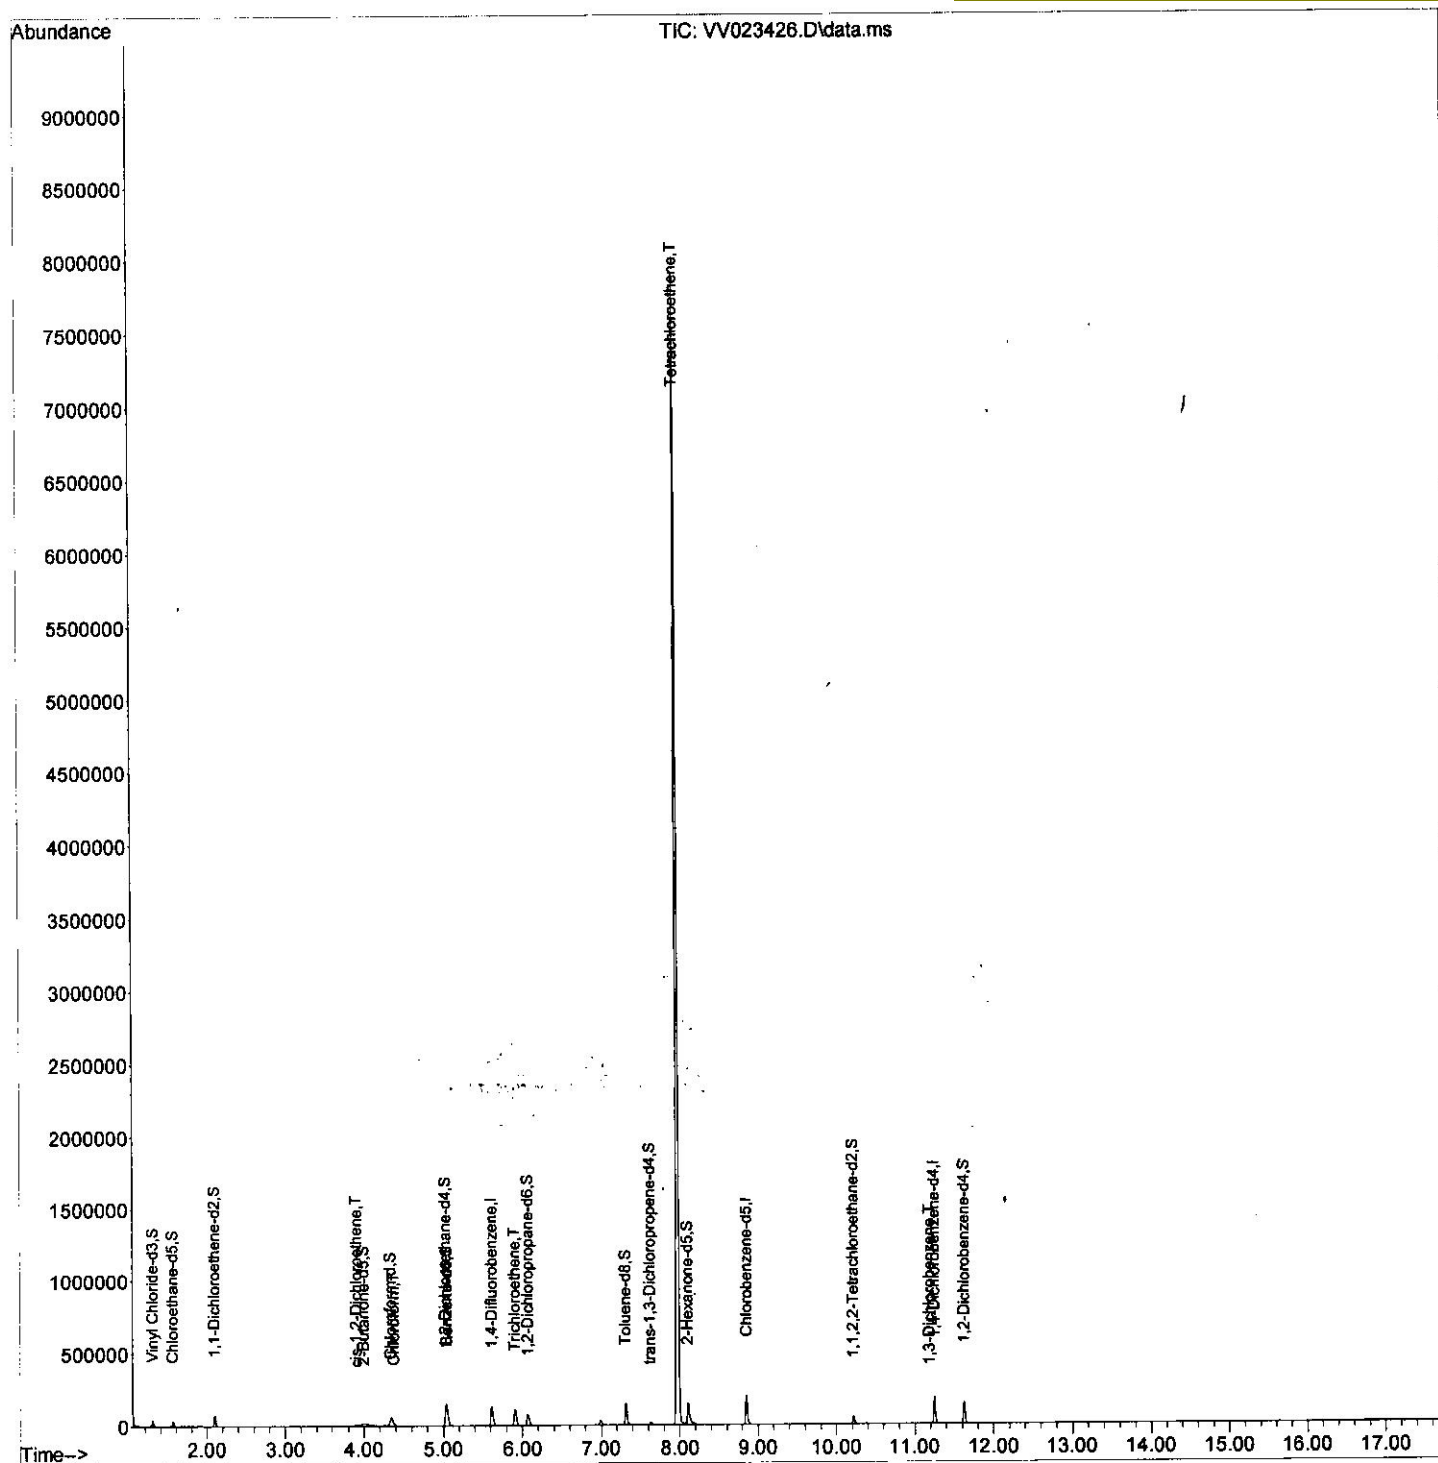

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023426.D
 Acq On : 12 Nov 2021 07:47
 Operator : SY/MD
 Sample : M4580-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 GB8H8

Manual Integrations APPROVED

Quant Time: Nov 13 00:09:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 12 04:43:24 2021
 Response via : Initial Calibration

Reviewed By : John Carlone 11/15/2021
 Supervised By : Mahesh Dadoda 11/15/2021

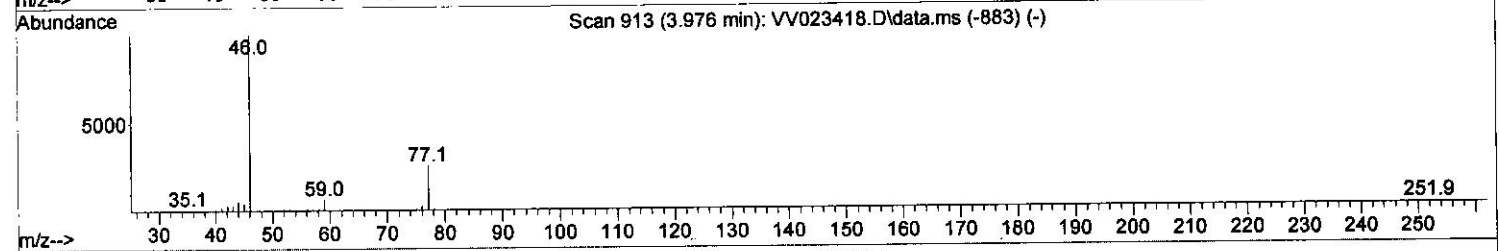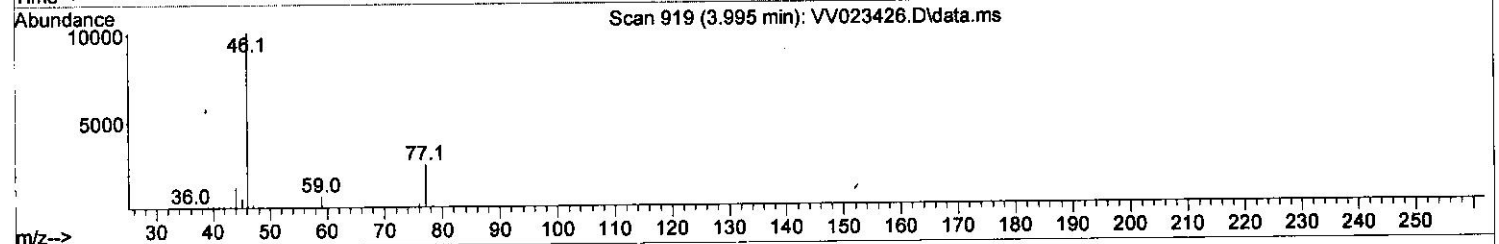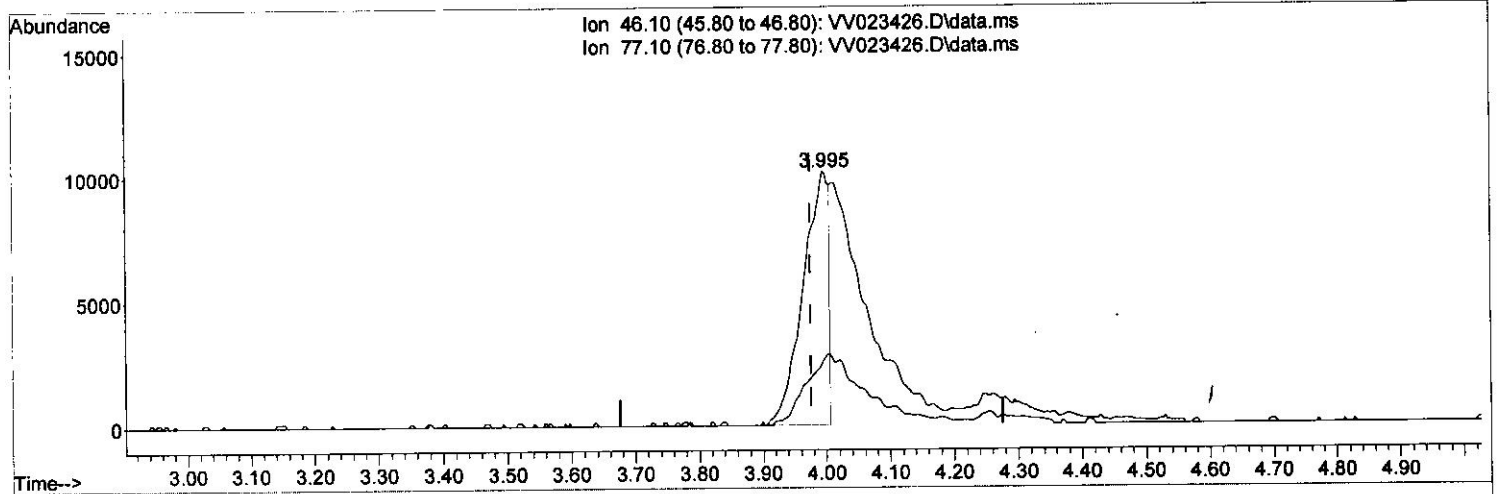

TIC: VV023426.D\data.ms

(20) 2-Butanone-d5 (S)

3.995min (+ 0.019) 23.09 ug/L

response 28184

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	31.45#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023426.D
 Acq On : 12 Nov 2021 07:47
 Operator : SY/MD
 Sample : M4580-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 GB8H8

Quant Time: Nov 13 00:09:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 12 04:43:24 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/15/2021
 Supervised By : Mahesh Dadoda 11/15/2021

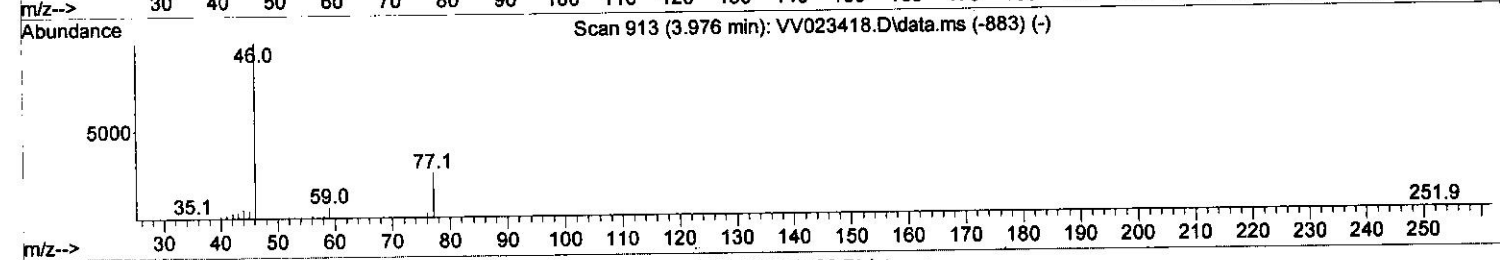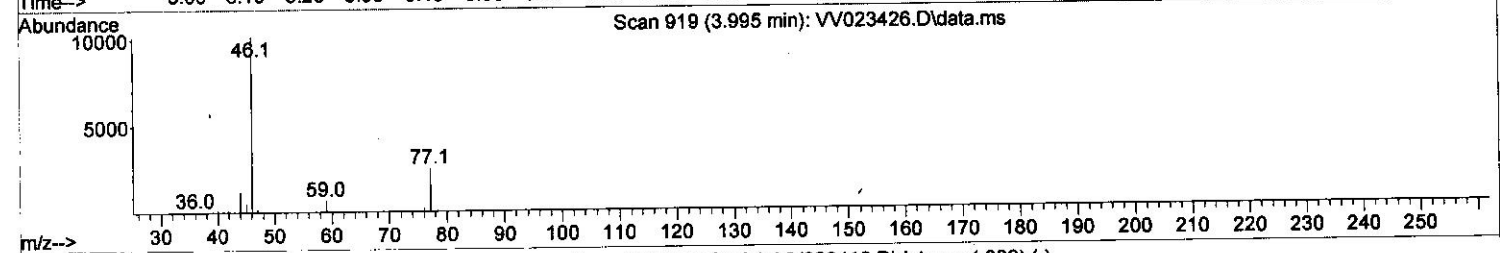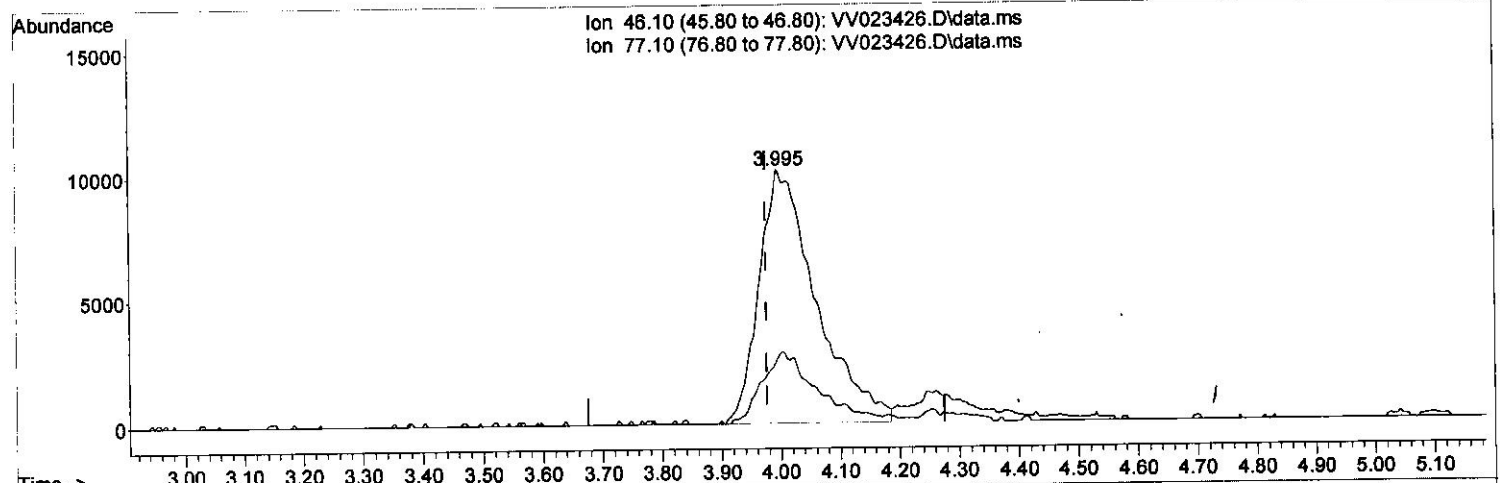

TIC: VV023426.D\data.ms

(20) 2-Butanone-d5 (S)

3.995min (+ 0.019) 55.05 ug/L m

response 67204

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	13.19#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111221\
 Data File : VW023426.D
 Acq On : 12 Nov 2021 07:47
 Operator : SY/MD
 Sample : M4580-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 GB8H8

Quant Time: Nov 13 00:09:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 12 04:43:24 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/15/2021
 Supervised By : Mahesh Dadoda 11/15/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	113119	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	115332	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50280	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	25587	3.611	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery =	72.200%		
7) Chloroethane-d5	1.558	69	23235	4.023	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery =	80.400%		
11) 1,1-Dichloroethene-d2	2.098	63	39582	2.984	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery =	59.600%#		
20) 2-Butanone-d5	3.995	46	67204m	55.046	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery =	110.100%		
24) Chloroform-d	4.343	84	58258	3.858	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery =	77.200%		
26) 1,2-Dichloroethane-d4	5.034	65	31531	4.643	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery =	92.800%		
32) Benzene-d6	5.043	84	124465	4.206	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery =	84.200%		
36) 1,2-Dichloropropane-d6	6.069	67	39214	4.502	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery =	90.000%		
41) Toluene-d8	7.313	98	101956	3.677	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery =	73.600%		
43) trans-1,3-Dichloroprop...	7.625	79	12120	3.669	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery =	73.400%		
46) 2-Hexanone-d5	8.104	63	54302	44.682	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery =	89.360%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26082	4.163	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery =	83.200%		
66) 1,2-Dichlorobenzene-d4	11.625	152	38598	4.610	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery =	92.200%		
Target Compounds						
22) cis-1,2-Dichloroethene	3.905	96	2903	0.364	ug/L #	93
25) Chloroform	4.375	83	9019	0.604	ug/L	96
34) Trichloroethene	5.908	95	39247	4.578	ug/L	99
47) Tetrachloroethene	7.973	164	1706642	229.718	ug/L	99
64) 1,3-Dichlorobenzene	11.188	146	1186	0.080	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed