

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023460.D
 Acq On : 12 Nov 2021 22:49
 Operator : SY/MD
 Sample : M4616-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1X7

Quant Time: Nov 13 01:59:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 13 01:39:11 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/15/2021
 Supervised By :Mahesh Dadoda 11/15/2021

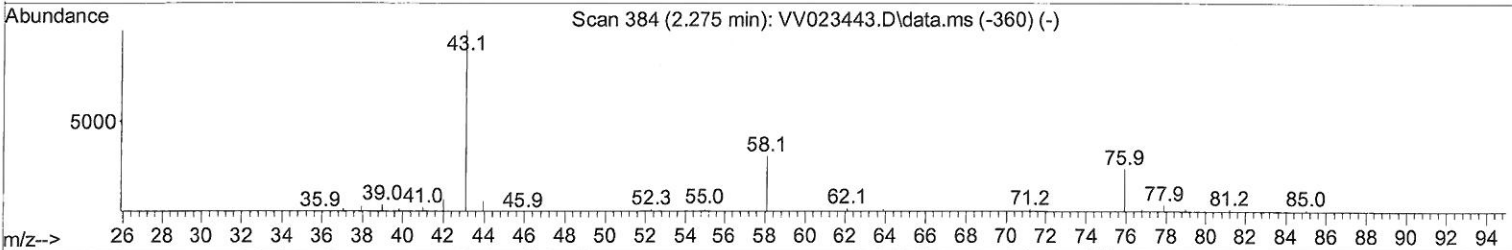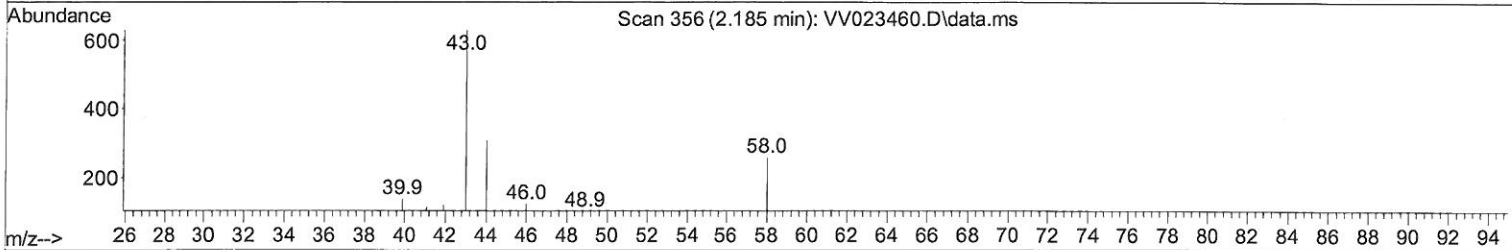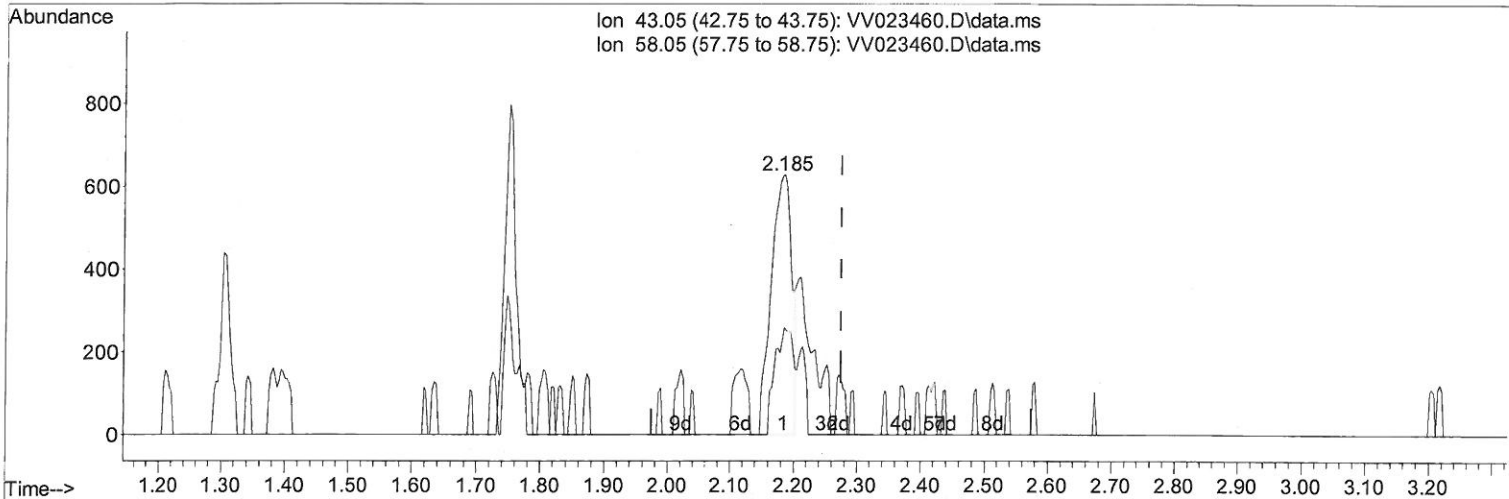

TIC: VV023460.D\data.ms

(13) Acetone (T)

2.185min (-0.090) 1.77 ug/L

response 1377

| Ion | Exp% | Act% |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 27.70 | 38.63 |
| 0.00 | 0.00 | 0.00 |
| 0.00 | 0.00 | 0.00 |

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111221\
 Data File : VW023460.D
 Acq On : 12 Nov 2021 22:49
 Operator : SY/MD
 Sample : M4616-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 BG1X7

Quant Time: Nov 13 01:59:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 13 01:39:11 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/15/2021
 Supervised By : Mahesh Dadoda 11/15/2021

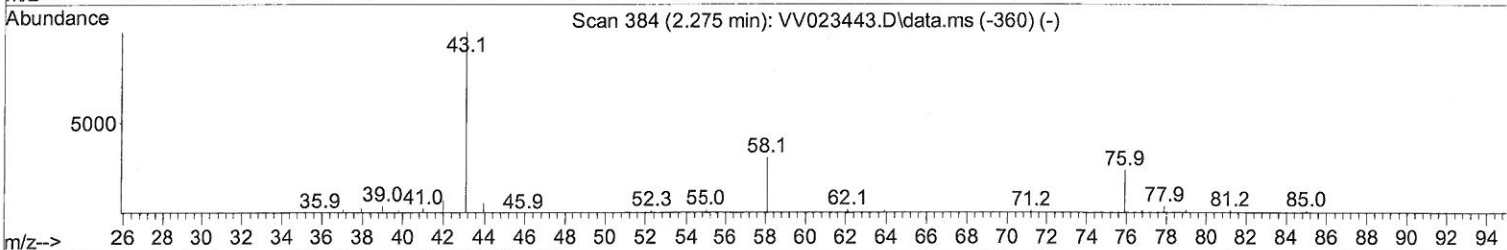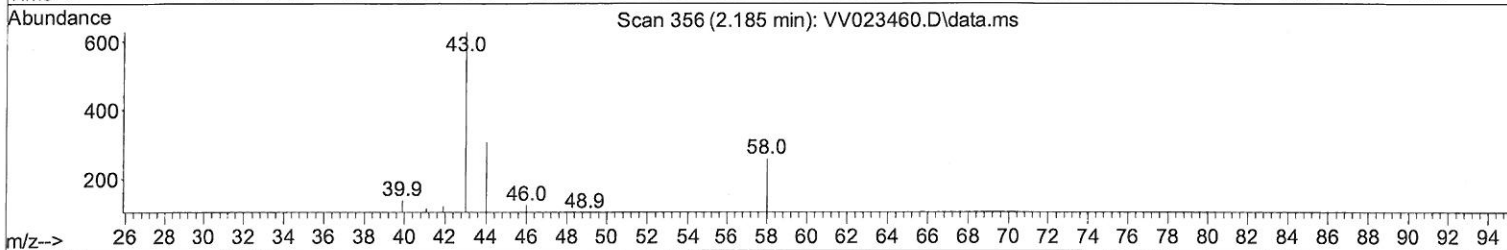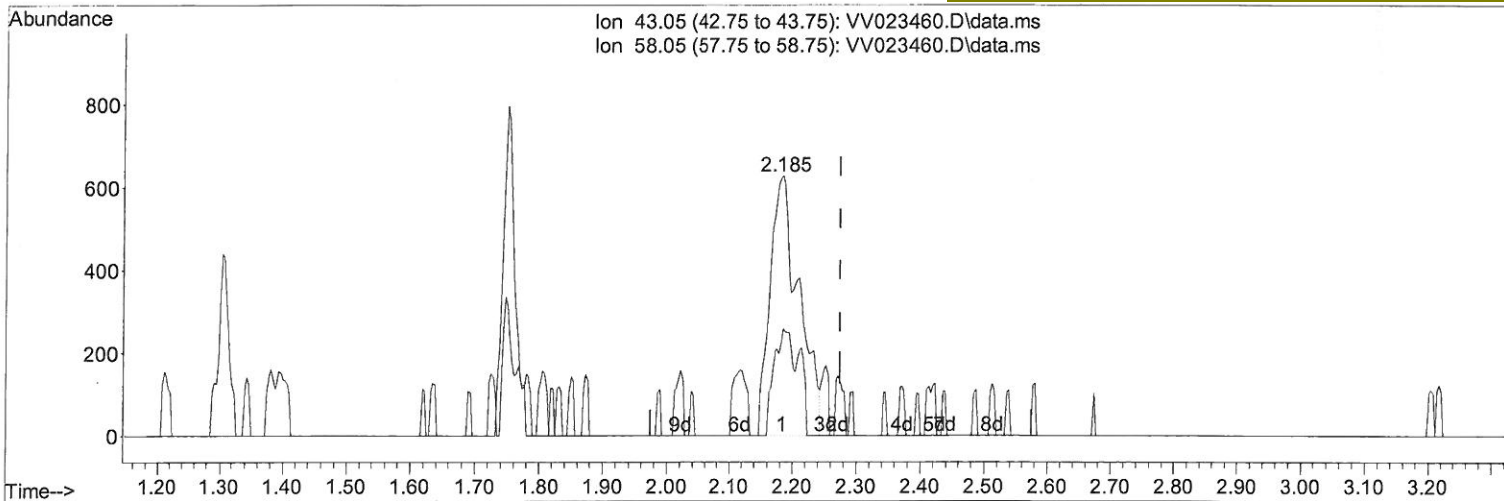

TIC: VV023460.D\data.ms

(13) Acetone (T)

2.185min (-0.090) 2.57 ug/L m

response 1993

| Ion | Exp% | Act% |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 27.70 | 26.69 |
| 0.00 | 0.00 | 0.00 |
| 0.00 | 0.00 | 0.00 |

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023460.D
 Acq On : 12 Nov 2021 22:49
 Operator : SY/MD
 Sample : M4616-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 BG1X7

Quant Time: Nov 13 01:59:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 13 01:39:11 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/15/2021
 Supervised By : Mahesh Dadoda 11/15/2021

| Compound | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|-------------------------------|----------------|------|----------------------|--------|--------|----------|
| ----- | | | | | | |
| Internal Standards | | | | | | |
| 1) 1,4-Difluorobenzene | 5.619 | 114 | 117661 | 5.000 | ug/L | -0.02 |
| 28) Chlorobenzene-d5 | 8.853 | 117 | 115687 | 5.000 | ug/L | 0.00 |
| 58) 1,4-Dichlorobenzene-d4 | 11.252 | 152 | 52262 | 5.000 | ug/L | 0.00 |
| | | | | | | |
| System Monitoring Compounds | | | | | | |
| 4) Vinyl Chloride-d3 | 1.307 | 65 | 49826 | 6.760 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 40 - 130 | | Recovery = 135.200%# | | | |
| 7) Chloroethane-d5 | 1.568 | 69 | 35936 | 5.982 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 65 - 130 | | Recovery = 119.600% | | | |
| 11) 1,1-Dichloroethene-d2 | 2.108 | 63 | 64914 | 4.704 | ug/L | -0.01 |
| Spiked Amount 5.000 | Range 60 - 125 | | Recovery = 94.000% | | | |
| 20) 2-Butanone-d5 | 3.892 | 46 | 81804 | 64.418 | ug/L | -0.10 |
| Spiked Amount 50.000 | Range 40 - 130 | | Recovery = 128.840% | | | |
| 24) Chloroform-d | 4.349 | 84 | 80698 | 5.137 | ug/L | -0.01 |
| Spiked Amount 5.000 | Range 70 - 125 | | Recovery = 102.800% | | | |
| 26) 1,2-Dichloroethane-d4 | 5.034 | 65 | 40965 | 5.799 | ug/L | -0.02 |
| Spiked Amount 5.000 | Range 70 - 130 | | Recovery = 116.000% | | | |
| 32) Benzene-d6 | 5.053 | 84 | 161885 | 5.454 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 70 - 125 | | Recovery = 109.000% | | | |
| 36) 1,2-Dichloropropane-d6 | 6.069 | 67 | 48863 | 5.592 | ug/L | -0.03 |
| Spiked Amount 5.000 | Range 60 - 140 | | Recovery = 111.800% | | | |
| 41) Toluene-d8 | 7.316 | 98 | 139469 | 5.014 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 70 - 130 | | Recovery = 100.200% | | | |
| 43) trans-1,3-Dichloroprop... | 7.625 | 79 | 16686 | 5.036 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 55 - 130 | | Recovery = 100.800% | | | |
| 46) 2-Hexanone-d5 | 8.091 | 63 | 52267 | 42.876 | ug/L | -0.02 |
| Spiked Amount 50.000 | Range 45 - 130 | | Recovery = 85.760% | | | |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84 | 30408 | 4.839 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 65 - 120 | | Recovery = 96.800% | | | |
| 66) 1,2-Dichlorobenzene-d4 | 11.625 | 152 | 50241 | 5.773 | ug/L | 0.00 |
| Spiked Amount 5.000 | Range 80 - 120 | | Recovery = 115.400% | | | |
| | | | | | | |
| Target Compounds | | | | | | Qvalue |
| 9) Trichlorofluoromethane | 1.754 | 101 | 1206490 | 82.421 | ug/L | 99 |
| 10) 1,1,2-Trichloro-1,2,2-... | 2.117 | 101 | 12438 | 1.688 | ug/L | 98 |
| 12) 1,1-Dichloroethene | 2.117 | 96 | 3660 | 0.522 | ug/L # | 1 |
| 13) Acetone | 2.185 | 43 | 1993m | 2.568 | ug/L | 96 |
| 19) 1,1-Dichloroethane | 3.191 | 63 | 30774 | 2.113 | ug/L | 96 |
| 22) cis-1,2-Dichloroethene | 3.912 | 96 | 6847 | 0.825 | ug/L # | 86 |
| 29) 1,1,1-Trichloroethane | 4.616 | 97 | 2137 | 0.152 | ug/L # | 58 |
| 34) Trichloroethene | 5.915 | 95 | 49645 | 5.774 | ug/L | 97 |
| 47) Tetrachloroethene | 7.976 | 164 | 917 | 0.123 | ug/L | 84 |
| ----- | | | | | | |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023460.D
Acq On : 12 Nov 2021 22:49
Operator : SY/MD
Sample : M4616-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sampled :
BG1X7

Quant Time: Nov 13 01:59:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 13 01:39:11 2021
Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/15/2021
Supervised By : Mahesh Dadoda 11/15/2021

