

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023444.D
 Acq On : 12 Nov 2021 16:25
 Operator : SY/MD
 Sample : VV1112WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Quant Time: Nov 13 01:39:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 13 01:39:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	123886	5.000	ug/L	-0.03
28) Chlorobenzene-d5	8.850	117	117336	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49903	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.297	65	28437	3.664	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.200%
7) Chloroethane-d5	1.558	69	25621	4.051	ug/L	-0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.000%
11) 1,1-Dichloroethene-d2	2.098	63	44989	3.097	ug/L	-0.02
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.000%
20) 2-Butanone-d5	3.957	46	77108	57.669	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.340%
24) Chloroform-d	4.339	84	61470	3.716	ug/L	-0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.400%
26) 1,2-Dichloroethane-d4	5.027	65	36152	4.861	ug/L	-0.03
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.200%
32) Benzene-d6	5.034	84	122055	4.054	ug/L	-0.03
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.000%
36) 1,2-Dichloropropane-d6	6.069	67	42808	4.830	ug/L	-0.03
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%
41) Toluene-d8	7.313	98	109610	3.885	ug/L	-0.01
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.800%
43) trans-1,3-Dichloroprop...	7.625	79	14623	4.351	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.000%
46) 2-Hexanone-d5	8.104	63	44472	35.969	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	71.940%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27057	4.245	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	40944	4.927	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.600%
Target Compounds						
					Qvalue	
25) Chloroform	4.365	83	6007	0.368	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023444.D
Acq On : 12 Nov 2021 16:25
Operator : SY/MD
Sample : VV1112WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK251

Quant Time: Nov 13 01:39:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 13 01:39:11 2021
Response via : Initial Calibration

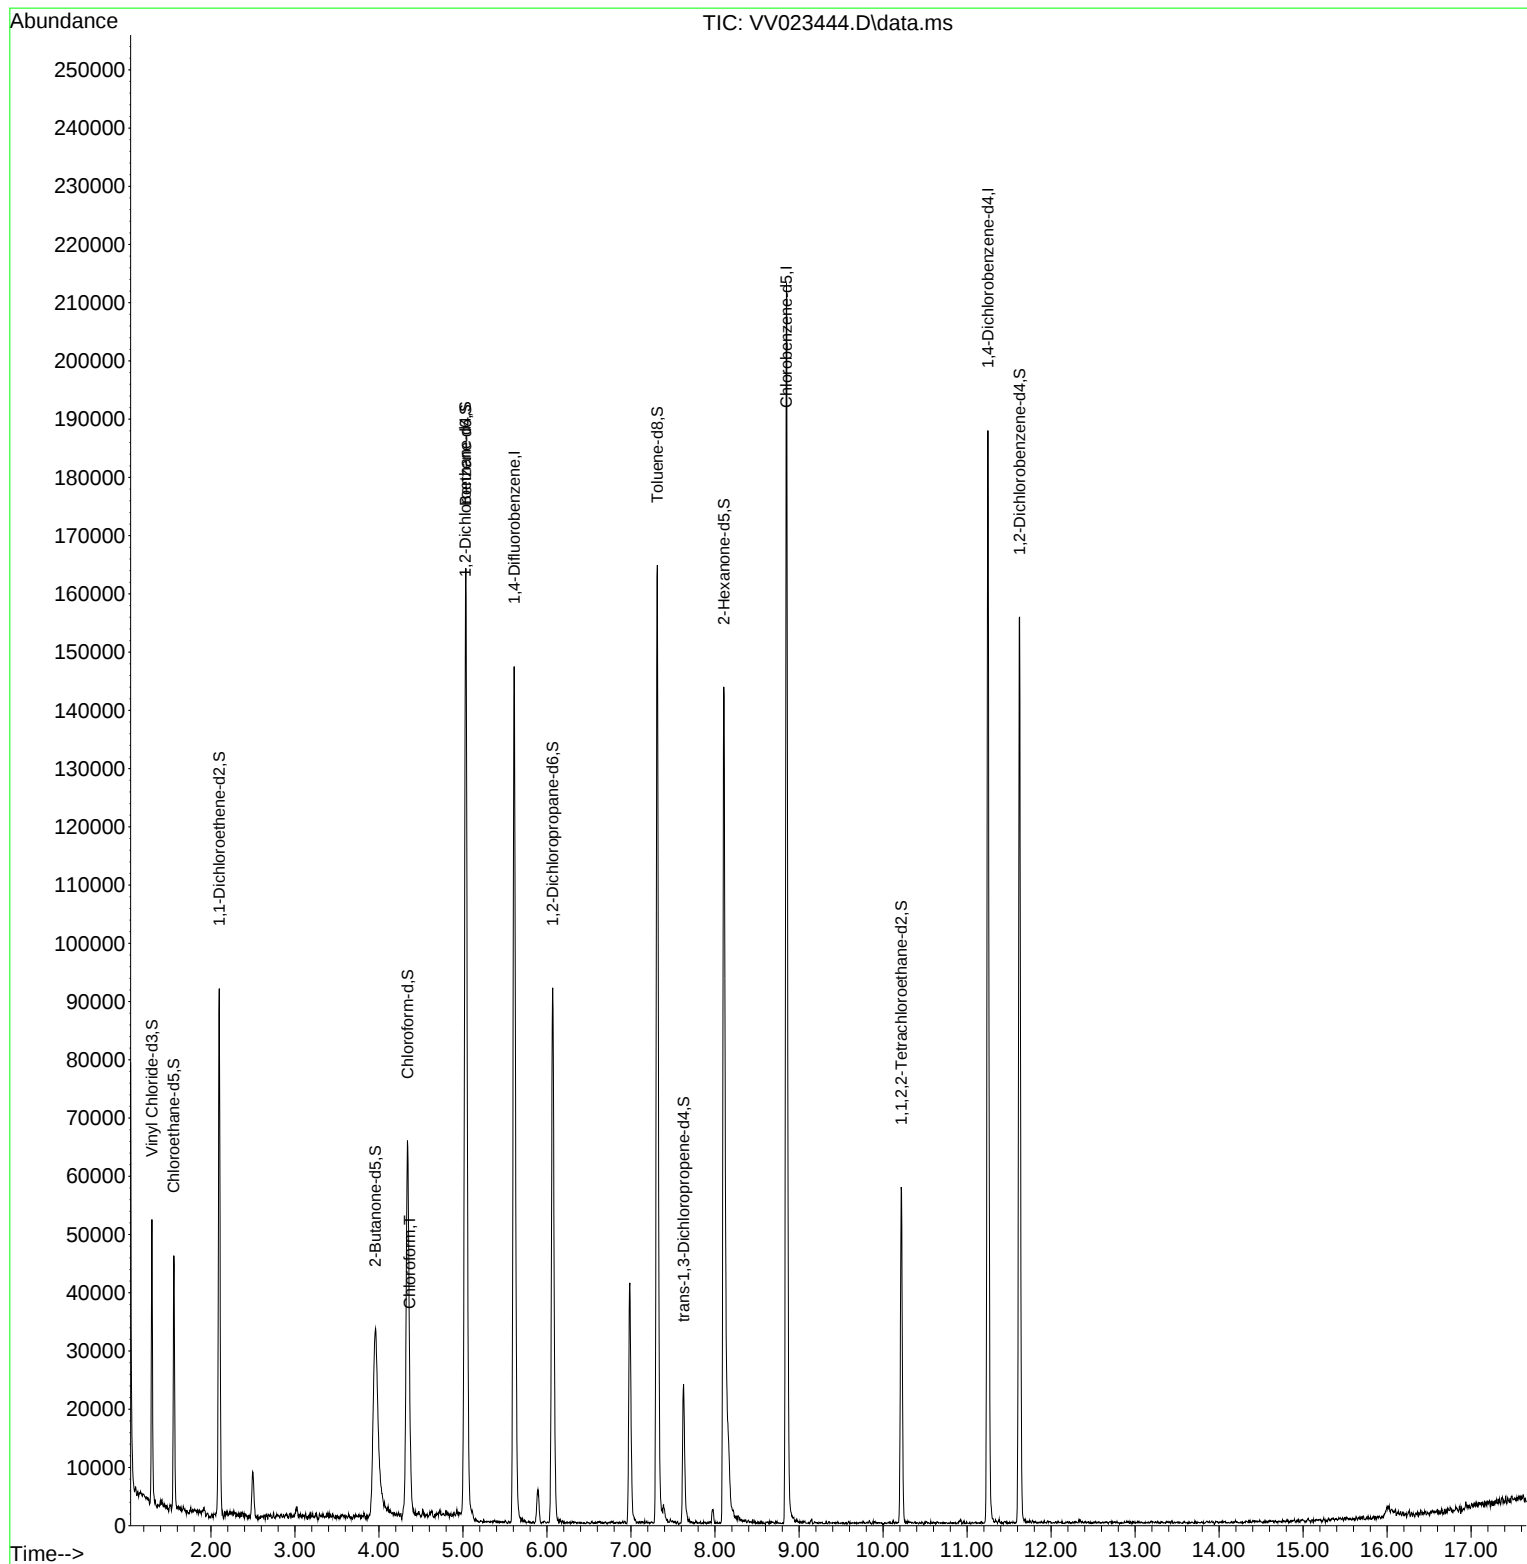

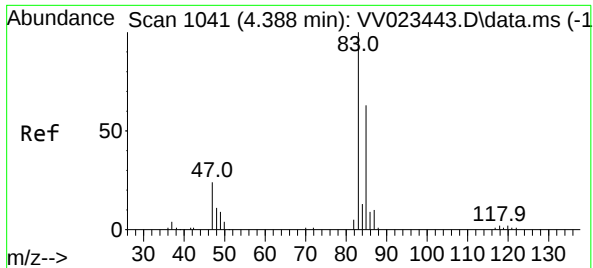

#25
 Chloroform
 Concen: 0.368 ug/L
 RT: 4.365 min Scan# 10
 Delta R.T. -0.023 min
 Lab File: VV023444.D
 Acq: 12 Nov 2021 16:25

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK251

Tgt Ion: 83 Resp: 6007
 Ion Ratio Lower Upper
 83 100
 85 64.9 46.8 86.8

