

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023420.D
 Acq On : 12 Nov 2021 05:23
 Operator : SY/MD
 Sample : M4580-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8H2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	92	rBV	49217	48173	13.81%	1.523%
2	1.561	155	162	172	rVB	40495	44898	12.87%	1.420%
3	2.101	320	330	345	rBV	85034	120252	34.47%	3.803%
4	3.931	887	899	925	rBV	19681	83790	24.02%	2.650%
5	4.349	1012	1029	1050	rBV	63549	159294	45.66%	5.037%
6	5.047	1230	1246	1269	rBV3	142086	348864	100.00%	11.032%
7	5.616	1411	1423	1449	rBV	132269	272401	78.08%	8.614%
8	5.912	1504	1515	1516	rBV5	3013	3861	1.11%	0.122%
9	6.072	1549	1565	1588	rBV	80061	169552	48.60%	5.362%
10	6.989	1840	1850	1872	rBV2	34055	64942	18.62%	2.054%
11	7.317	1939	1952	1972	rBV	156159	274526	78.69%	8.681%
12	7.629	2037	2049	2063	rBV	20572	37210	10.67%	1.177%
13	7.976	2144	2157	2176	rBV	201142	334195	95.80%	10.568%
14	8.095	2184	2194	2229	rBV2	118665	264184	75.73%	8.354%
15	8.854	2418	2430	2454	rBV	205386	340051	97.47%	10.754%
16	10.217	2842	2854	2868	rBV	53064	83770	24.01%	2.649%
17	11.249	3162	3175	3199	rBV	181437	282093	80.86%	8.921%
18	11.542	3258	3266	3275	rBV6	1929	3586	1.03%	0.113%
19	11.625	3281	3292	3310	rBV	143101	226581	64.95%	7.165%




Sum of corrected areas: 3162223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023420.D
Acq On : 12 Nov 2021 05:23
Operator : SY/MD
Sample : M4580-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

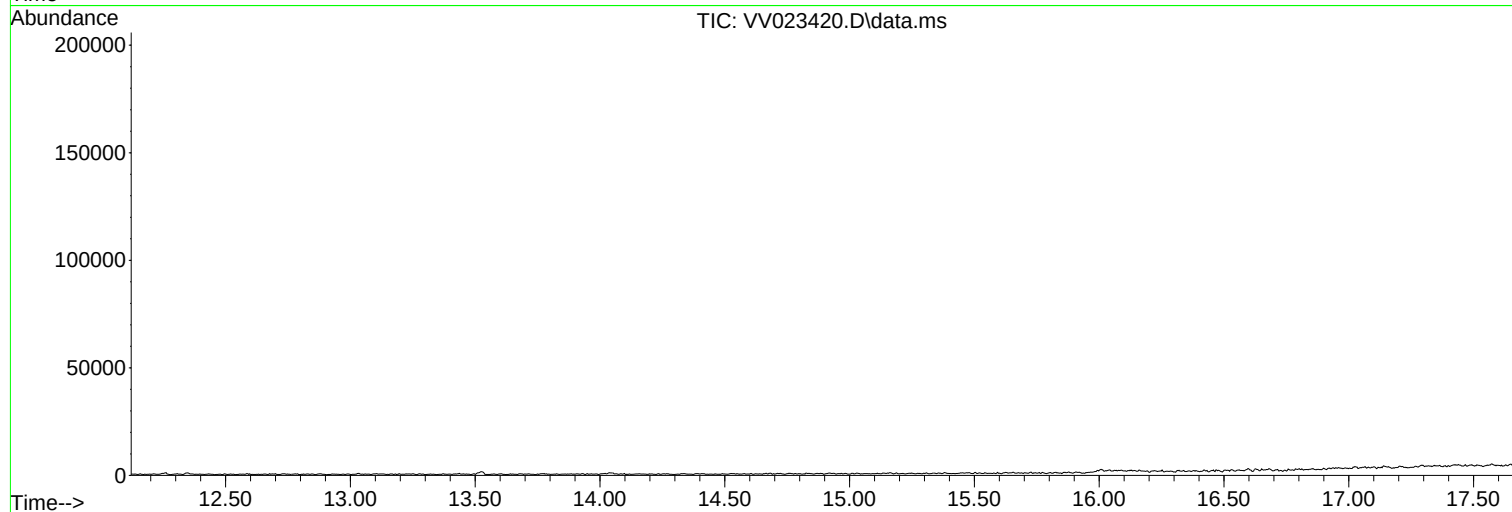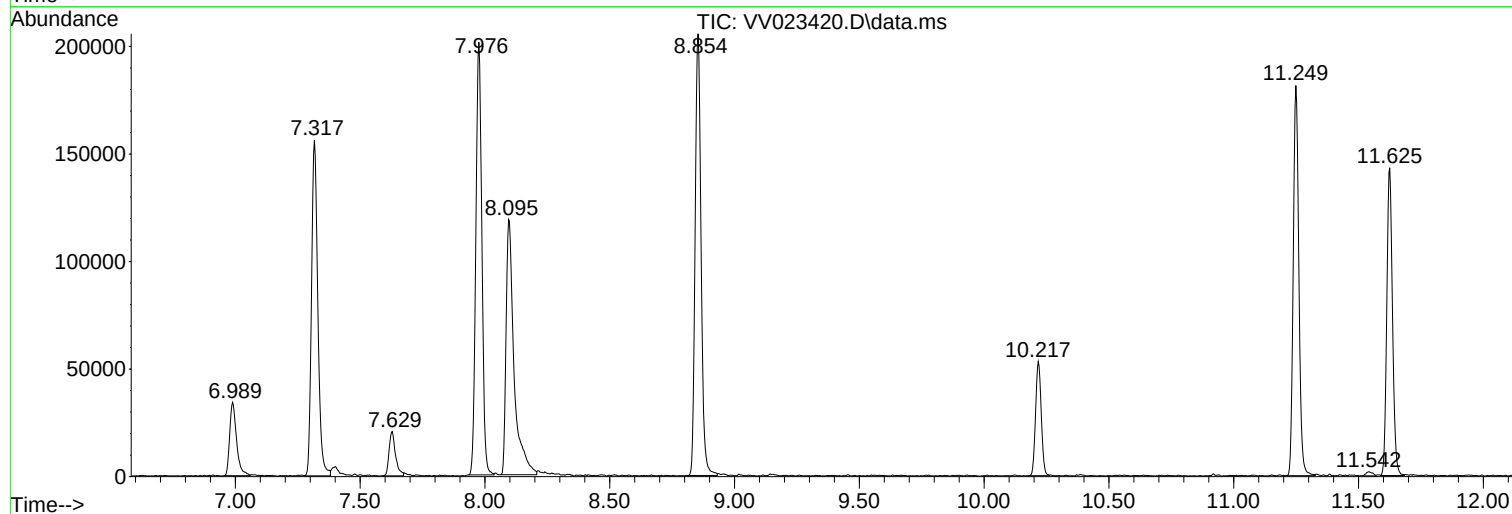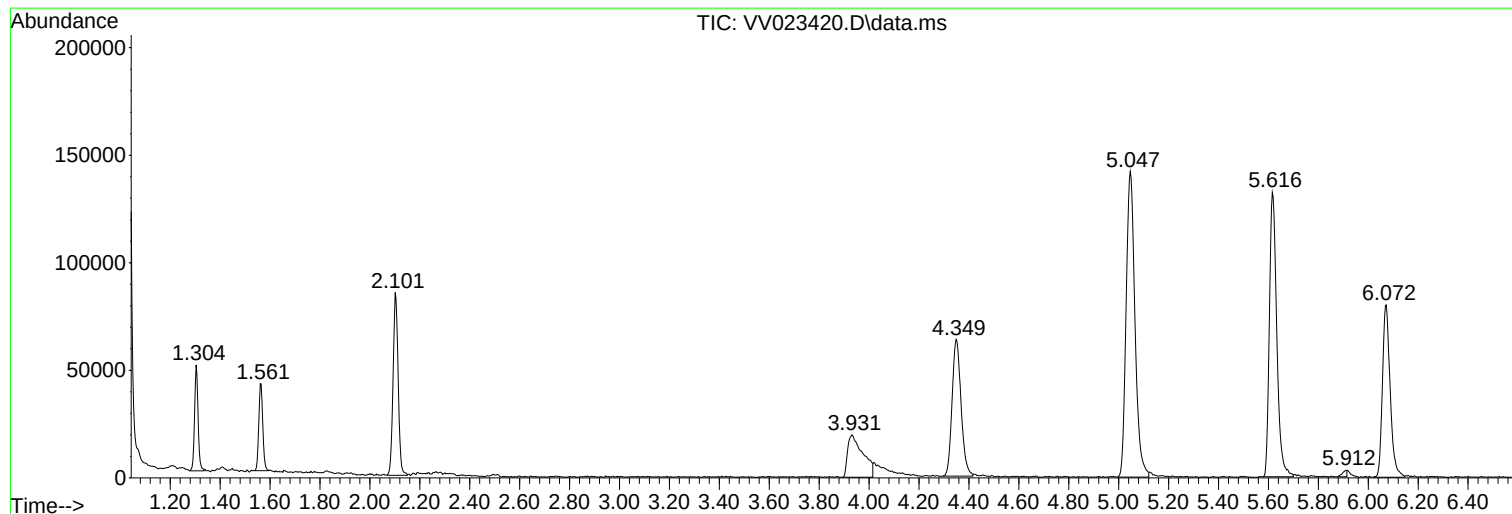

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023420.D
Acq On : 12 Nov 2021 05:23
Operator : SY/MD
Sample : M4580-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023420.D
Acq On : 12 Nov 2021 05:23
Operator : SY/MD
Sample : M4580-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc