

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023424.D
 Acq On : 12 Nov 2021 06:59
 Operator : SY/MD
 Sample : M4580-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8H6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	59	rBV	137102	117444	33.66%	3.572%
2	1.304	76	82	94	rVB	48553	51241	14.68%	1.558%
3	1.568	154	164	177	rBV	44686	51940	14.88%	1.580%
4	2.108	321	332	348	rBV	87253	125473	35.96%	3.816%
5	3.912	882	893	923	rBV	15572	67505	19.35%	2.053%
6	4.352	1014	1030	1055	rVB2	60268	161308	46.23%	4.906%
7	5.050	1228	1247	1277	rBV3	137218	348947	100.00%	10.612%
8	5.619	1410	1424	1445	rBV	132454	273235	78.30%	8.309%
9	6.072	1551	1565	1586	rBV	78824	165379	47.39%	5.029%
10	6.989	1839	1850	1870	rBV	33501	65188	18.68%	1.982%
11	7.317	1941	1952	1972	rBV	156615	278998	79.95%	8.485%
12	7.629	2039	2049	2064	rBV2	19740	37232	10.67%	1.132%
13	7.976	2137	2157	2174	rBV	170715	290348	83.21%	8.830%
14	8.095	2183	2194	2230	rBV2	100053	271254	77.74%	8.249%
15	8.854	2416	2430	2452	rBV	209015	348754	99.94%	10.606%
16	10.217	2842	2854	2870	rBV2	54968	88679	25.41%	2.697%
17	11.249	3164	3175	3194	rBV	187612	294065	84.27%	8.943%
18	11.538	3254	3265	3280	rBV4	6255	11906	3.41%	0.362%
19	11.625	3280	3292	3307	rBV	149250	239373	68.60%	7.280%




Sum of corrected areas: 3288269

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023424.D
Acq On : 12 Nov 2021 06:59
Operator : SY/MD
Sample : M4580-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

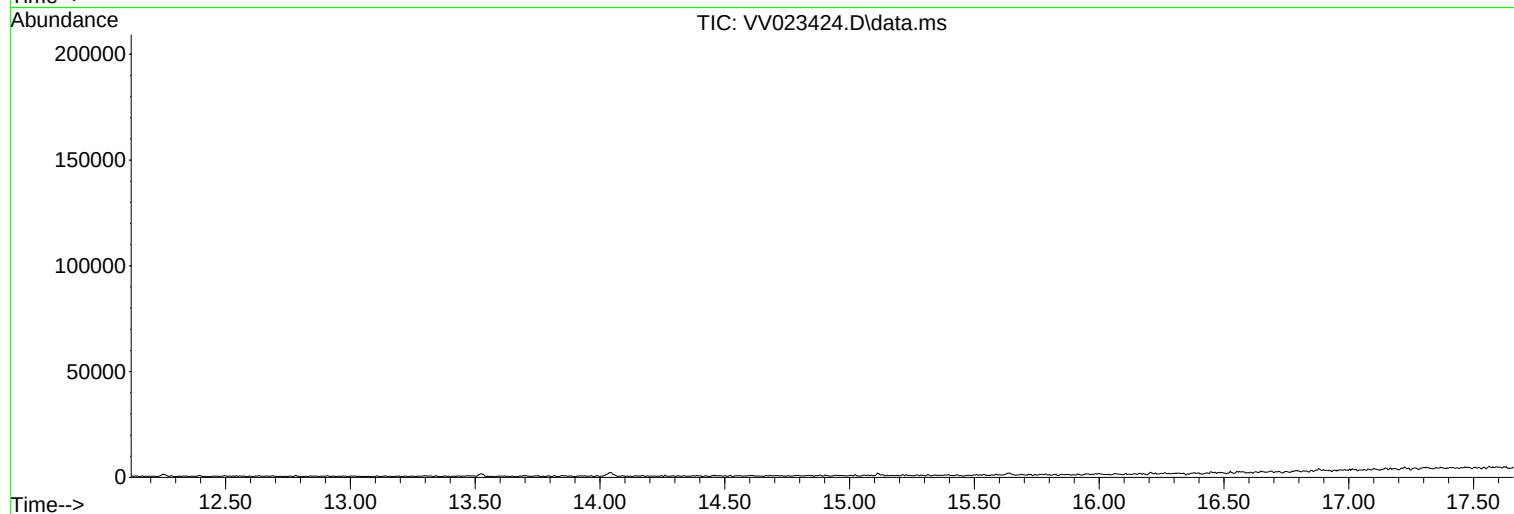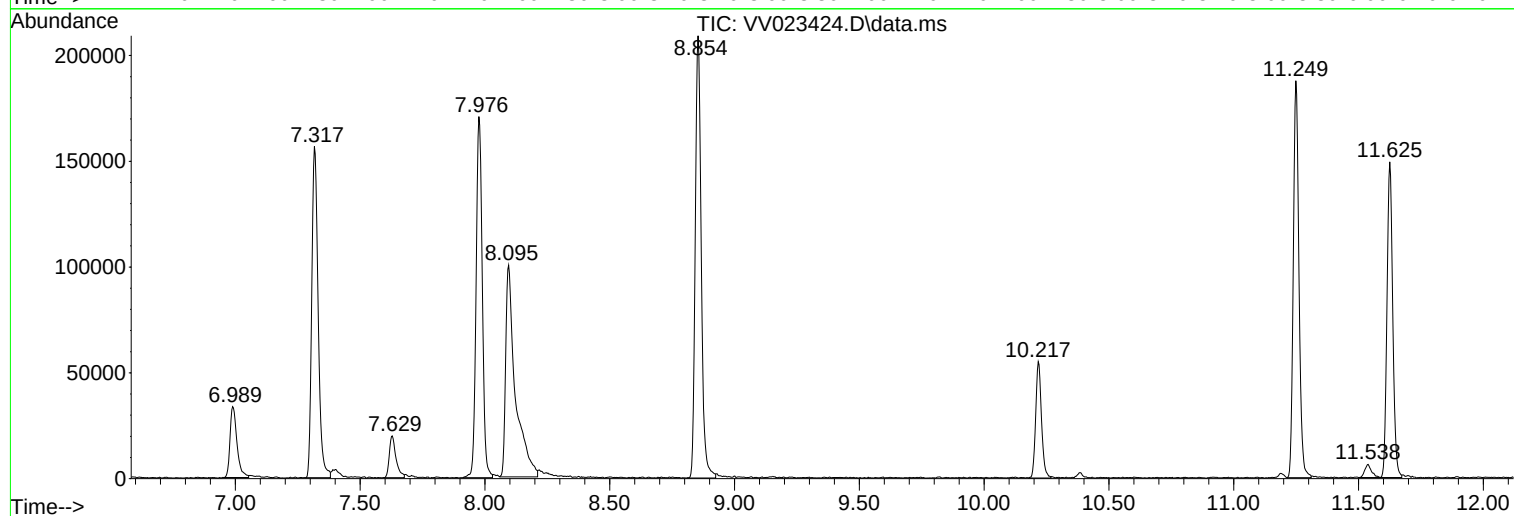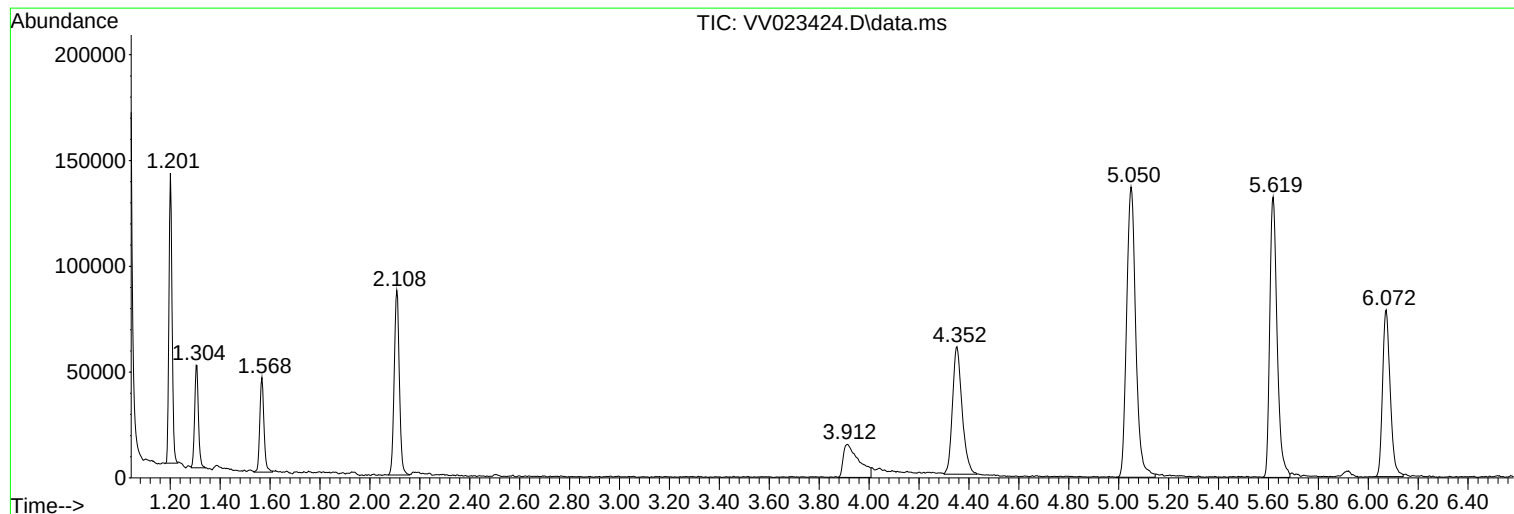

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023424.D
Acq On : 12 Nov 2021 06:59
Operator : SY/MD
Sample : M4580-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	2.15 ug/L	117444	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			Ethyne, chloro-	60	C2HCl	000593-63-5	5
3			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
4			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4
5			Cyanogen chloride	61	CClN	000506-77-4	4

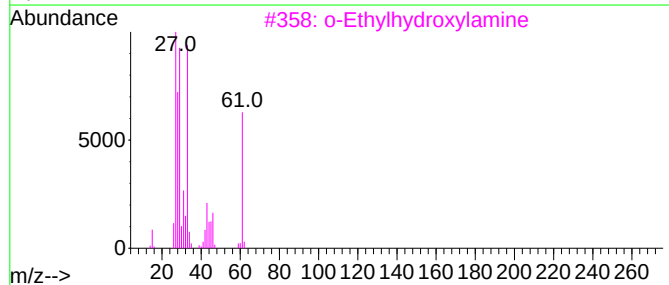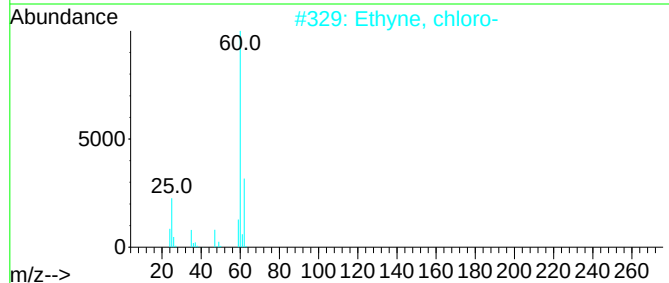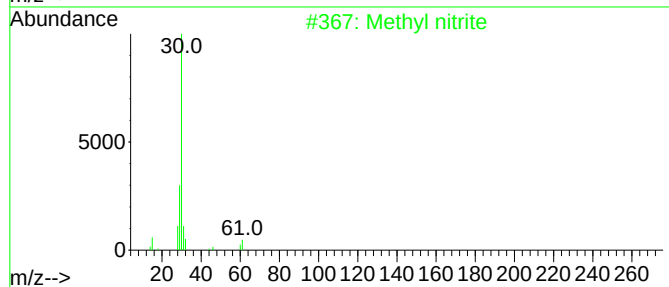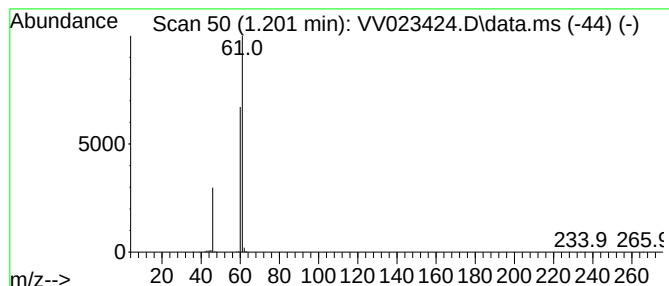

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023424.D
Acq On : 12 Nov 2021 06:59
Operator : SY/MD
Sample : M4580-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	2.1	ug/L	117444	1	5.619	273235	5.0