

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023428.D
 Acq On : 12 Nov 2021 08:44
 Operator : SY/MD
 Sample : M4542-06DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG266DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	60	rBV	143721	124761	32.82%	3.137%
2	1.304	76	82	91	rBV2	52636	55182	14.52%	1.387%
3	1.568	155	164	174	rBV	44512	52590	13.83%	1.322%
4	2.105	322	331	343	rBV	83884	122751	32.29%	3.086%
5	2.507	448	456	464	rVB5	2918	5023	1.32%	0.126%
6	3.188	655	668	686	rBV	29258	62288	16.38%	1.566%
7	3.908	876	892	912	rBV3	49098	145940	38.39%	3.669%
8	4.346	1012	1028	1050	rBV2	59643	156074	41.05%	3.924%
9	4.603	1091	1108	1129	rBV3	63903	162296	42.69%	4.081%
10	5.047	1229	1246	1271	rBV2	130906	327266	86.08%	8.229%
11	5.616	1410	1423	1442	rBV	118809	247261	65.04%	6.217%
12	5.912	1492	1515	1536	rBV	188095	380167	100.00%	9.559%
13	6.069	1550	1564	1581	rBV	76579	159204	41.88%	4.003%
14	6.986	1838	1849	1872	rBV	33540	64998	17.10%	1.634%
15	7.317	1940	1952	1969	rBV	141969	257903	67.84%	6.485%
16	7.394	1969	1976	1987	rVB4	4981	9648	2.54%	0.243%
17	7.625	2038	2048	2063	rBV	19013	37053	9.75%	0.932%
18	7.973	2148	2156	2172	rVB3	21471	38880	10.23%	0.978%
19	8.092	2179	2193	2226	rBV2	96308	248608	65.39%	6.251%
20	8.850	2418	2429	2454	rBV2	191131	378493	99.56%	9.517%
21	9.146	2516	2521	2530	rVB8	2833	4965	1.31%	0.125%
22	9.317	2566	2574	2583	rVB7	2738	4013	1.06%	0.101%
23	9.477	2608	2624	2640	rBV7	6043	18106	4.76%	0.455%
24	9.674	2672	2685	2687	rBV8	3792	5329	1.40%	0.134%
25	9.702	2687	2694	2707	rVB5	9273	15819	4.16%	0.398%
26	9.799	2715	2724	2734	rBV9	4783	9246	2.43%	0.232%
27	9.934	2756	2766	2772	rBV2	6100	10280	2.70%	0.258%
28	10.127	2815	2826	2835	rBV6	6392	11267	2.96%	0.283%
29	10.217	2842	2854	2873	rVB2	50518	93358	24.56%	2.347%
30	10.355	2887	2897	2901	rBV2	6516	9508	2.50%	0.239%
31	10.452	2919	2927	2937	rBV9	3416	5957	1.57%	0.150%
32	10.738	3003	3016	3029	rVB2	14057	23749	6.25%	0.597%
33	10.918	3064	3072	3080	rBV3	12273	18615	4.90%	0.468%
34	11.088	3119	3125	3138	rVB	11722	17705	4.66%	0.445%
35	11.249	3163	3175	3194	rVV	189849	306722	80.68%	7.712%
36	11.339	3194	3203	3212	rVB4	6263	9368	2.46%	0.236%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023428.D
 Acq On : 12 Nov 2021 08:44
 Operator : SY/MD
 Sample : M4542-06DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG266DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

37	11.452	3231	3238	3247	rVB6	3000	4478	1.18%	0.113%
38	11.529	3251	3262	3276	rBV3	17403	36196	9.52%	0.910%
39	11.625	3279	3292	3309	rBV	154327	280537	73.79%	7.054%
40	12.046	3412	3423	3432	rVB9	6020	9344	2.46%	0.235%
41	12.114	3435	3444	3457	rBV2	13138	22077	5.81%	0.555%
42	12.246	3477	3485	3495	rBV5	2837	4616	1.21%	0.116%
43	12.300	3495	3502	3511	rVV8	4129	5669	1.49%	0.143%
44	12.882	3677	3683	3696	rVB5	2369	3864	1.02%	0.097%
45	13.368	3828	3834	3842	rVB4	3310	4548	1.20%	0.114%
46	14.040	4031	4043	4053	rBV3	3063	5495	1.45%	0.138%




Sum of corrected areas: 3977217

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023428.D
Acq On : 12 Nov 2021 08:44
Operator : SY/MD
Sample : M4542-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG266DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

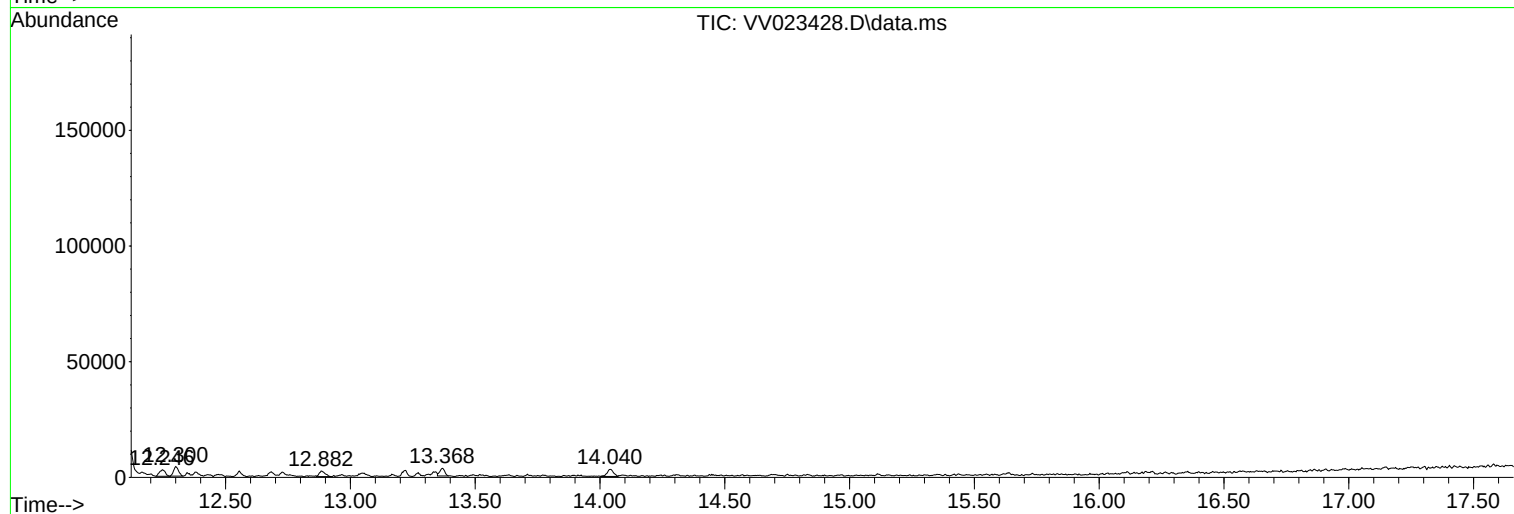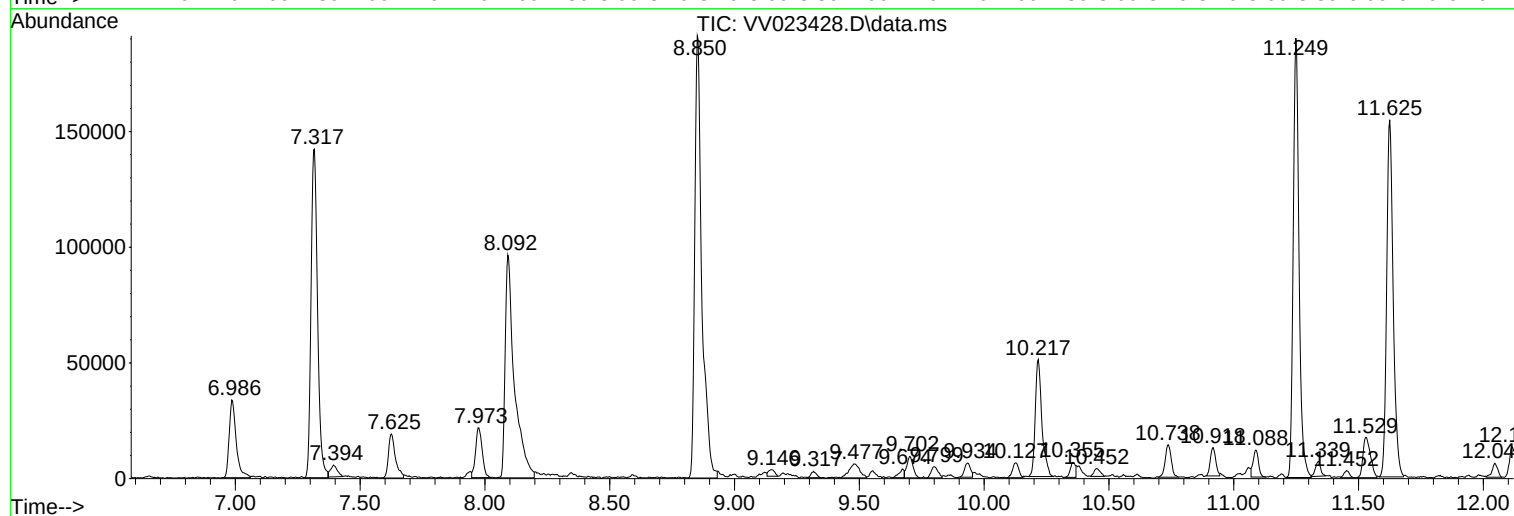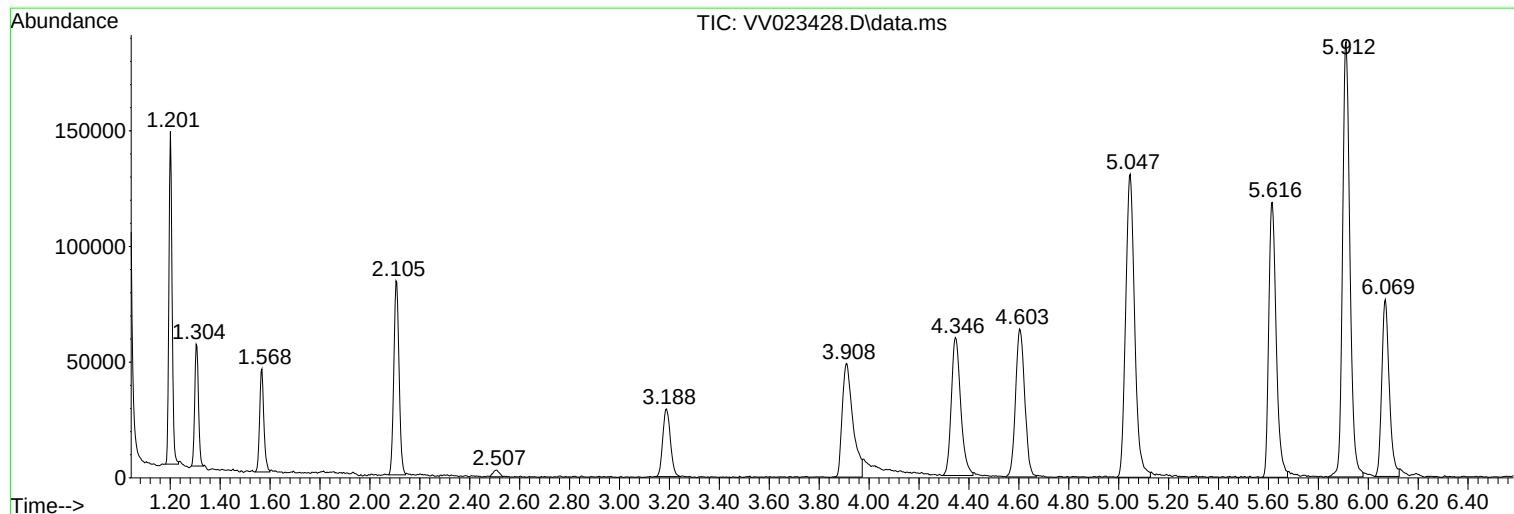

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023428.D
Acq On : 12 Nov 2021 08:44
Operator : SY/MD
Sample : M4542-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG266DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.529	0.59 ug/L	36196	1,4-Dichlorobenzene-d4	11.249

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Indane	118	C9H10	000496-11-7	76
2		Indane	118	C9H10	000496-11-7	70
3		(Z)-1-Phenylpropene	118	C9H10	000766-90-5	70
4		Benzene, cyclopropyl-	118	C9H10	000873-49-4	70
5		Indane	118	C9H10	000496-11-7	64

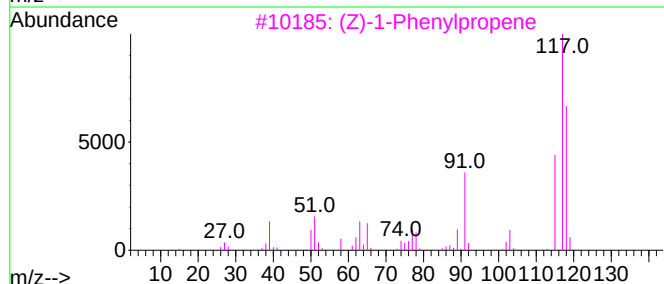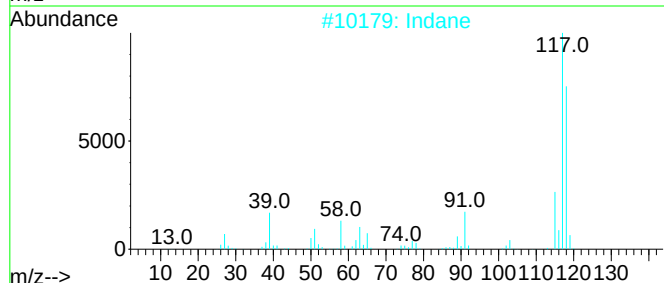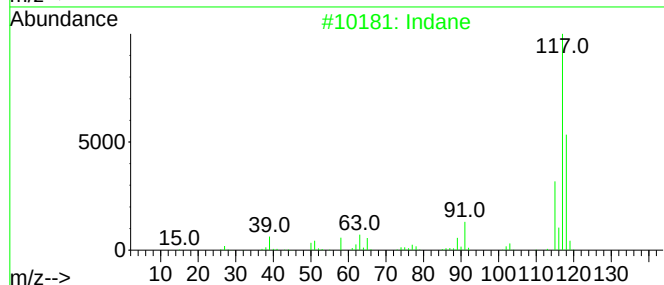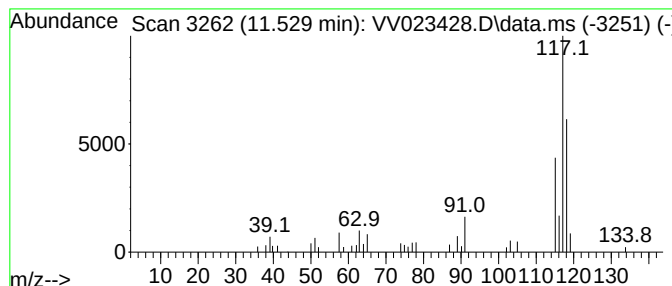

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023428.D
Acq On : 12 Nov 2021 08:44
Operator : SY/MD
Sample : M4542-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG266DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	11.529	0.6	ug/L	36196	3	11.249	306722	5.0