

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023435.D
 Acq On : 12 Nov 2021 11:31
 Operator : SY/MD
 Sample : M4558-26
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	49785	52397	14.41%	1.802%
2	1.568	155	164	178	rBV	47310	53351	14.67%	1.834%
3	2.108	322	332	347	rBV	87338	126135	34.69%	4.337%
4	3.912	882	893	920	rBV	17429	70473	19.38%	2.423%
5	4.352	1012	1030	1055	rBV2	58850	167077	45.95%	5.745%
6	5.050	1230	1247	1271	rBV3	144832	363642	100.00%	12.503%
7	5.619	1409	1424	1446	rBV	126451	260687	71.69%	8.963%
8	5.911	1502	1515	1526	rBV9	3736	8131	2.24%	0.280%
9	6.069	1551	1564	1589	rBV	83184	175282	48.20%	6.027%
10	6.989	1840	1850	1867	rBV2	37475	70563	19.40%	2.426%
11	7.317	1941	1952	1969	rBV	162755	283650	78.00%	9.753%
12	7.625	2039	2048	2066	rBV2	21864	40972	11.27%	1.409%
13	7.982	2150	2159	2170	rVB5	6098	10598	2.91%	0.364%
14	8.095	2183	2194	2224	rBV2	107046	271153	74.57%	9.323%
15	8.853	2419	2430	2450	rBV	204995	333225	91.64%	11.457%
16	10.217	2844	2854	2871	rBV	55854	90223	24.81%	3.102%
17	11.249	3164	3175	3192	rBV	180616	281031	77.28%	9.663%
18	11.625	3279	3292	3306	rBV2	155361	246188	67.70%	8.465%
19	14.046	4036	4045	4052	rVB4	2147	3641	1.00%	0.125%




Sum of corrected areas: 2908419

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023435.D
Acq On : 12 Nov 2021 11:31
Operator : SY/MD
Sample : M4558-26
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

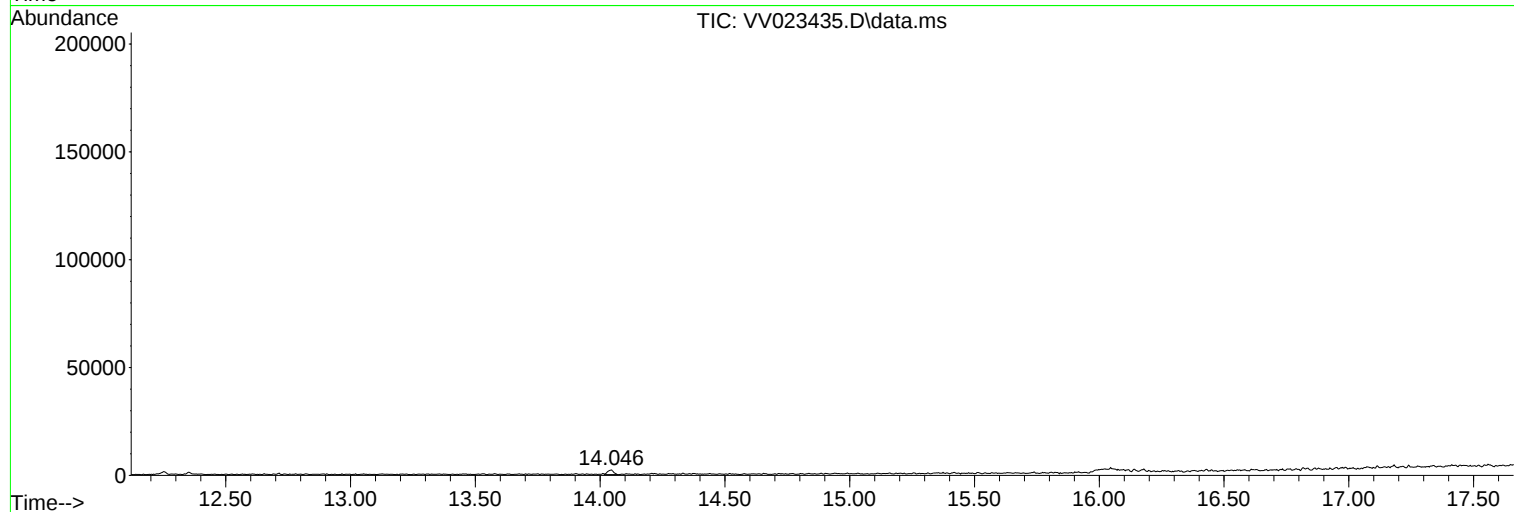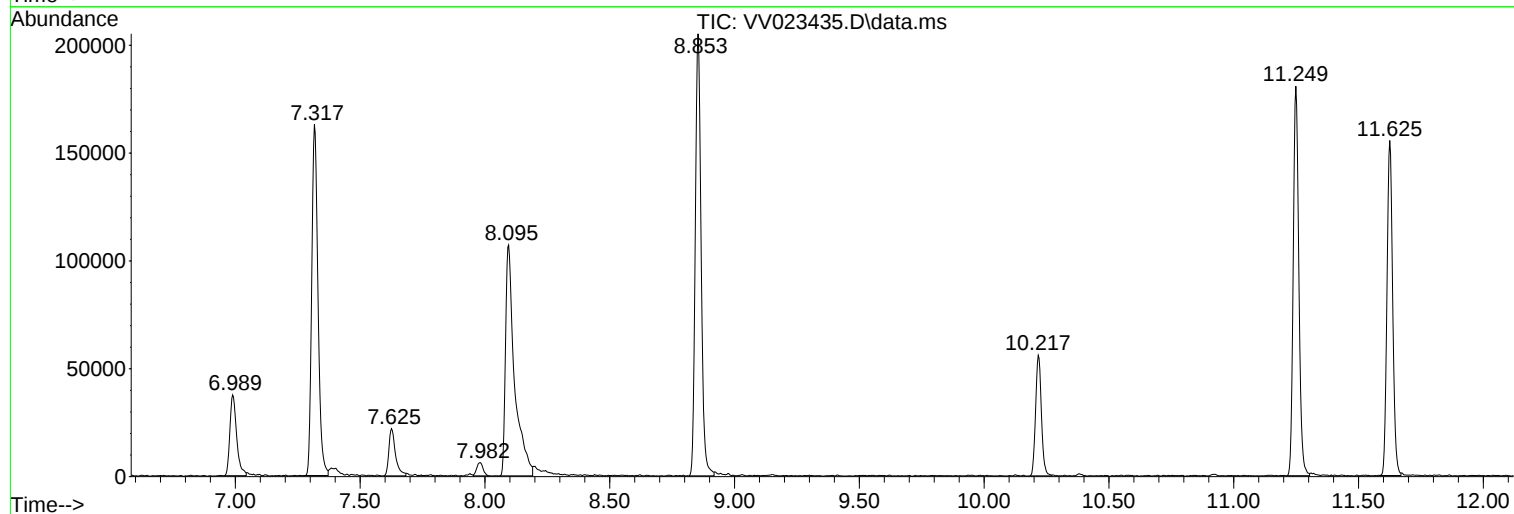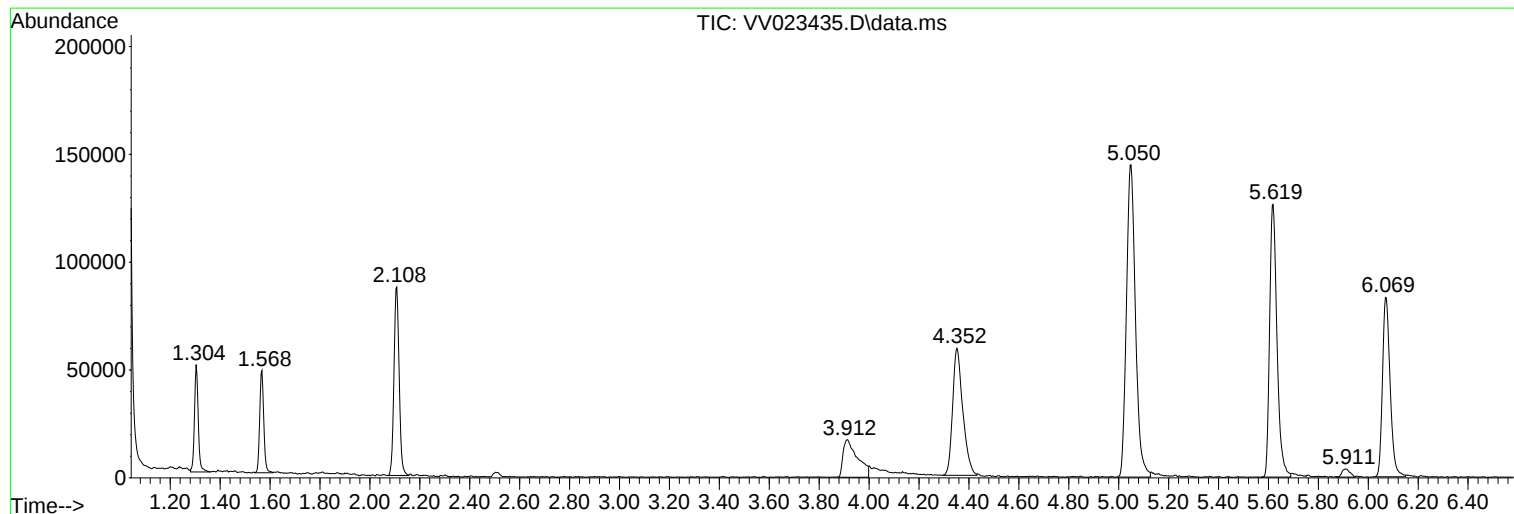

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023435.D
Acq On : 12 Nov 2021 11:31
Operator : SY/MD
Sample : M4558-26
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023435.D
Acq On : 12 Nov 2021 11:31
Operator : SY/MD
Sample : M4558-26
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc