

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023442.D
 Acq On : 12 Nov 2021 14:18
 Operator : SY/MD
 Sample : M4580-19DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8H7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	57	rBV	79232	66489	19.44%	2.108%
2	1.304	75	82	96	rVB	47195	49723	14.54%	1.577%
3	1.568	154	164	173	rBV	42819	49491	14.47%	1.569%
4	2.105	319	331	346	rBV	81154	119173	34.85%	3.779%
5	2.507	447	456	467	rBV3	8095	13889	4.06%	0.440%
6	3.915	883	894	930	rBV2	16823	76740	22.44%	2.433%
7	4.352	1014	1030	1058	rBV4	57624	161140	47.12%	5.110%
8	5.050	1231	1247	1273	rBV2	136723	341997	100.00%	10.845%
9	5.619	1407	1424	1446	rBV	125350	256873	75.11%	8.146%
10	5.915	1504	1516	1532	rVB8	7516	16345	4.78%	0.518%
11	6.072	1552	1565	1593	rBV	80061	170319	49.80%	5.401%
12	6.989	1835	1850	1870	rBV	35529	68357	19.99%	2.168%
13	7.317	1940	1952	1973	rBV	157796	276037	80.71%	8.753%
14	7.625	2039	2048	2065	rBV	20879	38660	11.30%	1.226%
15	7.976	2144	2157	2173	rBV	144675	242409	70.88%	7.687%
16	8.095	2181	2194	2229	rBV2	102876	280301	81.96%	8.889%
17	8.854	2419	2430	2447	rBV	194918	322682	94.35%	10.232%
18	10.217	2842	2854	2871	rBV	53942	88962	26.01%	2.821%
19	11.249	3164	3175	3192	rBV	175475	273575	79.99%	8.675%
20	11.625	3280	3292	3315	rBV	149837	235240	68.78%	7.460%
21	14.040	4036	4043	4051	rBV	3566	5118	1.50%	0.162%




Sum of corrected areas: 3153520

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023442.D
Acq On : 12 Nov 2021 14:18
Operator : SY/MD
Sample : M4580-19DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

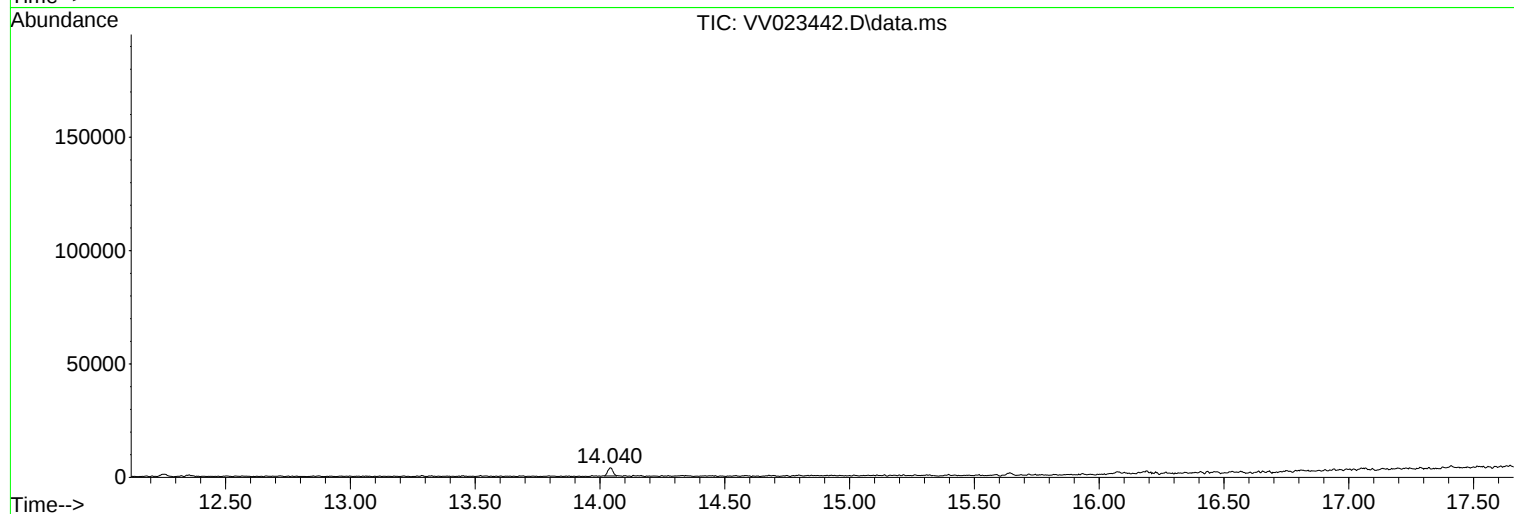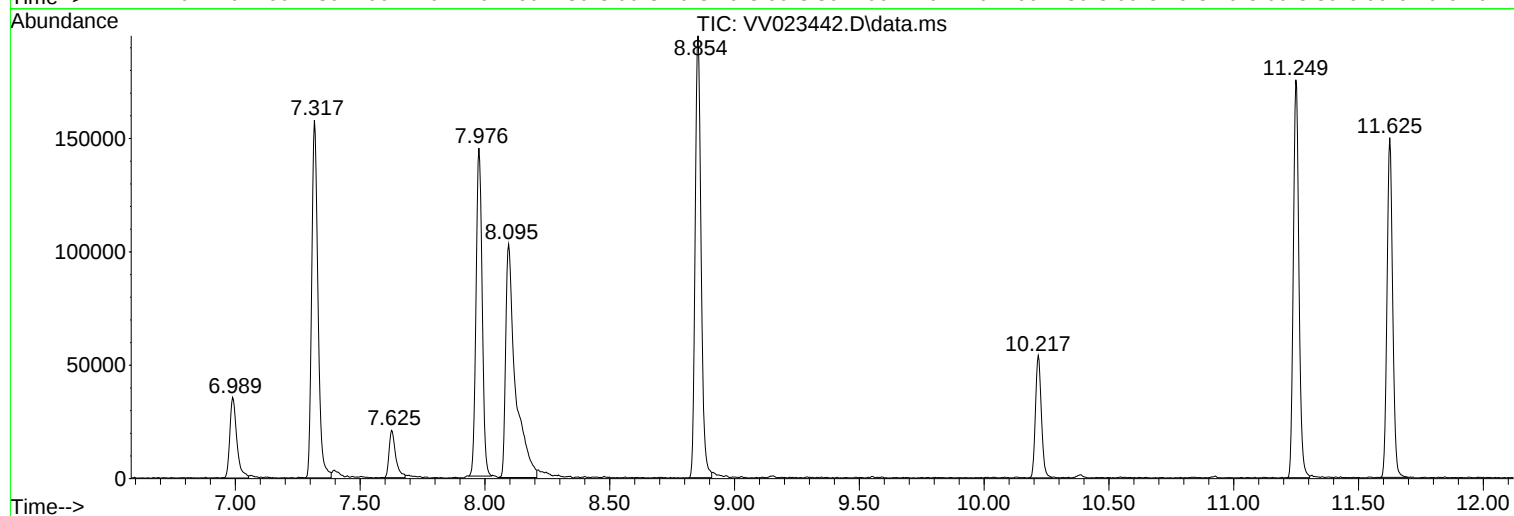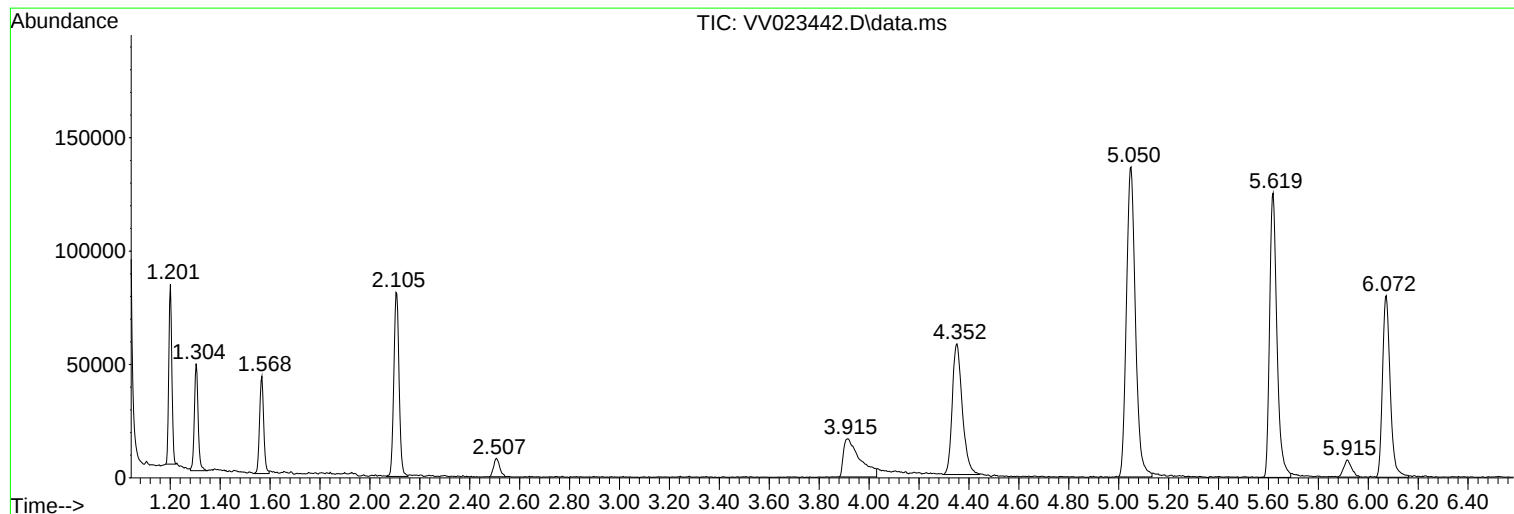

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023442.D
Acq On : 12 Nov 2021 14:18
Operator : SY/MD
Sample : M4580-19DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H7DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	1.29 ug/L	66489	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-([2-(Butane-1-sulfonyl)ethyl]s...	226	C8H18O3S2	1000388-83-2	9		
2	1,4,7-Oxadithionane	164	C6H12O2S2	040474-73-5	9		
3	Methyl nitrite	61	CH3NO2	000624-91-9	5		
4	Ethyne, chloro-	60	C2HCl	000593-63-5	5		
5	o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4		

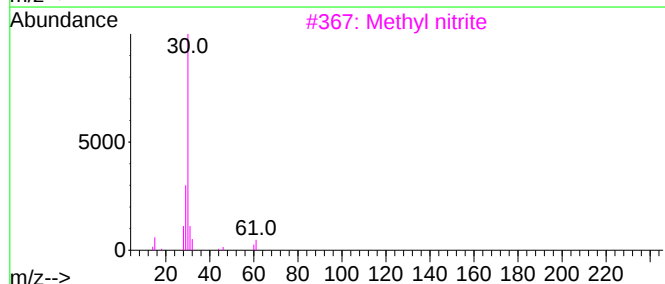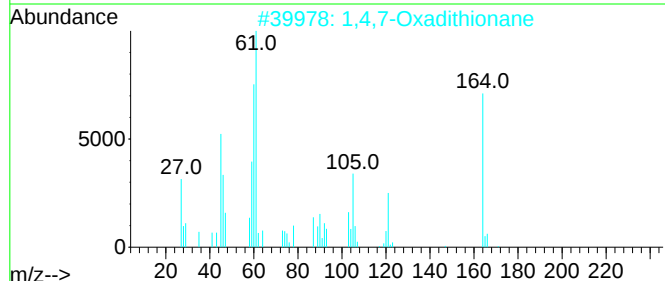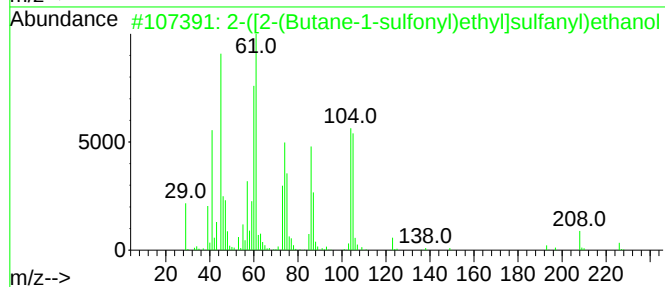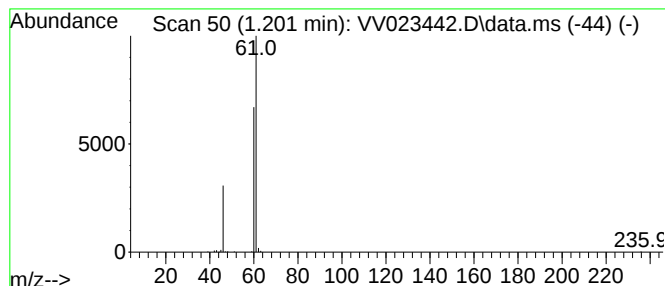

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023442.D
Acq On : 12 Nov 2021 14:18
Operator : SY/MD
Sample : M4580-19DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	1.3	ug/L	66489	1	5.619	256873	5.0