

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023447.D
 Acq On : 12 Nov 2021 17:36
 Operator : SY/MD
 Sample : M4580-20DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8H8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	73	81	96	rVB	48493	53758	9.79%	1.423%
2	1.568	157	164	172	rBV	47600	54414	9.91%	1.440%
3	2.105	318	331	344	rBV	91491	129235	23.54%	3.421%
4	2.500	447	454	465	rBV9	4636	7732	1.41%	0.205%
5	3.973	893	912	932	rBV	27118	111379	20.29%	2.948%
6	4.346	1013	1028	1052	rVB	72153	187250	34.11%	4.956%
7	5.043	1228	1245	1270	rBV4	188725	415092	75.62%	10.987%
8	5.622	1407	1425	1443	rBV	136994	272893	49.72%	7.223%
9	5.912	1501	1515	1530	rVB	9040	20818	3.79%	0.551%
10	6.079	1554	1567	1587	rBV2	97069	197087	35.91%	5.217%
11	6.998	1842	1853	1874	rBV2	42375	80106	14.59%	2.120%
12	7.323	1942	1954	1971	rBV	176600	309722	56.43%	8.198%
13	7.404	1973	1979	1990	rVB6	3253	5919	1.08%	0.157%
14	7.632	2041	2050	2066	rBV	26209	46285	8.43%	1.225%
15	7.979	2145	2158	2179	rBV	326871	548893	100.00%	14.529%
16	8.108	2188	2198	2231	rBV2	162803	350617	63.88%	9.281%
17	8.857	2419	2431	2450	rBV	209635	337787	61.54%	8.941%
18	10.220	2844	2855	2871	rBV	65203	100731	18.35%	2.666%
19	11.249	3161	3175	3195	rBV	180557	281274	51.24%	7.445%
20	11.625	3280	3292	3310	rBV	169358	266940	48.63%	7.066%




Sum of corrected areas: 3777932

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023447.D
Acq On : 12 Nov 2021 17:36
Operator : SY/MD
Sample : M4580-20DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

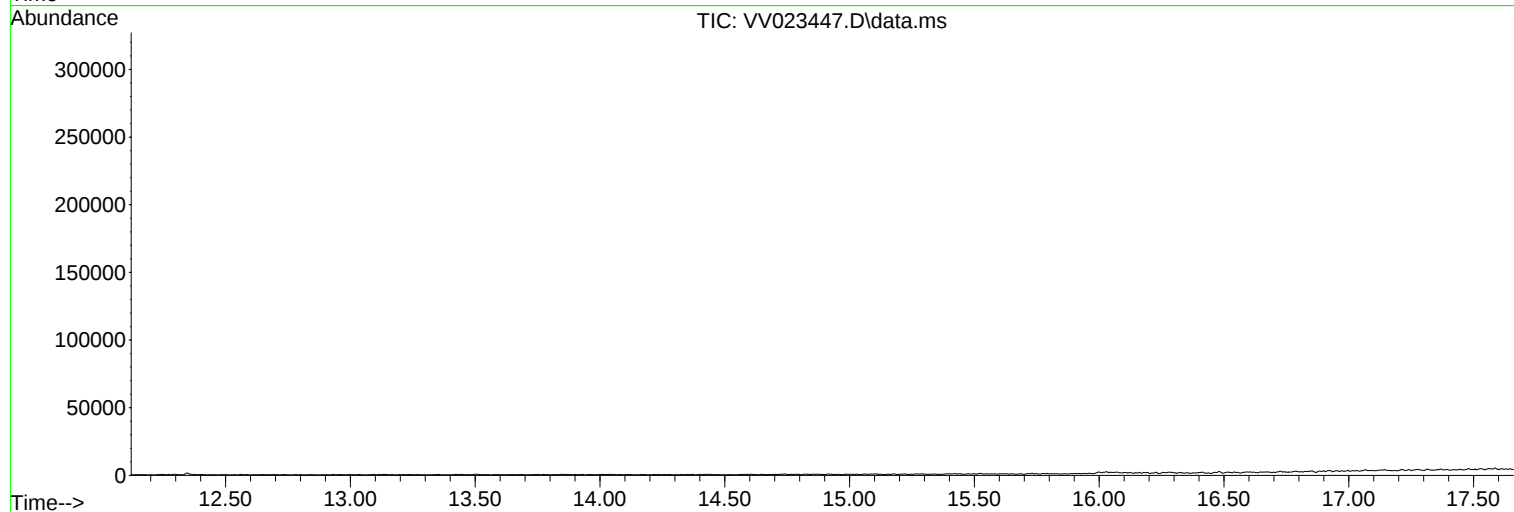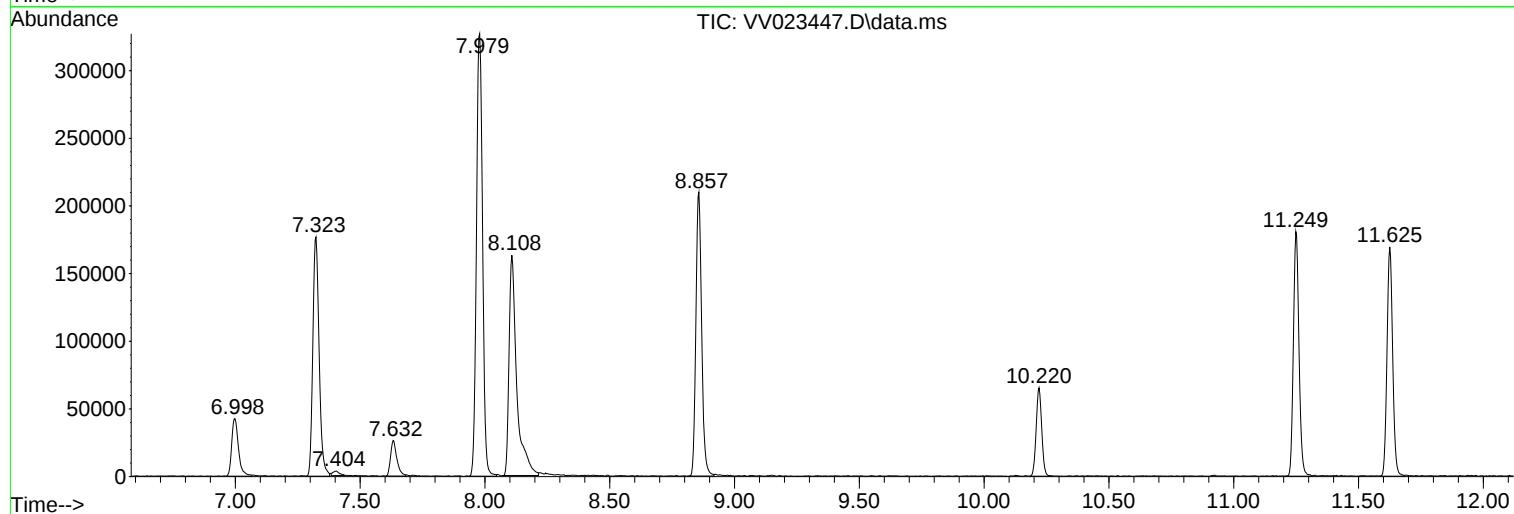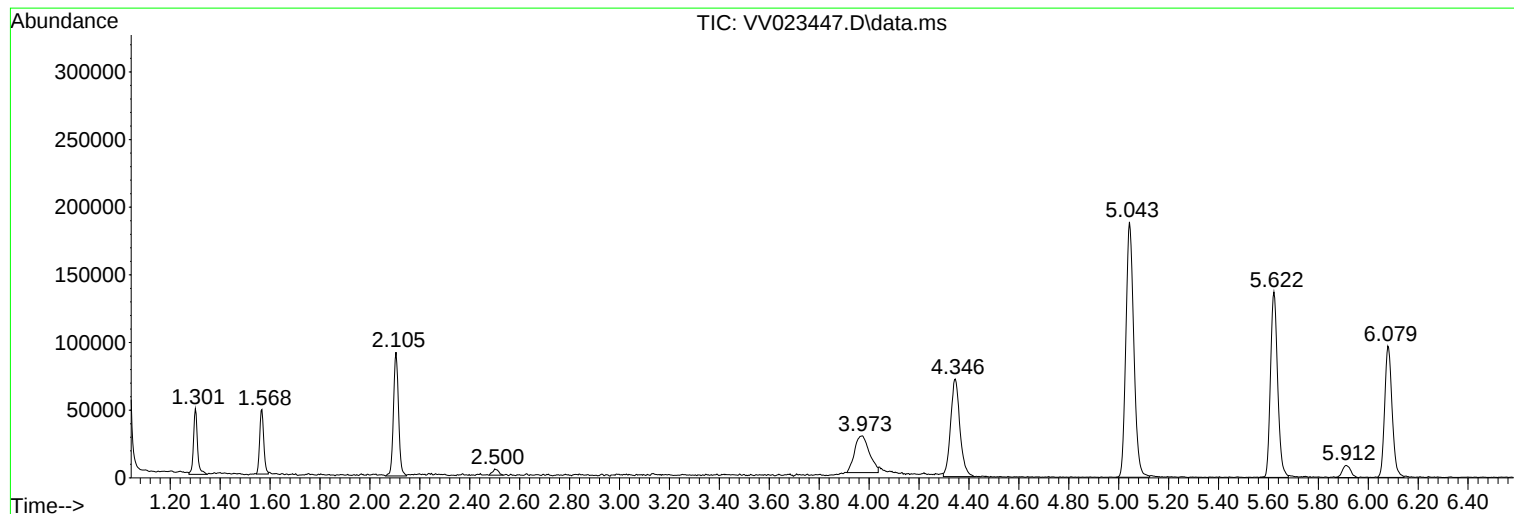

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023447.D
Acq On : 12 Nov 2021 17:36
Operator : SY/MD
Sample : M4580-20DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023447.D
Acq On : 12 Nov 2021 17:36
Operator : SY/MD
Sample : M4580-20DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc