

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023448.D
 Acq On : 12 Nov 2021 18:00
 Operator : SY/MD
 Sample : M4580-16DL 400X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8H4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	73	79	92	rVB	47690	48688	10.93%	1.379%
2	1.558	153	161	174	rVB	47137	53751	12.07%	1.523%
3	2.098	319	329	343	rBV	90018	128708	28.91%	3.646%
4	2.500	447	454	464	rVB5	5486	8940	2.01%	0.253%
5	3.966	887	910	913	rBV2	24305	59985	13.47%	1.699%
6	4.342	1010	1027	1057	rVB3	71620	181145	40.68%	5.131%
7	5.034	1225	1242	1264	rVB2	205286	445266	100.00%	12.613%
8	5.613	1408	1422	1447	rBV	140368	276278	62.05%	7.826%
9	5.895	1499	1510	1524	rVB8	5545	11427	2.57%	0.324%
10	6.069	1550	1564	1585	rBV	97549	197364	44.32%	5.591%
11	6.985	1836	1849	1871	rBV2	42497	78085	17.54%	2.212%
12	7.313	1939	1951	1971	rBV	177917	310236	69.67%	8.788%
13	7.625	2037	2048	2064	rBV	27088	47449	10.66%	1.344%
14	7.969	2144	2155	2173	rBV	224513	375330	84.29%	10.632%
15	8.108	2187	2198	2234	rBV2	153552	337416	75.78%	9.558%
16	8.850	2417	2429	2451	rBV	202974	332717	74.72%	9.425%
17	10.217	2844	2854	2866	rBV	64043	99823	22.42%	2.828%
18	11.249	3164	3175	3191	rBV	177365	273023	61.32%	7.734%
19	11.625	3280	3292	3311	rBV	168146	264581	59.42%	7.495%




Sum of corrected areas: 3530212

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023448.D
Acq On : 12 Nov 2021 18:00
Operator : SY/MD
Sample : M4580-16DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

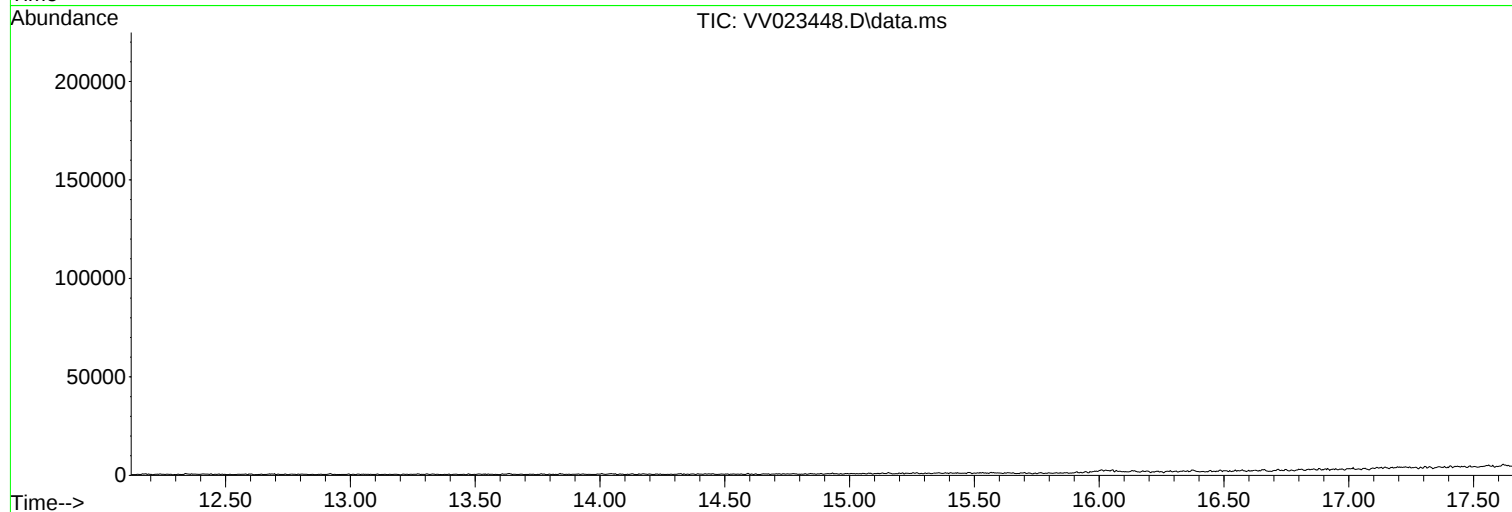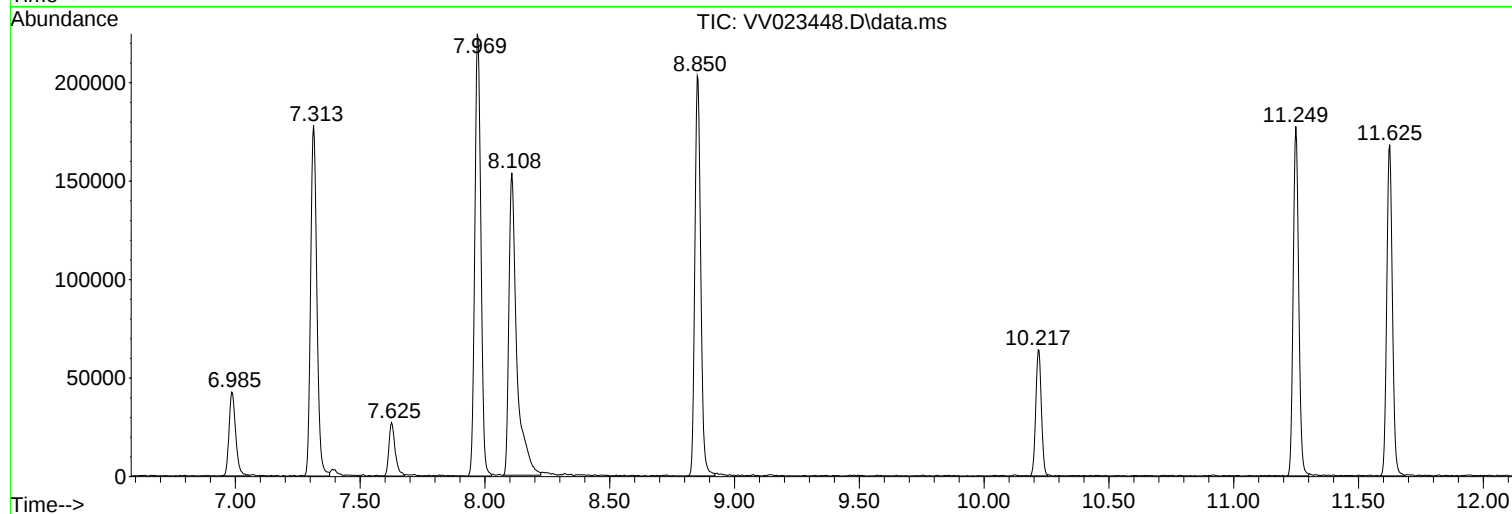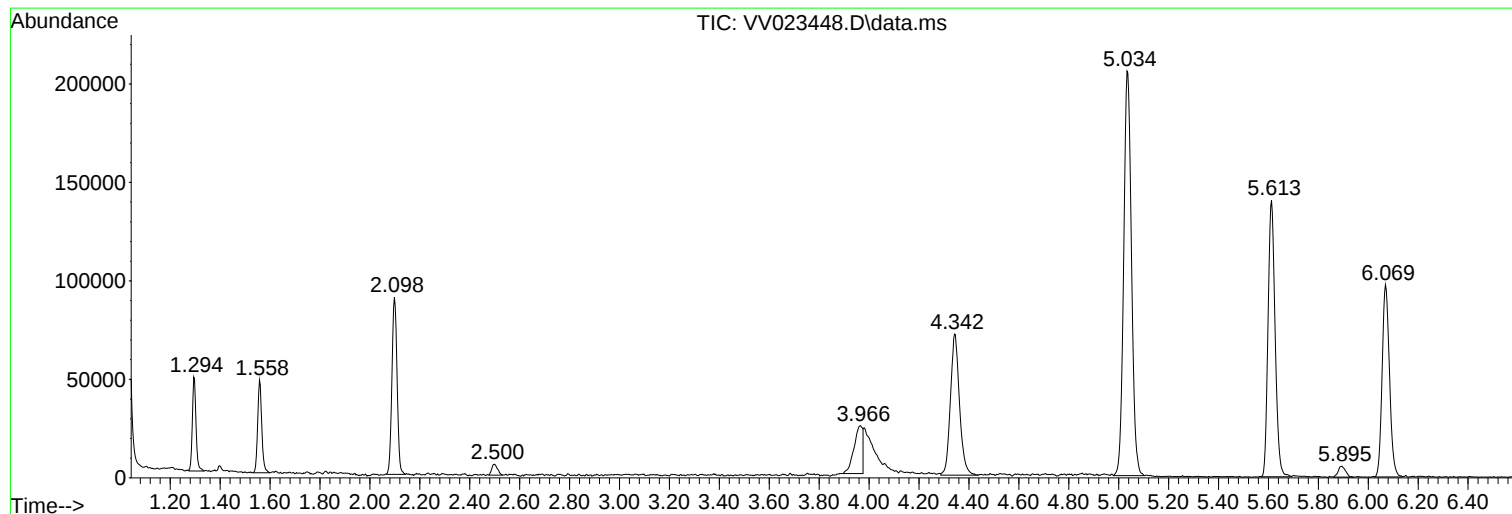

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023448.D
Acq On : 12 Nov 2021 18:00
Operator : SY/MD
Sample : M4580-16DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023448.D
Acq On : 12 Nov 2021 18:00
Operator : SY/MD
Sample : M4580-16DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc