

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023449.D
 Acq On : 12 Nov 2021 18:24
 Operator : SY/MD
 Sample : M4580-17DL 400X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8H5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	94	rVB	52998	55144	13.12%	1.530%
2	1.577	159	167	179	rBV	47154	55202	13.14%	1.532%
3	2.121	323	336	350	rBV	96206	133437	31.76%	3.702%
4	2.516	450	459	472	rVB	3950	8451	2.01%	0.234%
5	3.976	890	913	936	rBV2	29321	118143	28.12%	3.278%
6	4.362	1016	1033	1055	rBV	74045	199390	47.45%	5.532%
7	5.069	1236	1253	1279	rBV3	176130	420178	100.00%	11.659%
8	5.651	1420	1434	1458	rBV	134387	268204	63.83%	7.442%
9	5.934	1512	1522	1537	rVB6	5580	11208	2.67%	0.311%
10	6.101	1558	1574	1595	rBV	99615	203836	48.51%	5.656%
11	7.008	1844	1856	1874	rBV3	42720	81161	19.32%	2.252%
12	7.333	1945	1957	1976	rBV	188806	326477	77.70%	9.059%
13	7.413	1978	1982	1997	rVB7	2691	4806	1.14%	0.133%
14	7.641	2042	2053	2067	rBV2	25285	46200	11.00%	1.282%
15	7.985	2148	2160	2180	rBV	207757	345174	82.15%	9.577%
16	8.108	2188	2198	2234	rBV2	159373	344990	82.11%	9.572%
17	8.860	2419	2432	2457	rBV	203991	334489	79.61%	9.281%
18	10.220	2841	2855	2870	rBV	63628	102428	24.38%	2.842%
19	11.252	3164	3176	3194	rBV	171977	270775	64.44%	7.513%
20	11.625	3280	3292	3311	rBV	169038	269641	64.17%	7.482%
21	16.004	4641	4654	4659	rBV	2158	4683	1.11%	0.130%




Sum of corrected areas: 3604017

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023449.D
Acq On : 12 Nov 2021 18:24
Operator : SY/MD
Sample : M4580-17DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

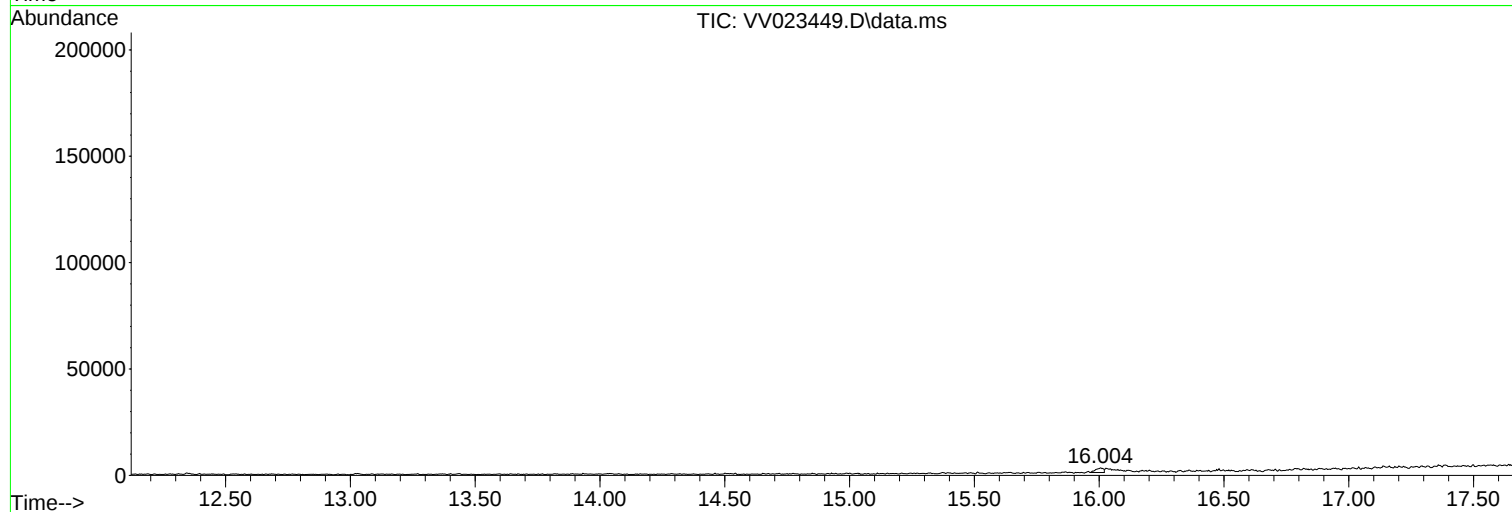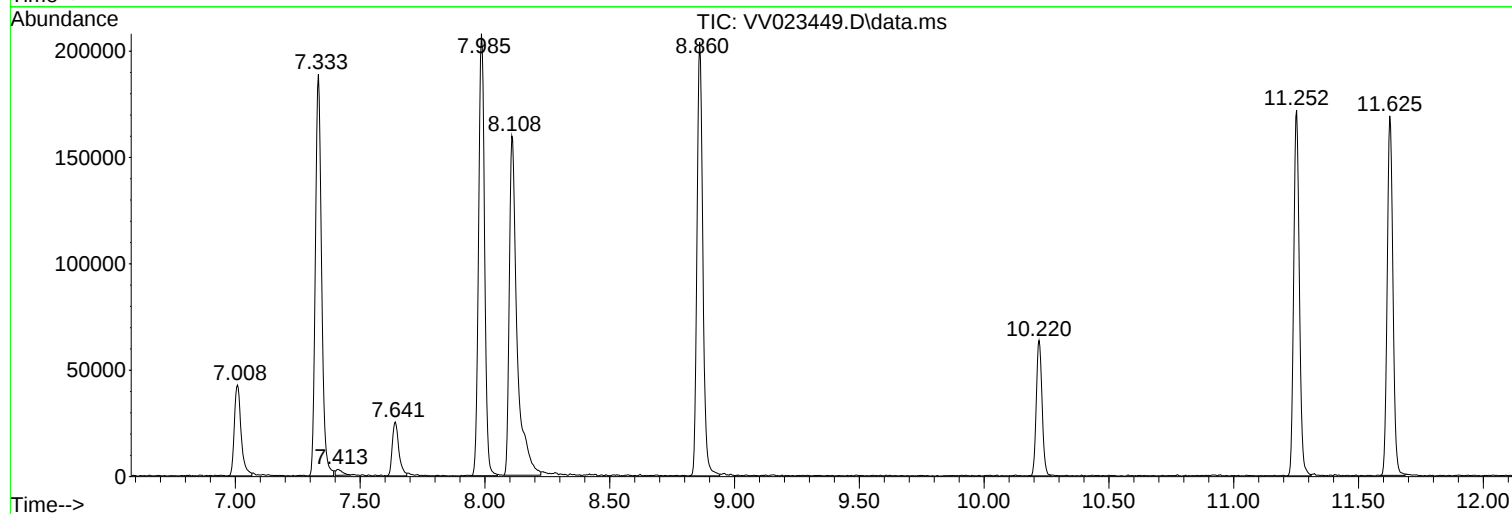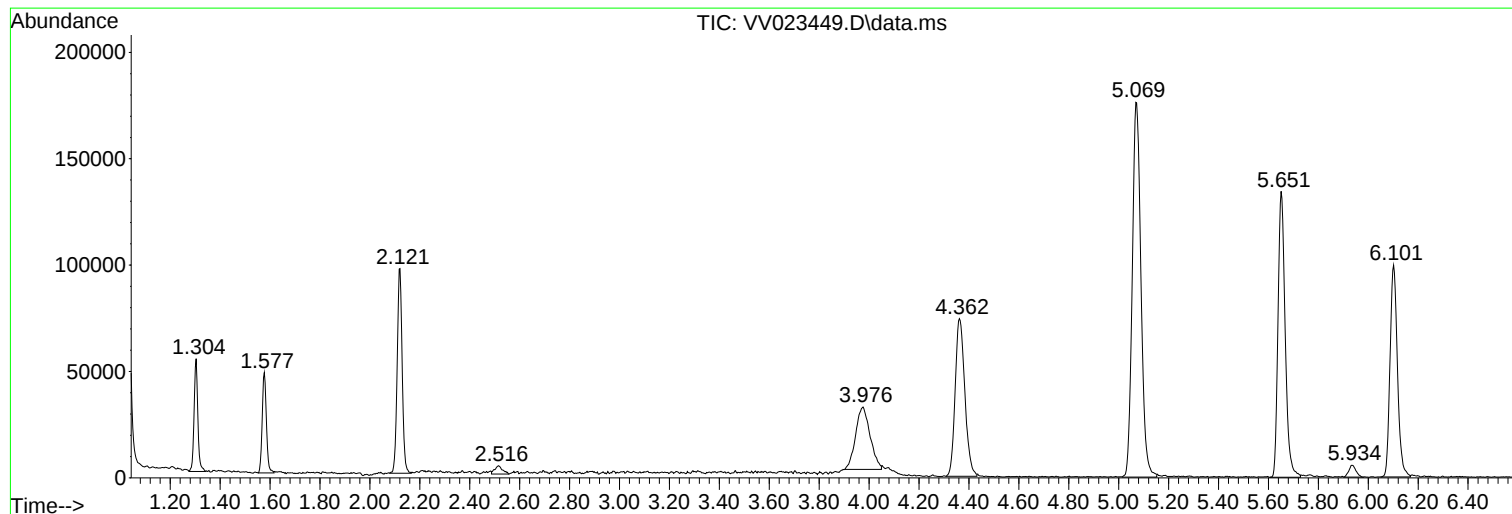

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023449.D
Acq On : 12 Nov 2021 18:24
Operator : SY/MD
Sample : M4580-17DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023449.D
Acq On : 12 Nov 2021 18:24
Operator : SY/MD
Sample : M4580-17DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
