

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023450.D
 Acq On : 12 Nov 2021 18:48
 Operator : SY/MD
 Sample : M4580-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	52246	53558	13.07%	1.658%
2	1.565	155	163	175	rVB	49019	55701	13.60%	1.724%
3	2.105	319	331	346	rBV	92831	135004	32.96%	4.179%
4	2.507	445	456	468	rVB3	4905	7797	1.90%	0.241%
5	3.902	878	890	928	rBV2	21626	97406	23.78%	3.015%
6	4.349	1013	1029	1053	rBV2	71554	189938	46.37%	5.880%
7	5.047	1229	1246	1272	rBV2	164644	409655	100.00%	12.681%
8	5.616	1408	1423	1446	rBV	127571	266013	64.94%	8.235%
9	5.905	1504	1513	1529	rVB5	4935	10173	2.48%	0.315%
10	6.069	1552	1564	1588	rBV	93959	198909	48.56%	6.157%
11	6.989	1840	1850	1870	rBV	42136	80068	19.55%	2.479%
12	7.317	1941	1952	1972	rBV	183776	324784	79.28%	10.054%
13	7.394	1973	1976	1988	rVB4	2905	4720	1.15%	0.146%
14	7.625	2039	2048	2067	rBV	25519	46504	11.35%	1.440%
15	8.095	2183	2194	2232	rBV2	130025	344441	84.08%	10.663%
16	8.854	2417	2430	2449	rBV	205099	340302	83.07%	10.534%
17	10.217	2839	2854	2867	rBV	65567	102870	25.11%	3.184%
18	11.249	3164	3175	3195	rBV	181658	281696	68.76%	8.720%
19	11.625	3279	3292	3309	rBV	176373	280823	68.55%	8.693%




Sum of corrected areas: 3230362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023450.D
Acq On : 12 Nov 2021 18:48
Operator : SY/MD
Sample : M4580-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

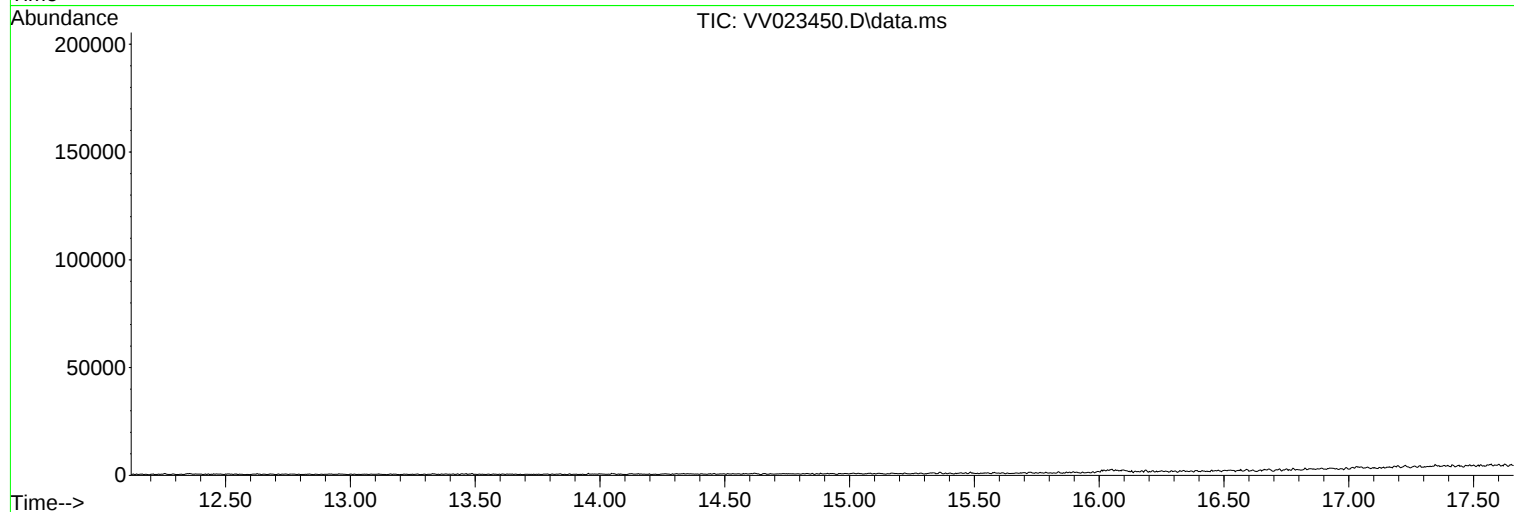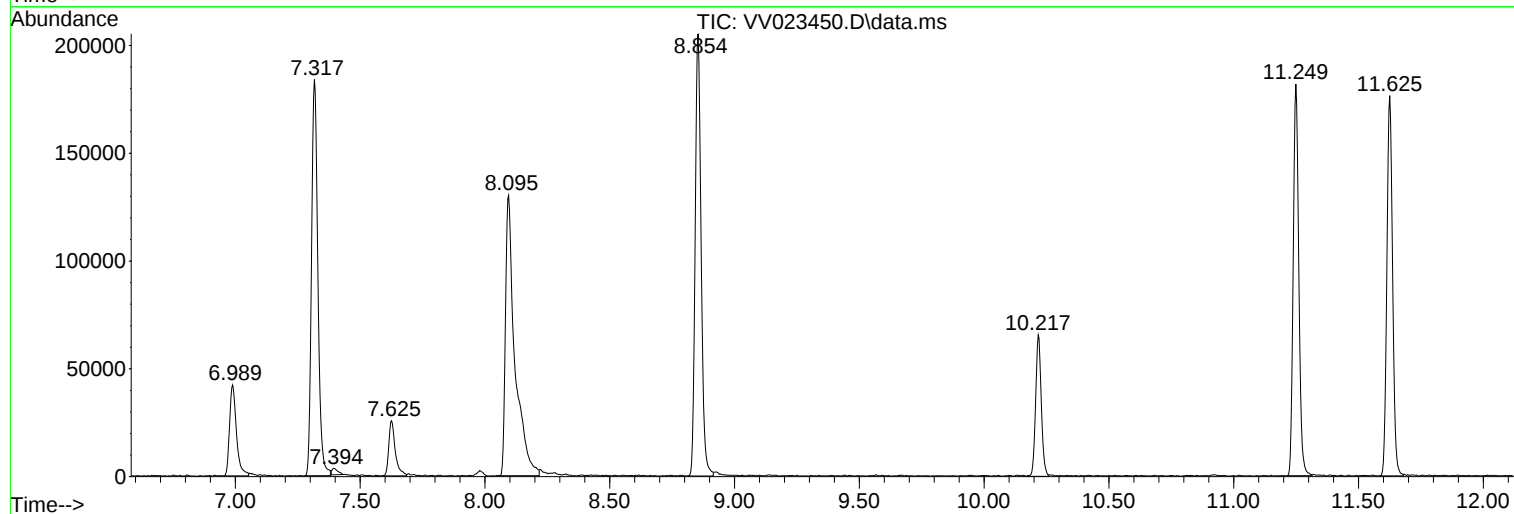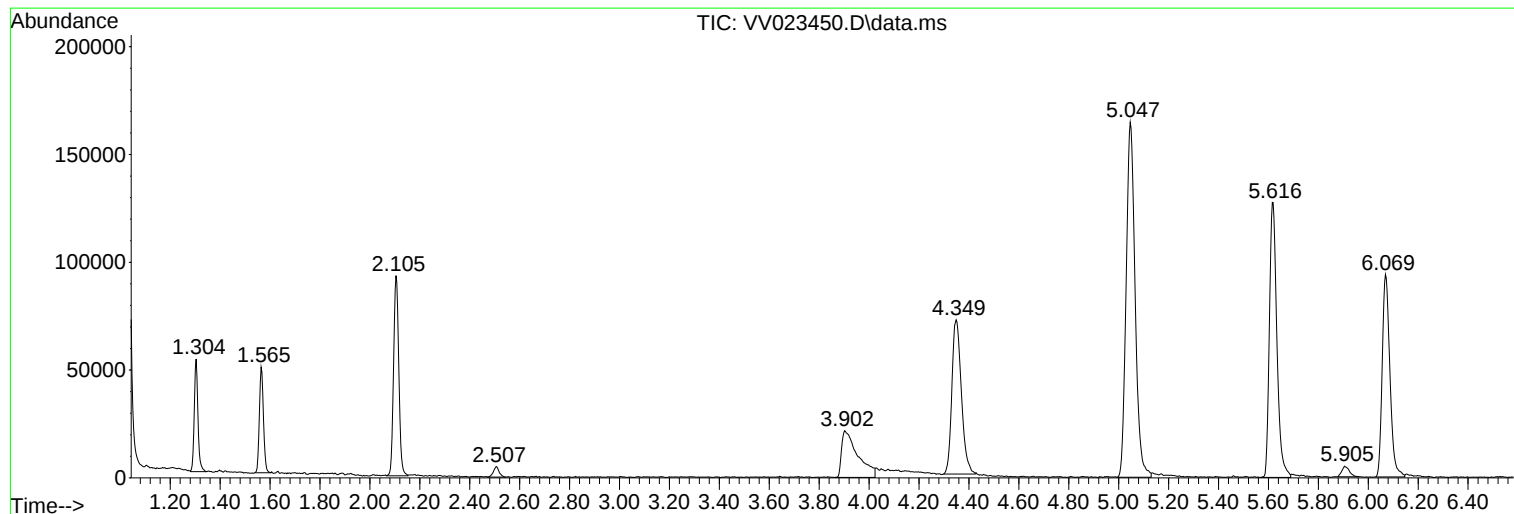

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023450.D
Acq On : 12 Nov 2021 18:48
Operator : SY/MD
Sample : M4580-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023450.D
Acq On : 12 Nov 2021 18:48
Operator : SY/MD
Sample : M4580-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc