

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023452.D
 Acq On : 12 Nov 2021 19:36
 Operator : SY/MD
 Sample : M4581-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8J5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.204	46	51	58	rVB3	3296	4047	1.01%	0.131%
2	1.304	74	82	92	rVB	50127	50906	12.71%	1.651%
3	1.565	156	163	176	rBV	48467	55891	13.95%	1.813%
4	2.105	313	331	349	rBV	92378	134595	33.60%	4.366%
5	3.905	880	891	892	rBV2	21578	28608	7.14%	0.928%
6	4.349	1014	1029	1055	rVB	71704	184853	46.14%	5.997%
7	5.047	1229	1246	1271	rBV3	161685	400635	100.00%	12.996%
8	5.616	1412	1423	1452	rBV	122587	255537	63.78%	8.290%
9	5.908	1502	1514	1531	rBV6	3297	7794	1.95%	0.253%
10	6.072	1552	1565	1581	rBV	91552	190765	47.62%	6.188%
11	6.989	1837	1850	1867	rBV	41746	78676	19.64%	2.552%
12	7.317	1941	1952	1969	rBV	177626	314154	78.41%	10.191%
13	7.397	1972	1977	1994	rVB3	5194	9709	2.42%	0.315%
14	7.625	2036	2048	2060	rBV	24969	43072	10.75%	1.397%
15	7.979	2149	2158	2171	rVB3	10796	19745	4.93%	0.641%
16	8.095	2183	2194	2237	rBV2	126207	342002	85.36%	11.094%
17	8.854	2416	2430	2448	rBV	197598	324981	81.12%	10.542%
18	10.217	2843	2854	2869	rBV	63266	103112	25.74%	3.345%
19	11.249	3165	3175	3194	rBV	168113	264296	65.97%	8.574%
20	11.625	3279	3292	3315	rBV	173218	269274	67.21%	8.735%




Sum of corrected areas: 3082652

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023452.D
Acq On : 12 Nov 2021 19:36
Operator : SY/MD
Sample : M4581-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

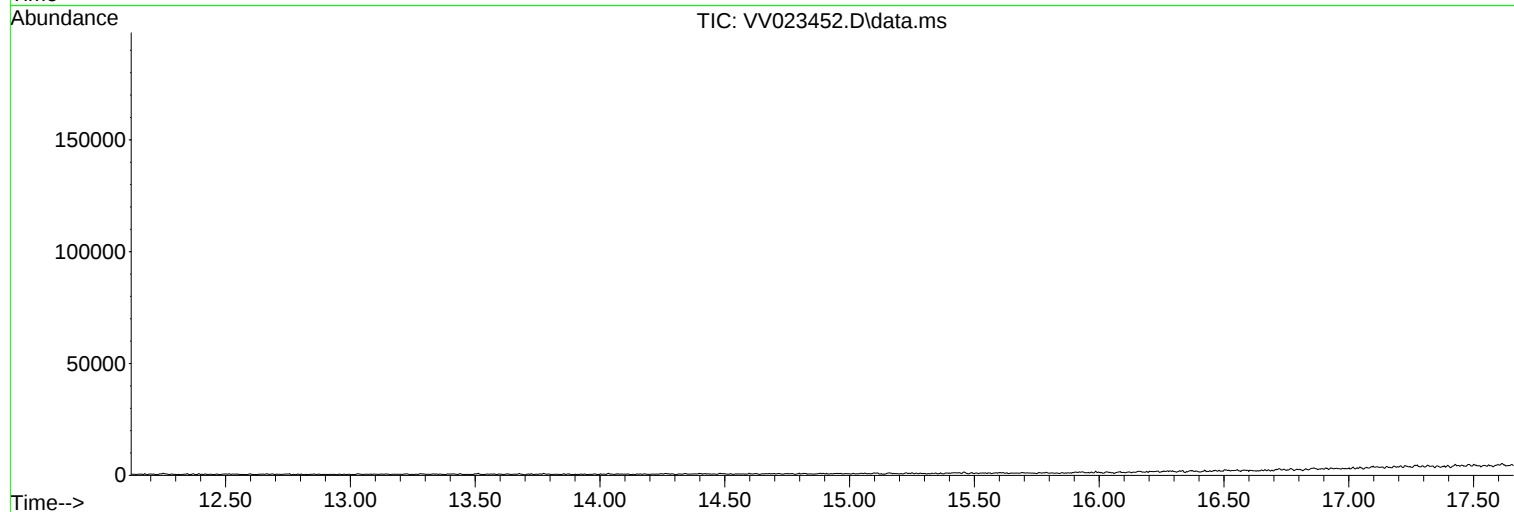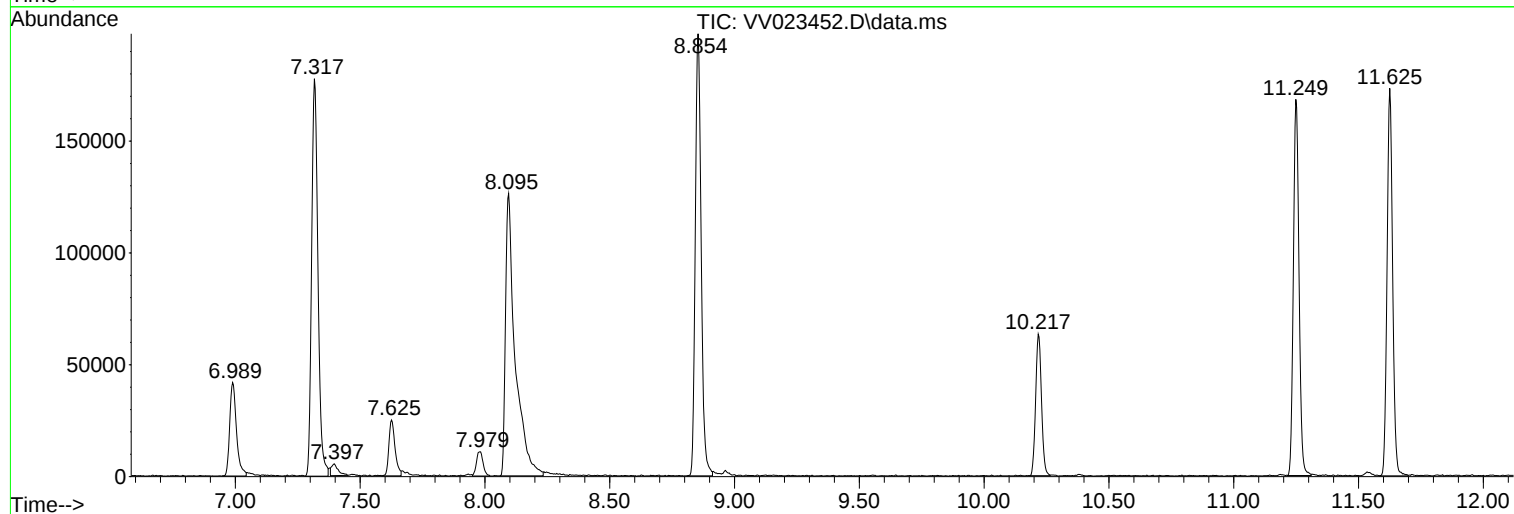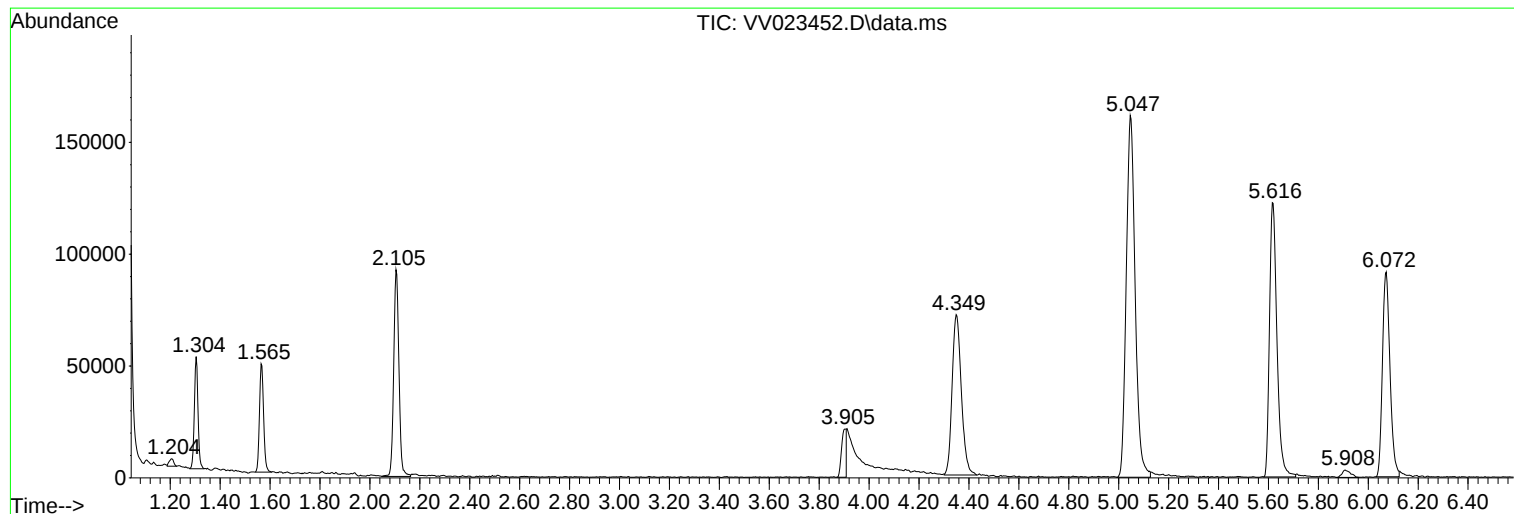

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023452.D
Acq On : 12 Nov 2021 19:36
Operator : SY/MD
Sample : M4581-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023452.D
Acq On : 12 Nov 2021 19:36
Operator : SY/MD
Sample : M4581-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
