

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023454.D
 Acq On : 12 Nov 2021 20:24
 Operator : SY/MD
 Sample : M4581-02DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8J1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	48505	48311	12.61%	1.456%
2	1.565	156	163	174	rBV	45849	51359	13.41%	1.548%
3	2.105	321	331	344	rBV	87536	124041	32.38%	3.739%
4	2.507	447	456	467	rBV4	4090	6596	1.72%	0.199%
5	3.909	883	892	908	rBV2	18466	61650	16.09%	1.858%
6	4.349	1013	1029	1058	rBV	67690	179581	46.88%	5.414%
7	5.047	1230	1246	1270	rBV2	155773	383067	100.00%	11.548%
8	5.619	1411	1424	1452	rBV2	126752	262324	68.48%	7.908%
9	5.918	1502	1517	1527	rBV7	4827	9954	2.60%	0.300%
10	6.072	1549	1565	1581	rBV	87919	186205	48.61%	5.613%
11	6.989	1840	1850	1872	rBV	38816	76012	19.84%	2.291%
12	7.317	1941	1952	1972	rBV	174376	306120	79.91%	9.228%
13	7.625	2039	2048	2075	rVB	23679	43360	11.32%	1.307%
14	7.976	2143	2157	2179	rBV	166740	284220	74.20%	8.568%
15	8.095	2183	2194	2227	rBV2	120301	319024	83.28%	9.617%
16	8.854	2418	2430	2453	rBV	205126	336311	87.79%	10.138%
17	10.217	2843	2854	2873	rBV	60377	95599	24.96%	2.882%
18	11.249	3165	3175	3194	rBV	177937	278511	72.71%	8.396%
19	11.625	3281	3292	3311	rBV	166998	264956	69.17%	7.987%




Sum of corrected areas: 3317201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023454.D
Acq On : 12 Nov 2021 20:24
Operator : SY/MD
Sample : M4581-02DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

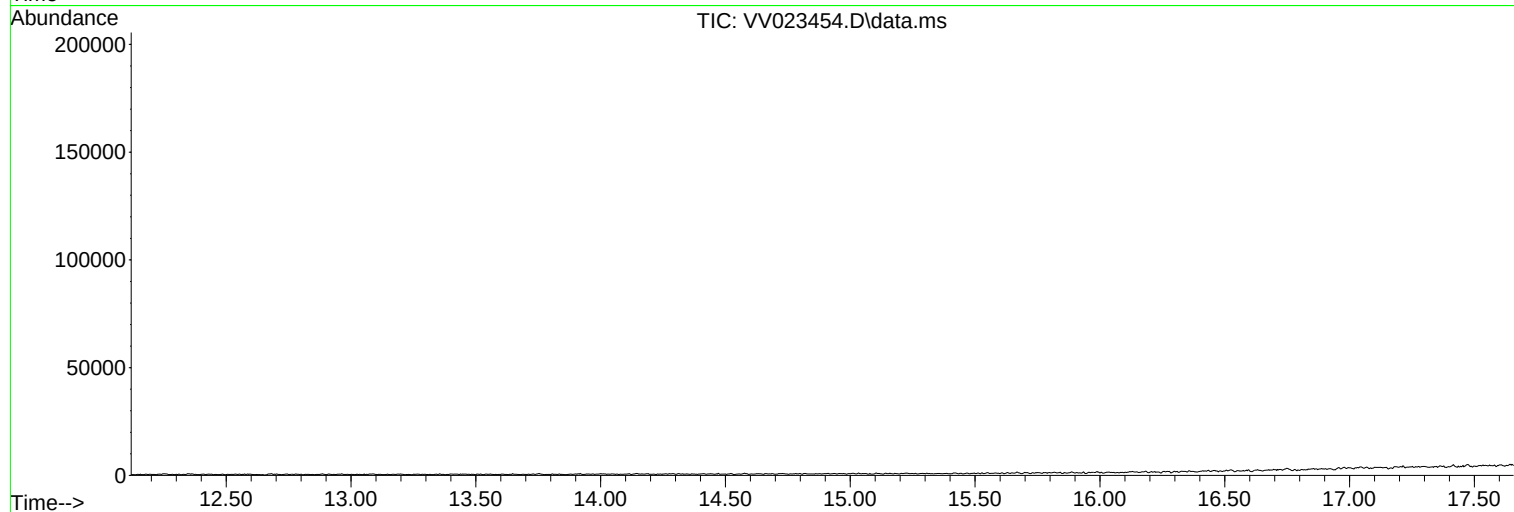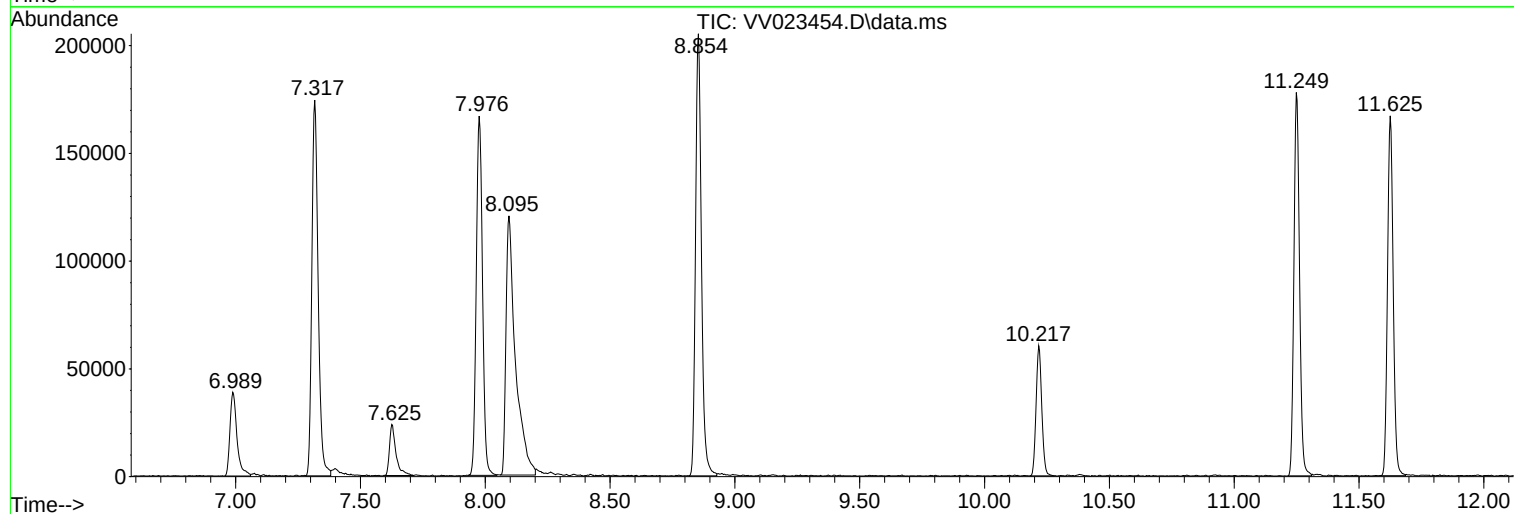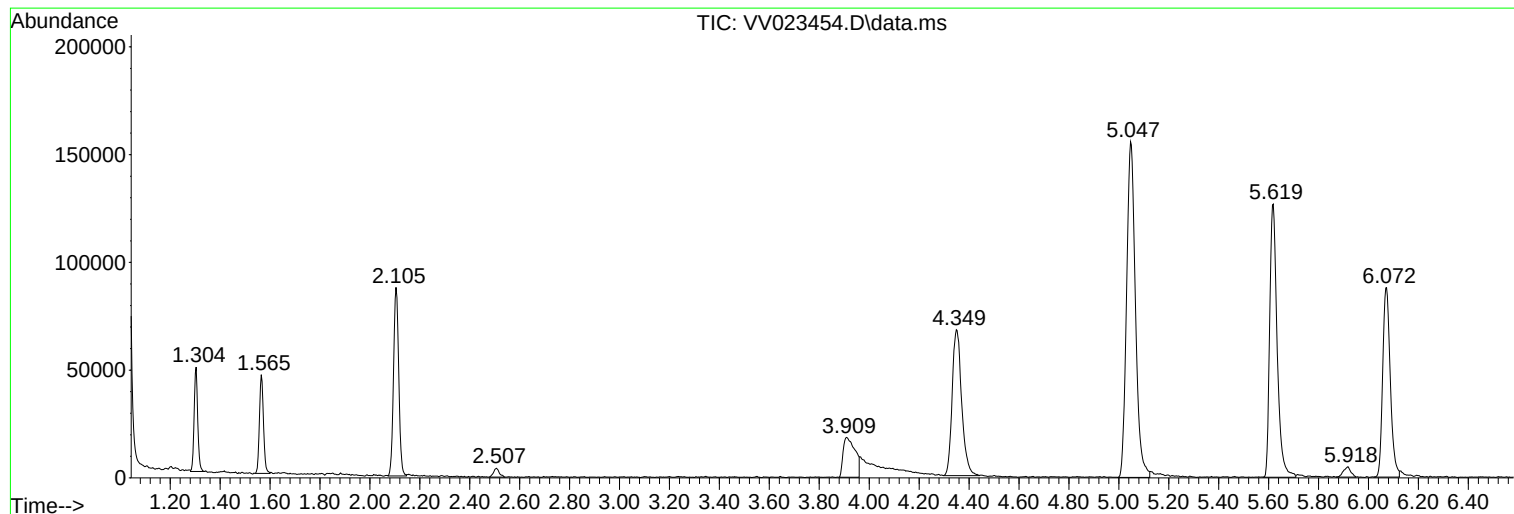

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023454.D
Acq On : 12 Nov 2021 20:24
Operator : SY/MD
Sample : M4581-02DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023454.D
Acq On : 12 Nov 2021 20:24
Operator : SY/MD
Sample : M4581-02DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc