

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023457.D
 Acq On : 12 Nov 2021 21:37
 Operator : SY/MD
 Sample : M4616-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXR2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	59	rVB	7317	5734	1.33%	0.139%
2	1.304	75	82	93	rBV	77618	80723	18.74%	1.960%
3	1.568	156	164	176	rBV	61676	71259	16.54%	1.730%
4	2.108	317	332	346	rBV	121335	177835	41.29%	4.318%
5	3.902	877	890	928	rBV2	33488	131429	30.51%	3.191%
6	4.352	1012	1030	1056	rBV	76193	198784	46.15%	4.826%
7	5.050	1229	1247	1277	rBV3	171026	430737	100.00%	10.458%
8	5.619	1411	1424	1447	rBV	130257	265528	61.65%	6.447%
9	5.915	1503	1516	1537	rBV	155971	316522	73.48%	7.685%
10	6.072	1553	1565	1588	rBV	97718	202215	46.95%	4.910%
11	6.989	1838	1850	1870	rBV	44764	85768	19.91%	2.082%
12	7.317	1939	1952	1973	rBV	205864	359880	83.55%	8.738%
13	7.397	1974	1977	1992	rVB3	3168	4893	1.14%	0.119%
14	7.625	2038	2048	2060	rBV2	27347	47625	11.06%	1.156%
15	7.976	2145	2157	2180	rBV	244233	415453	96.45%	10.087%
16	8.092	2184	2193	2224	rBV2	143454	305781	70.99%	7.424%
17	8.854	2417	2430	2451	rBV	207216	338299	78.54%	8.214%
18	10.217	2837	2854	2868	rBV	60536	95546	22.18%	2.320%
19	11.249	3165	3175	3196	rBV	185276	289284	67.16%	7.024%
20	11.538	3256	3265	3275	rBV6	2513	4495	1.04%	0.109%
21	11.625	3281	3292	3310	rBV	179122	286505	66.52%	6.956%
22	12.130	3441	3449	3456	rVB3	3133	4430	1.03%	0.108%




Sum of corrected areas: 4118725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023457.D
Acq On : 12 Nov 2021 21:37
Operator : SY/MD
Sample : M4616-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

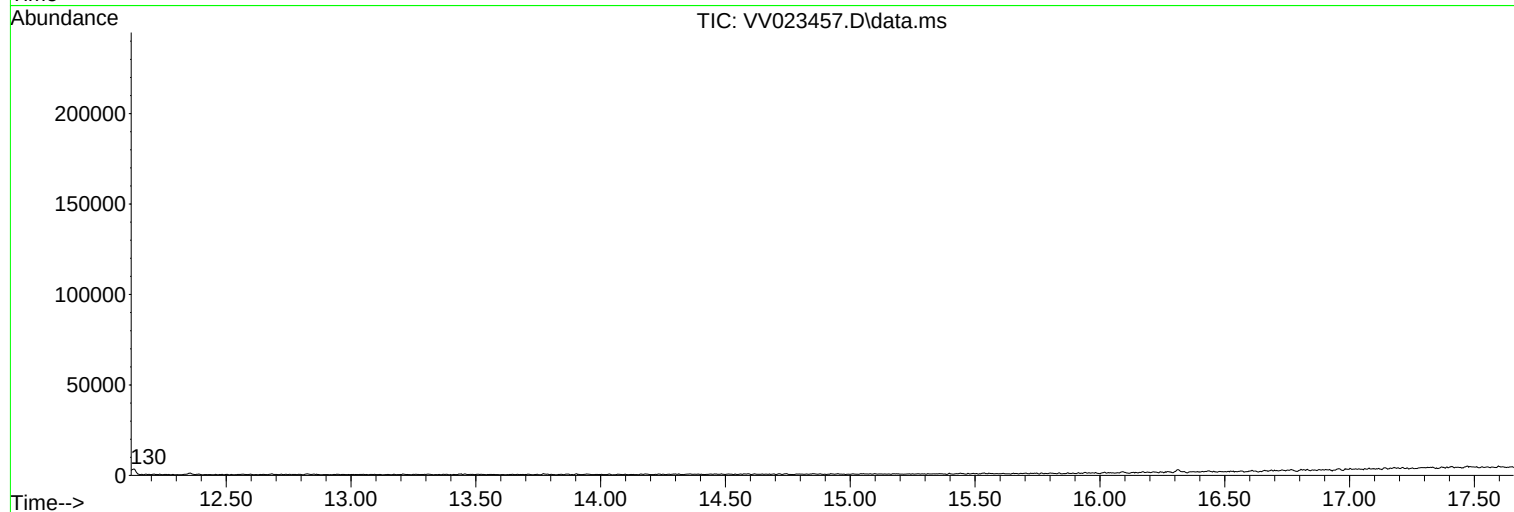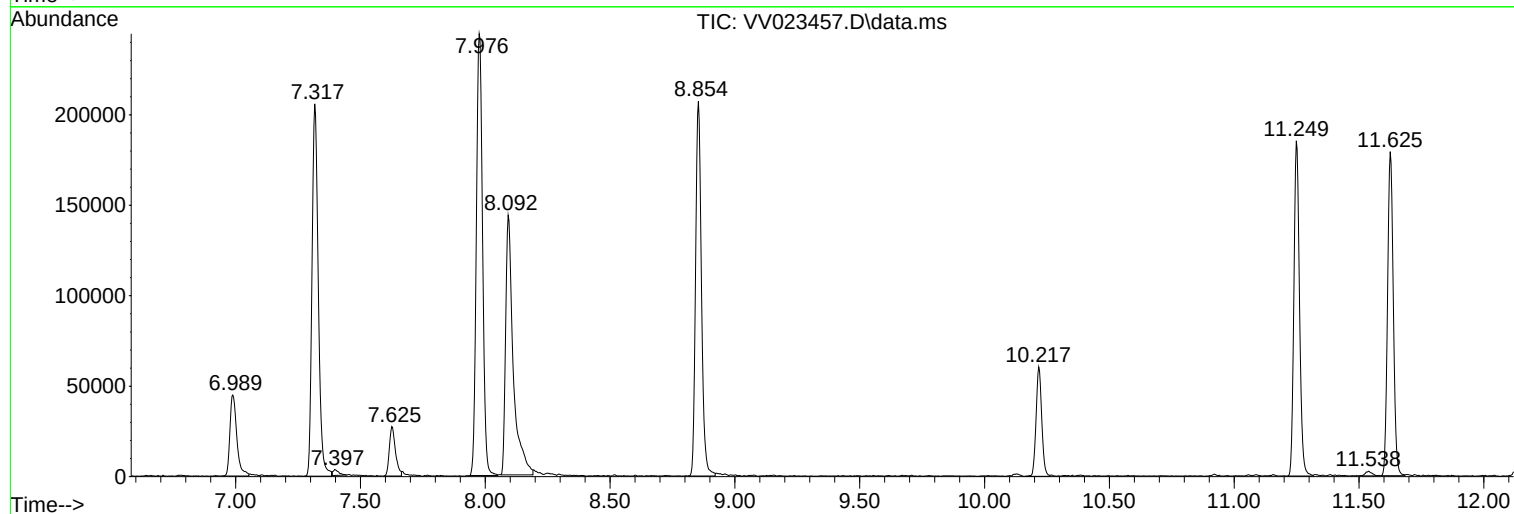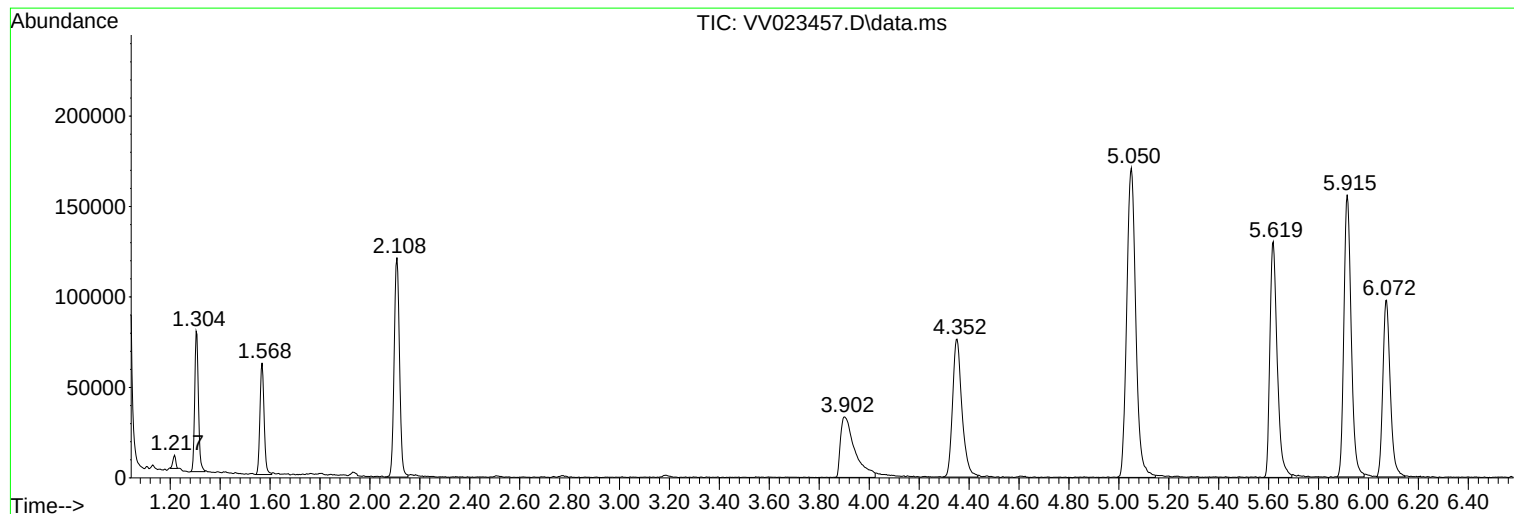

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023457.D
Acq On : 12 Nov 2021 21:37
Operator : SY/MD
Sample : M4616-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023457.D
Acq On : 12 Nov 2021 21:37
Operator : SY/MD
Sample : M4616-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc