

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023458.D
 Acq On : 12 Nov 2021 22:01
 Operator : SY/MD
 Sample : M4616-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXR3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.208	47	52	58	rBV	8077	7180	1.63%	0.214%
2	1.304	74	82	94	rBV	79719	79350	17.98%	2.364%
3	1.568	154	164	177	rBV	61602	71799	16.27%	2.139%
4	2.108	320	332	349	rBV	119268	174707	39.58%	5.206%
5	2.506	447	456	467	rBV	14350	23652	5.36%	0.705%
6	3.905	881	891	916	rBV2	21029	81224	18.40%	2.420%
7	4.349	1013	1029	1052	rBV2	75823	190795	43.22%	5.685%
8	5.050	1229	1247	1279	rBV2	177873	441410	100.00%	13.152%
9	5.619	1412	1424	1442	rBV	129345	260286	58.97%	7.756%
10	5.908	1505	1514	1530	rVB4	6817	13637	3.09%	0.406%
11	6.072	1551	1565	1588	rBV	97644	202464	45.87%	6.033%
12	6.989	1838	1850	1868	rBV2	44451	83775	18.98%	2.496%
13	7.317	1939	1952	1970	rBV	201011	357437	80.98%	10.650%
14	7.397	1971	1977	1988	rVB2	5626	10366	2.35%	0.309%
15	7.625	2039	2048	2066	rBV2	26523	47656	10.80%	1.420%
16	8.095	2181	2194	2233	rBV3	111580	312995	70.91%	9.326%
17	8.853	2418	2430	2453	rBV	204509	334662	75.82%	9.972%
18	9.548	2636	2646	2656	rBV4	4085	6098	1.38%	0.182%
19	10.217	2843	2854	2872	rBV2	54992	87658	19.86%	2.612%
20	11.249	3164	3175	3193	rBV	179894	281649	63.81%	8.392%
21	11.625	3280	3292	3316	rVB	180334	287341	65.10%	8.562%




Sum of corrected areas: 3356141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023458.D
Acq On : 12 Nov 2021 22:01
Operator : SY/MD
Sample : M4616-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

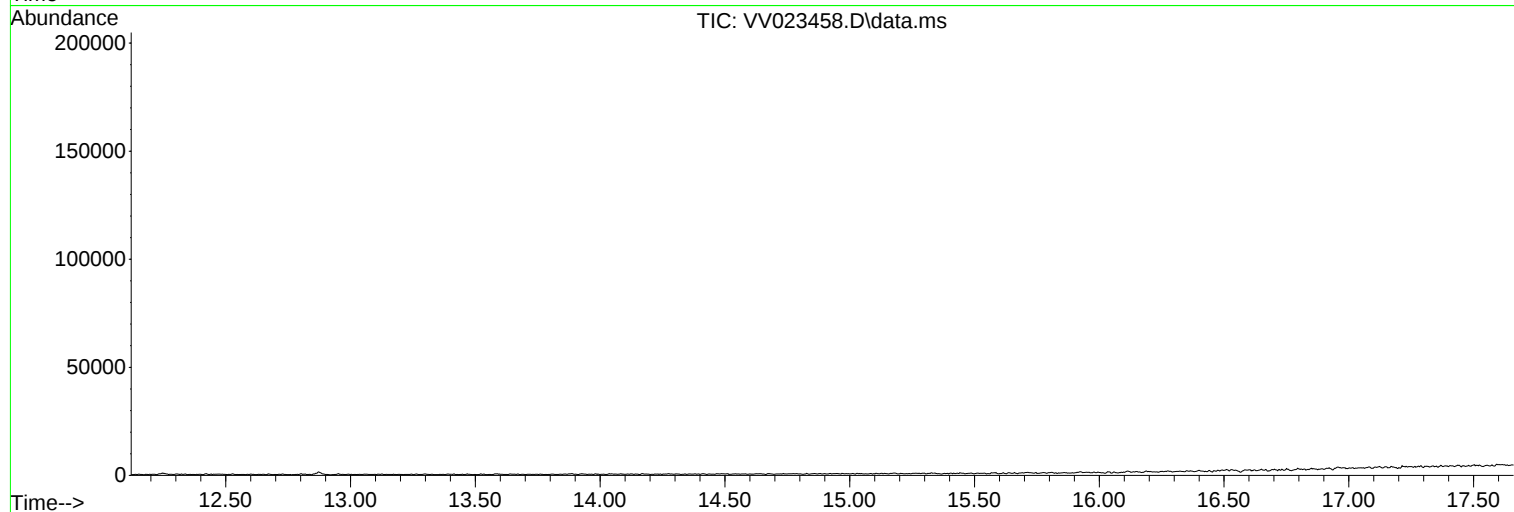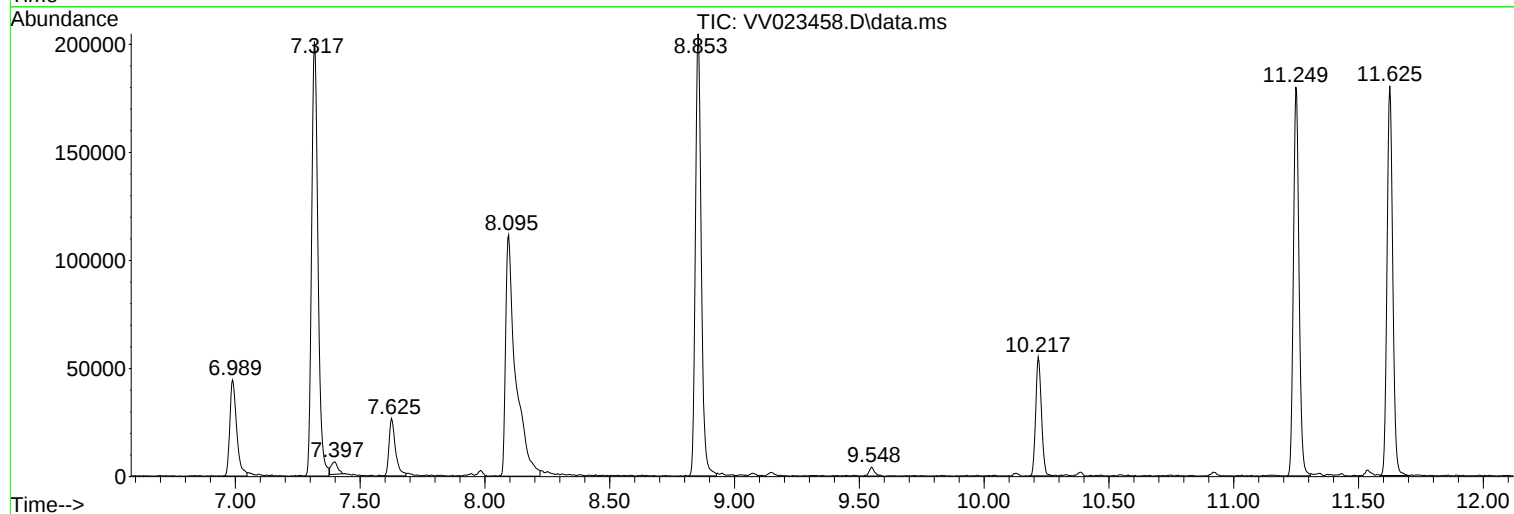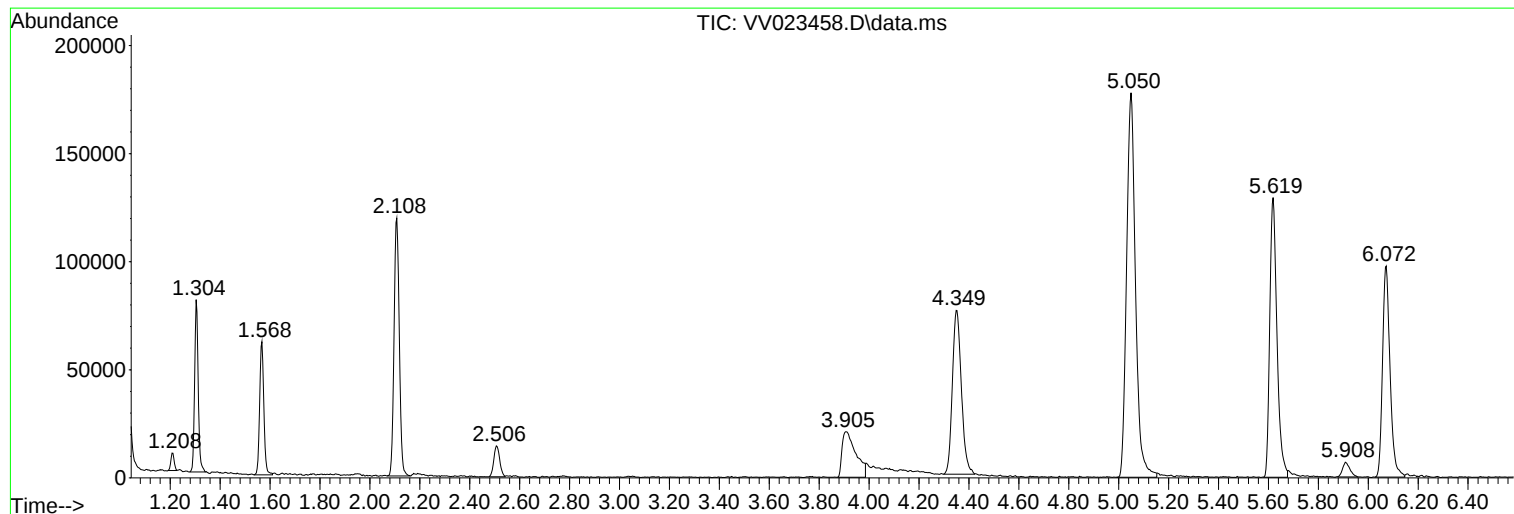

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023458.D
Acq On : 12 Nov 2021 22:01
Operator : SY/MD
Sample : M4616-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023458.D
Acq On : 12 Nov 2021 22:01
Operator : SY/MD
Sample : M4616-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc