

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023461.D
 Acq On : 12 Nov 2021 23:13
 Operator : SY/MD
 Sample : M4616-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1X8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	99	rVB	82935	84841	1.67%	0.765%
2	1.568	156	164	178	rVB	64756	71385	1.40%	0.644%
3	1.751	211	221	240	rBV	1121341	1459102	28.70%	13.160%
4	2.111	317	333	347	rBV3	156541	259451	5.10%	2.340%
5	2.767	524	537	557	rBV3	27147	58010	1.14%	0.523%
6	3.191	652	669	689	rBV	34768	72426	1.42%	0.653%
7	3.912	876	893	926	rBV2	146658	432145	8.50%	3.898%
8	4.352	1014	1030	1063	rBV3	83632	235491	4.63%	2.124%
9	5.050	1231	1247	1273	rBV2	185133	465324	9.15%	4.197%
10	5.619	1411	1424	1448	rBV	133906	273262	5.37%	2.465%
11	5.912	1500	1515	1550	rBV	2681661	5084610	100.00%	45.861%
12	6.069	1552	1564	1591	rVB	106750	225055	4.43%	2.030%
13	6.989	1838	1850	1875	rBV	49058	95069	1.87%	0.857%
14	7.317	1940	1952	1972	rBV	222168	388761	7.65%	3.506%
15	7.625	2039	2048	2063	rBV	30698	53815	1.06%	0.485%
16	7.976	2146	2157	2175	rVB	242003	403691	7.94%	3.641%
17	8.092	2180	2193	2221	rBV2	169202	358290	7.05%	3.232%
18	8.854	2419	2430	2458	rBV	208321	344652	6.78%	3.109%
19	10.217	2843	2854	2873	rBV	68348	107080	2.11%	0.966%
20	11.249	3164	3175	3197	rBV	193808	300370	5.91%	2.709%
21	11.625	3279	3292	3312	rBV	199075	314197	6.18%	2.834%




Sum of corrected areas: 11087027

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023461.D
Acq On : 12 Nov 2021 23:13
Operator : SY/MD
Sample : M4616-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

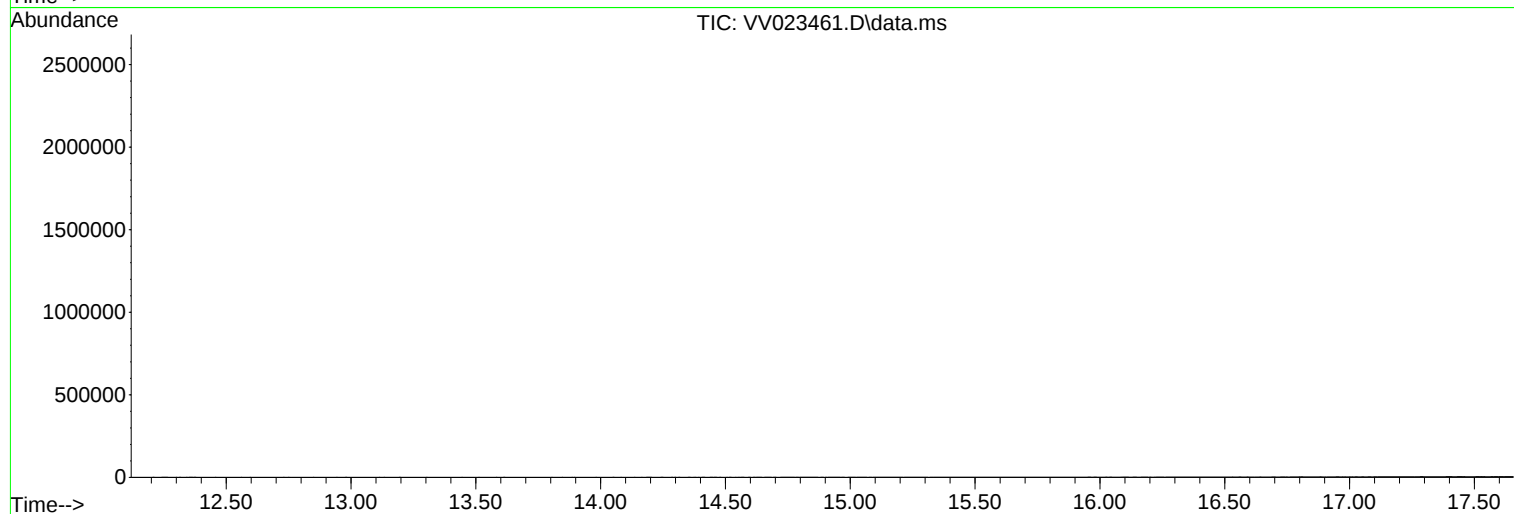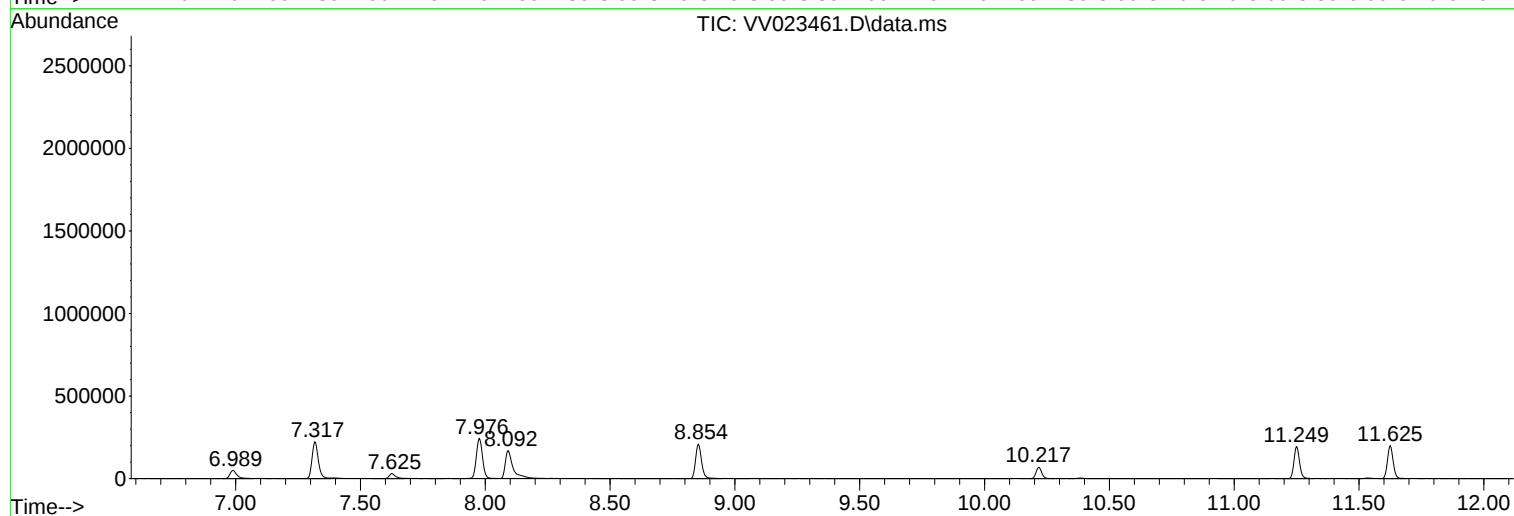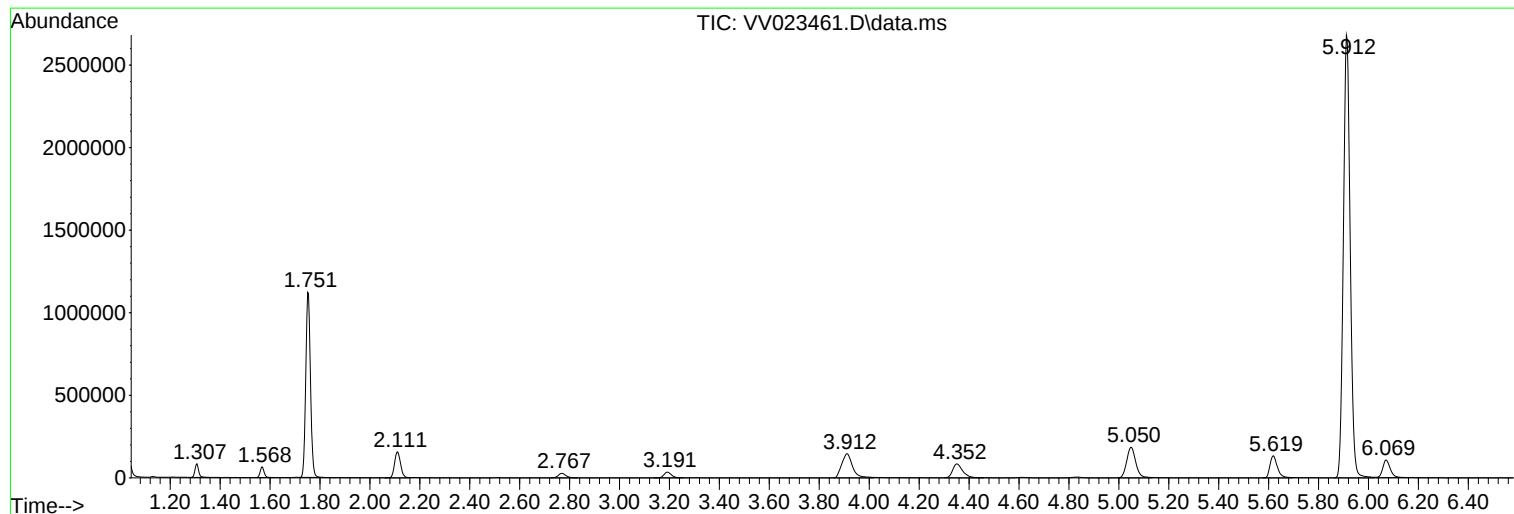

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023461.D
Acq On : 12 Nov 2021 23:13
Operator : SY/MD
Sample : M4616-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023461.D
Acq On : 12 Nov 2021 23:13
Operator : SY/MD
Sample : M4616-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc