

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023464.D
 Acq On : 13 Nov 2021 00:25
 Operator : SY/MD
 Sample : M4616-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1Y1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.133	23	29	39	rVB2	11947	12385	2.75%	0.338%
2	1.307	76	83	95	rVB	78155	79990	17.77%	2.184%
3	1.568	156	164	176	rBV	63195	71182	15.82%	1.943%
4	2.108	321	332	347	rBV	127277	181947	40.43%	4.967%
5	2.770	523	538	557	rBV	44357	94475	20.99%	2.579%
6	3.892	877	887	924	rBV2	40589	141015	31.33%	3.850%
7	4.349	1013	1029	1057	rBV	77956	197610	43.91%	5.395%
8	5.050	1231	1247	1272	rBV2	178478	450049	100.00%	12.286%
9	5.619	1412	1424	1447	rBV	130927	268996	59.77%	7.343%
10	5.921	1505	1518	1532	rBV7	12996	29081	6.46%	0.794%
11	6.069	1550	1564	1590	rBV2	100726	210910	46.86%	5.758%
12	6.989	1838	1850	1865	rBV	47282	84919	18.87%	2.318%
13	7.317	1941	1952	1970	rBV	211280	367683	81.70%	10.038%
14	7.625	2039	2048	2062	rBV2	27592	49320	10.96%	1.346%
15	7.979	2150	2158	2173	rVB3	10927	18917	4.20%	0.516%
16	8.091	2181	2193	2224	rBV2	165438	350984	77.99%	9.582%
17	8.853	2419	2430	2452	rBV	207476	343370	76.30%	9.374%
18	10.217	2843	2854	2873	rBV	66356	105473	23.44%	2.879%
19	11.249	3164	3175	3195	rBV	190518	293528	65.22%	8.013%
20	11.538	3254	3265	3277	rBV6	3331	6615	1.47%	0.181%
21	11.625	3281	3292	3313	rVV	193803	304611	67.68%	8.316%




Sum of corrected areas: 3663060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023464.D
Acq On : 13 Nov 2021 00:25
Operator : SY/MD
Sample : M4616-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

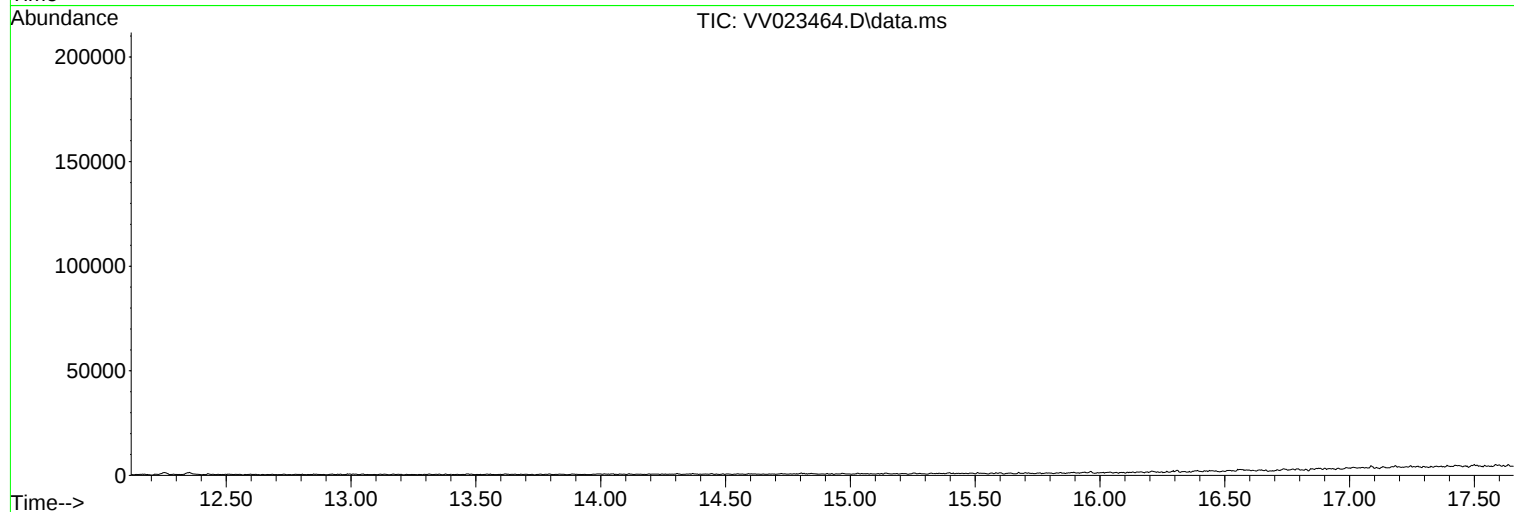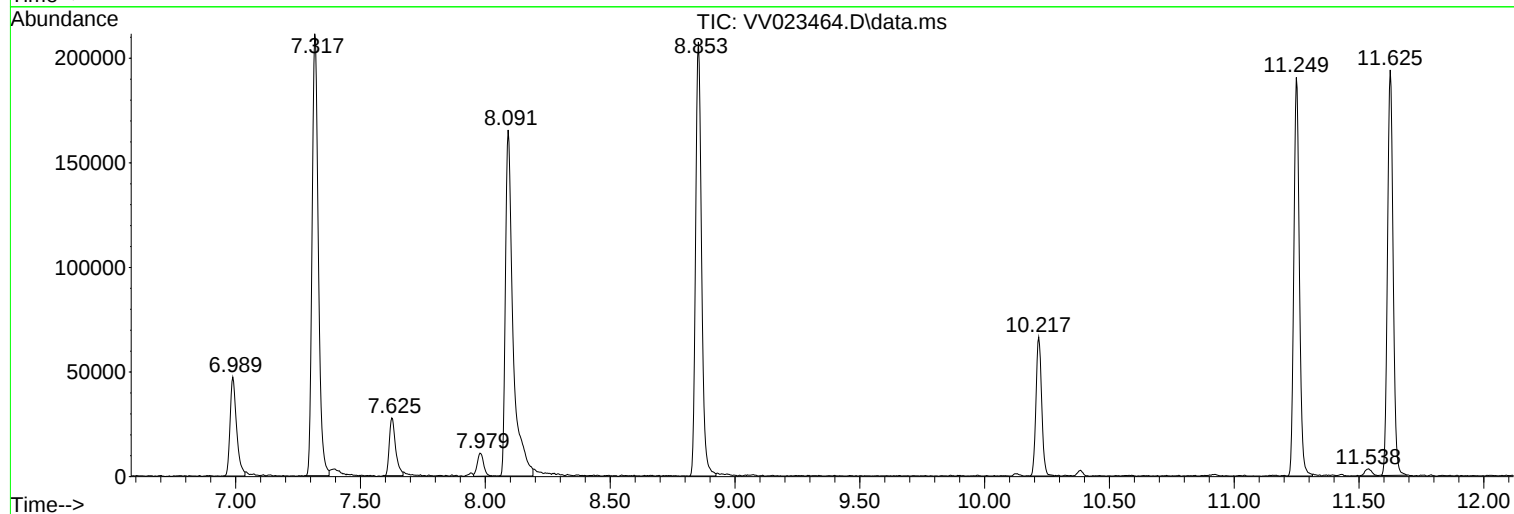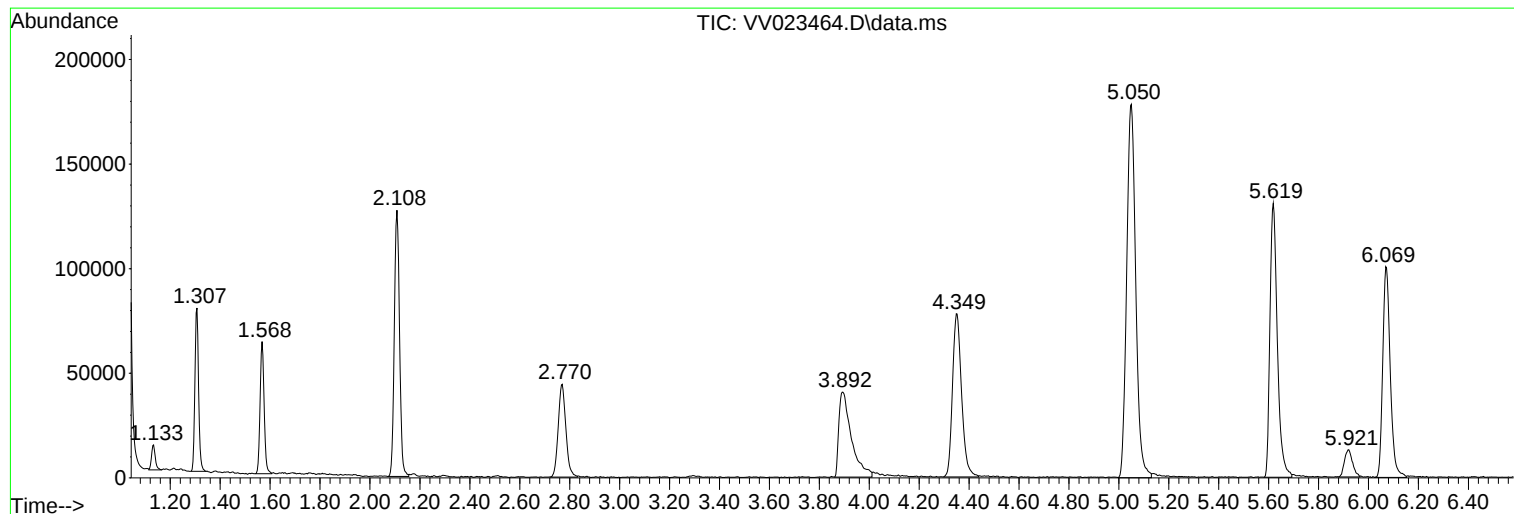

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023464.D
Acq On : 13 Nov 2021 00:25
Operator : SY/MD
Sample : M4616-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023464.D
Acq On : 13 Nov 2021 00:25
Operator : SY/MD
Sample : M4616-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
