

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023467.D
 Acq On : 13 Nov 2021 01:37
 Operator : SY/MD
 Sample : M4581-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	97	rVB	50952	53794	14.13%	1.724%
2	1.568	156	164	175	rBV	49039	53995	14.18%	1.730%
3	2.108	322	332	343	rBV	92418	130866	34.36%	4.194%
4	2.510	449	457	468	rBV3	5377	8643	2.27%	0.277%
5	3.892	875	887	917	rBV	37040	121957	32.03%	3.908%
6	4.352	1014	1030	1054	rBV2	68266	174124	45.72%	5.580%
7	5.050	1231	1247	1274	rBV3	152097	380813	100.00%	12.204%
8	5.619	1407	1424	1446	rBV	134845	276739	72.67%	8.869%
9	5.912	1502	1515	1527	rBV7	4887	10265	2.70%	0.329%
10	6.072	1552	1565	1584	rBV2	90362	183986	48.31%	5.896%
11	6.989	1840	1850	1869	rBV2	38403	72117	18.94%	2.311%
12	7.317	1940	1952	1972	rBV	172107	306218	80.41%	9.814%
13	7.625	2039	2048	2074	rBV3	22374	41617	10.93%	1.334%
14	8.092	2183	2193	2227	rBV2	138440	300758	78.98%	9.639%
15	8.854	2419	2430	2451	rBV	214493	346595	91.01%	11.108%
16	10.217	2843	2854	2868	rBV	56269	87007	22.85%	2.788%
17	10.384	2896	2906	2915	rBV3	3468	5363	1.41%	0.172%
18	11.249	3164	3175	3195	rBV	195117	300096	78.80%	9.617%
19	11.625	3281	3292	3309	rBV	165934	261525	68.68%	8.381%
20	12.252	3477	3487	3495	rVB2	2726	3850	1.01%	0.123%




Sum of corrected areas: 3120328

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023467.D
Acq On : 13 Nov 2021 01:37
Operator : SY/MD
Sample : M4581-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

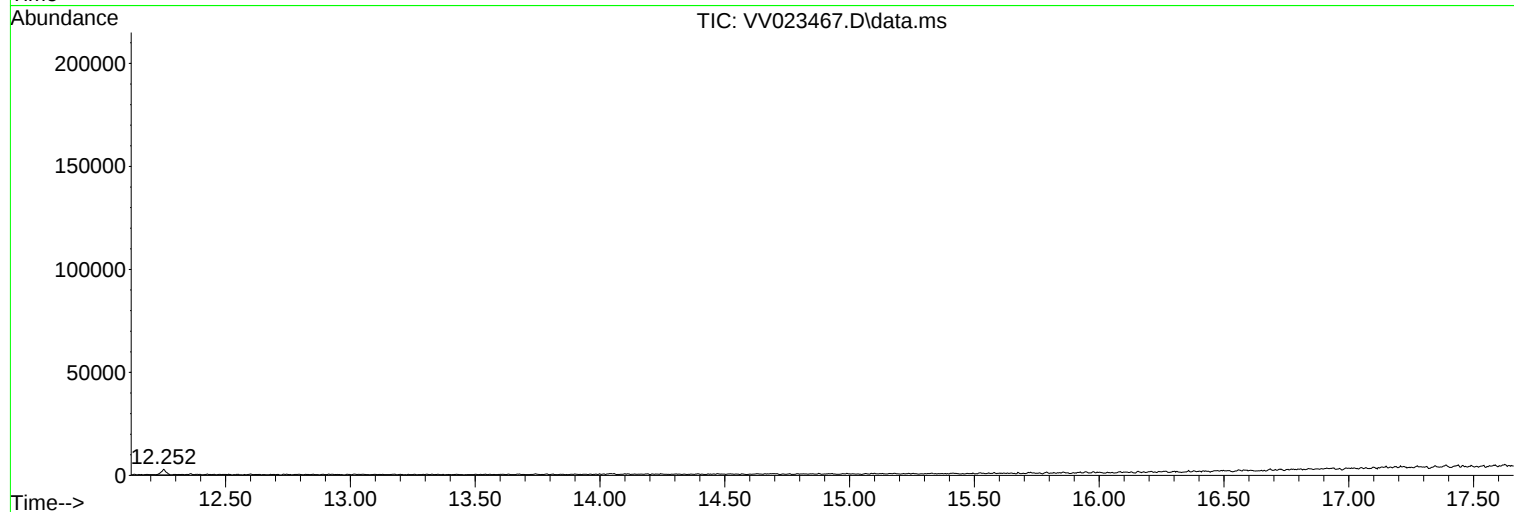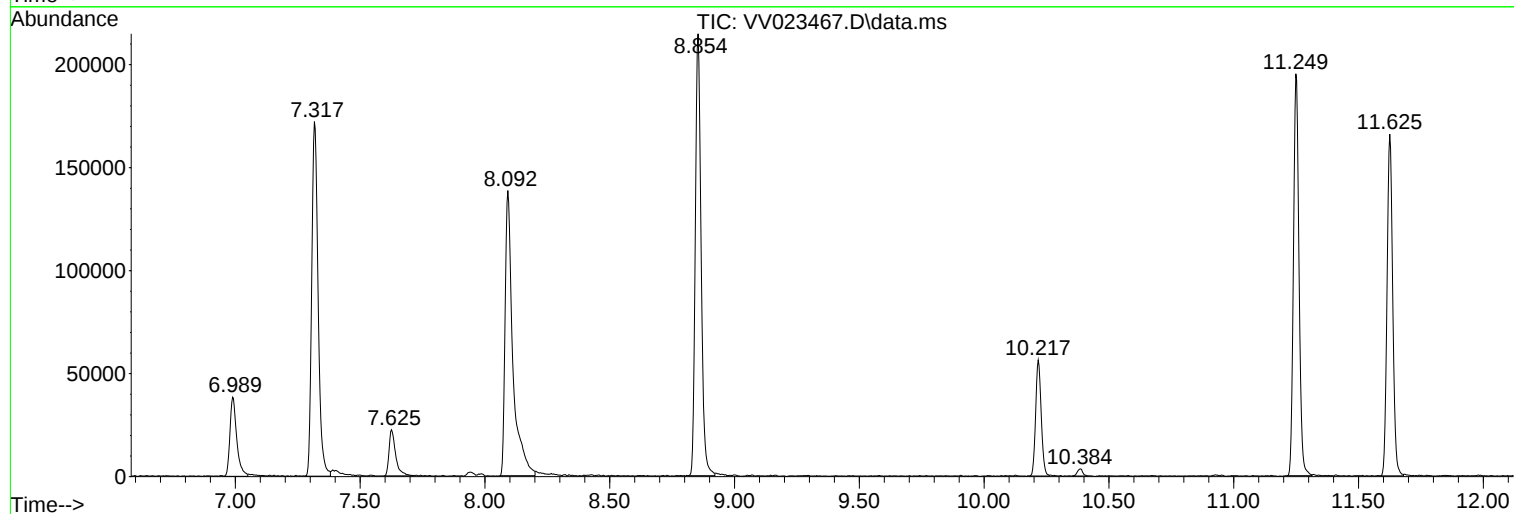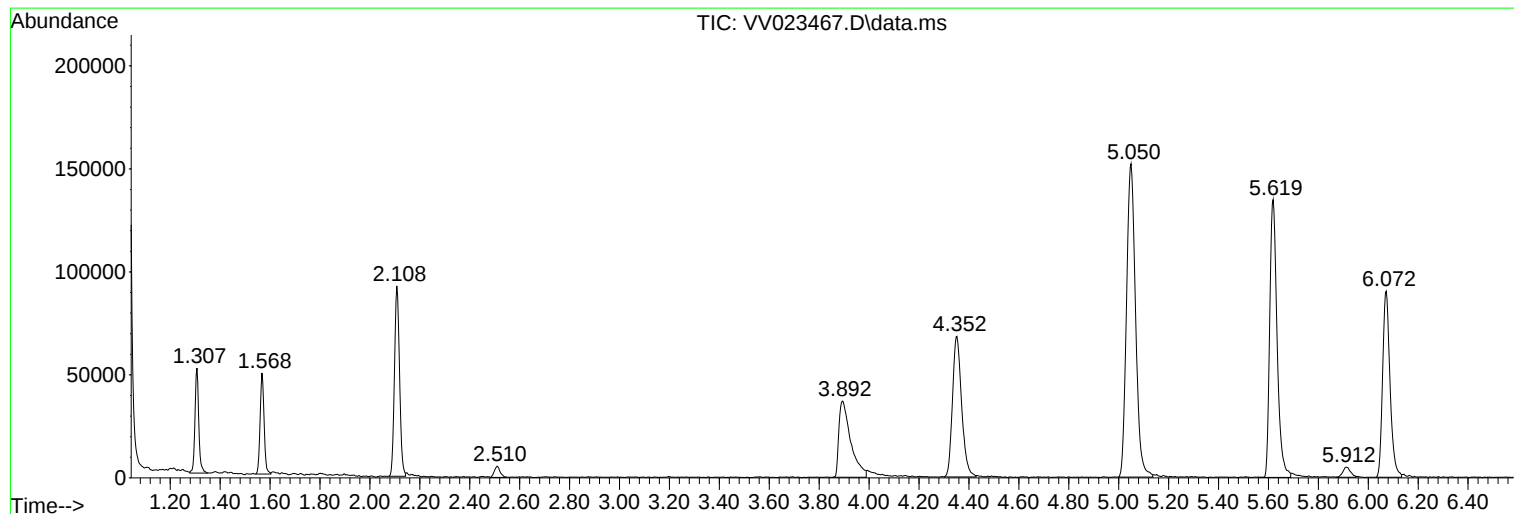

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023467.D
Acq On : 13 Nov 2021 01:37
Operator : SY/MD
Sample : M4581-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
Data File : VV023467.D
Acq On : 13 Nov 2021 01:37
Operator : SY/MD
Sample : M4581-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
